

PARTICIPANT FINAL ASSESSMENT REPORT (SUMMARY)

PT SCHEME: BIOCHEMISTRY

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

All Methods

	Parameters	Labs (n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
1	CHOLESTEROL	32	156.90	mg/dL	188.31	10.15	2.278	3.10	Unsatisfactory
2	TRIGLYCERIDES	28	453.30	mg/dL	556.63	24.08	6.567	4.29	Unsatisfactory
3	CREATININE	33	8.04	mg/dL	11.07	0.86	0.186	3.53	Unsatisfactory
4	HDL-CHOL	26	29.28	mg/dL	140.80	24.63	6.565	4.53	Unsatisfactory
5	URIC ACID	31	13.49	mg/dL	10.98	0.46	0.109	5.45	Unsatisfactory
6	ALT	33	19.45	U/L	31.02	4.79	1.131	2.42	Questionable
7	BILIRUBIN	33	6.86	mg/dL	9.82	1.28	0.291	2.32	Questionable
8	TOTAL PROTEIN	32	5.00	g/dL	5.48	0.44	0.100	1.09	Satisfactory
9	ALBUMIN	32	3.61	g/dL	4.96	0.90	0.209	1.49	Satisfactory
10	GLUCOSE	33	609.80	mg/dL	572.85	50.07	14.751	0.74	Good
11	UREA	33	118.60	mg/dL	125.42	8.95	1.948	0.76	Good
12	AST	33	24.75	U/L	27.72	4.76	1.125	0.62	Good
13	CALCIUM	28	5.16	mg/dL	5.39	0.24	0.056	0.96	Good
14	Alkaline Phosphatase	33	355.20	U/L	337.94	31.78	7.507	0.54	Good
15	Direct Bilirubin	30	2.49	mg/dL	2.84	0.65	0.148	0.54	Good
16	SODIUM	27	Not Recvd.	mmol/L	119.29	10.69	2.850		N/A
17	POTASSIUM	27	Not Recvd.	mmol/L	4.49	0.92	0.236		N/A
18	CHLORIDE	27	Not Recvd.	mmol/L	93.74	6.29	1.758		N/A

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 1 of 22

PARTICIPANT FINAL ASSESSMENT REPORT (SUMMARY)

PT SCHEME: BIOCHEMISTRY

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

Peer group

	Parameters	Labs (n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
19	GGTP (IFCC)	10	144.50	U/L	203.50	10.19		5.79	Unsatisfactory
20	CHOLESTEROL (CHOD-PAP)	13	156.90	mg/dL	183.50	10.33		2.58	Questionable
21	BILIRUBIN (Diazotized Sulphanilic Ac)	14	6.86	mg/dL	9.00	0.87		2.46	Questionable
22	ALBUMIN (BCG)	23	3.61	g/dL	5.15	0.97	0.271	1.59	Satisfactory
23	GLUCOSE (GOD-POD)	7	609.80	mg/dL	598.40	45.58		0.25	Good
24	UREA (Urease/GLDH coupled reac)	5	118.60	mg/dL	124.90	8.48		0.74	Good
25	AST (Modified IFCC)	2	24.75	U/L	26.68	2.72		0.71	Good
26	TOTAL PROTEIN (Biuret)	22	5.00	g/dL	5.38	0.41	0.112	0.94	Good
27	CALCIUM (Arsenazo III)	3	5.16	mg/dL	5.12	0.06		0.67	Good
28	Alkaline Phosphatase (Modified IFCC)	10	355.20	U/L	355.20	22.77			Good
29	Direct Bilirubin (Diazotised Sulphanilic)	8	2.49	mg/dL	2.60	0.48		0.22	Good
30	TRIGLYCERIDES (GPO-Trinder)	3	453.30	mg/dL					N/A
31	CREATININE (Modified Jaffe's)	1	8.04	mg/dL					N/A
32	ALT (Modified IFCC)	2	19.45	U/L					N/A
33	HDL-CHOL (PEG modified enzymatic)	1	29.28	mg/dL					N/A

Authorised Signatory

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor




Dr. Sujay Prasad
Technical Manager and Program coordinator

This report is for use only by the intended participant.

Dr Venkatesh

Page 2 of 22



PARTICIPANT FINAL ASSESSMENT REPORT (SUMMARY)

PT SCHEME: BIOCHEMISTRY

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

Peer group

	Parameters	Labs (n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
34	URIC ACID (Trinder Peroxidase)	1	13.49	mg/dL					N/A

Interpretation of z scores is as follows:

- | Z score | ≤ 1.0 – Good
- | Z score | between 1.0 to 2.0 - Satisfactory
- | Z score | between 2.0 to 3.0 - Questionable
- | Z score | ≥ 3.0 - Unsatisfactory

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

Page 3 of 22

This report is for use only by the intended participant.



Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

ALBUMIN


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (BCG)	23	3.61	g/dL	5.15	0.97	0.271	1.59	Satisfactory

ZScore




All Methods	32	3.61	g/dL	4.96	0.90	0.209	1.49	Satisfactory
-------------	----	------	------	------	------	-------	------	--------------

ZScore



Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 4 of 22

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4


Report Date : 12/08/2022

Sample : JUL 2022

Alkaline Phosphatase


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (Modified IFCC)	10	355.20	U/L	355.20	22.77			Good

ZScore

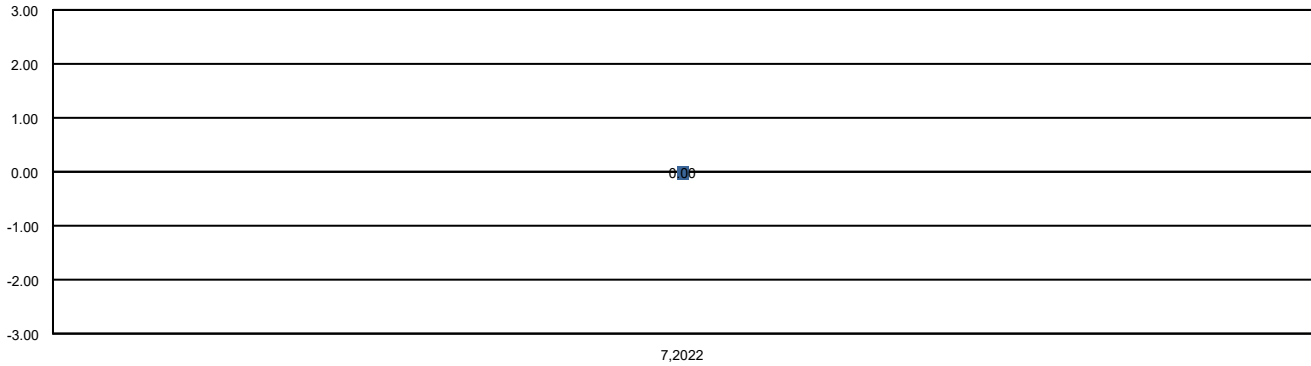

All Methods	33	355.20	U/L	337.94	31.78	7.507	0.54	Good
-------------	----	--------	-----	--------	-------	-------	------	------

ZScore



Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 5 of 22

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

ALT


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	33	19.45	U/L	31.02	4.79	1.131	2.42	Questionable

ZScore



Peer group (Modified IFCC)	2	19.45	U/L					N/A
----------------------------	---	--------------	-----	--	--	--	--	-----

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 6 of 22



Neu-QAP

(an EXTERNAL QUALITY ASSURANCE PROGRAMME)

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY



PC-1047

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

AST

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	33	24.75	U/L	27.72	4.76	1.125	0.62	Good

ZScore



Peer group (Modified IFCC)	2	24.75	U/L	26.68	2.72		0.71	Good
----------------------------	---	-------	-----	-------	------	--	------	------

Authorised Signatory

Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor

Dr Venkatesh

Page 7 of 22

This report is for use only by the intended participant.



An external quality assurance program from
NEUBERG ANAND ACADEMY OF LABORATORY MEDICINE PVT.LTD.

Anand Tower, 54, Bowring Hospital Road,
Shivajinagar, Bangalore - 560001
+91-9902277355 · qap@naalm.com · www.naalm.com
CIN: U85300KA2018PTC115147

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4


Report Date : 12/08/2022

Sample : JUL 2022

BILIRUBIN


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (Diazotized Sulphanilic Ac)	14	6.86	mg/dL	9.00	0.87		2.46	Questionable

ZScore

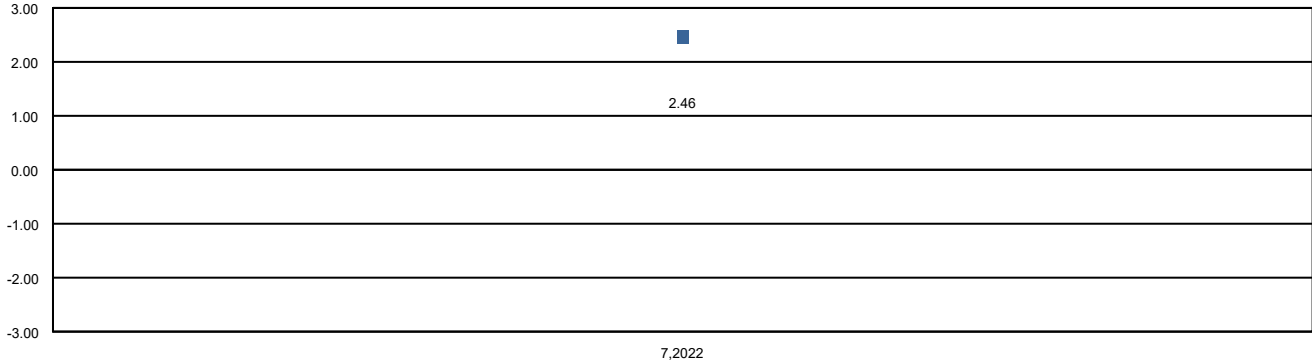

All Methods	33	6.86	mg/dL	9.82	1.28	0.291	2.32	Questionable
-------------	----	-------------	-------	------	------	-------	------	--------------

ZScore

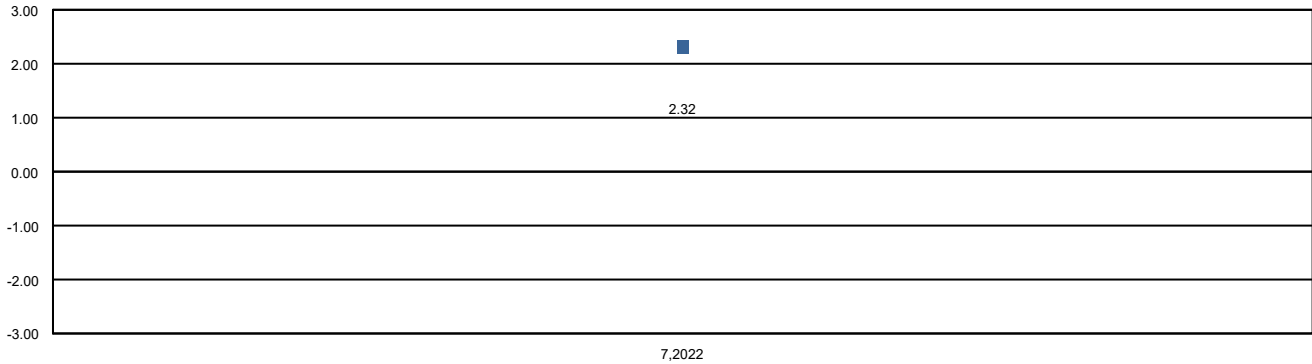

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 8 of 22

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022


Sample : JUL 2022

CALCIUM


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (Arsenazo III)	3	5.16	mg/dL	5.12	0.06		0.67	Good

All Methods	28	5.16	mg/dL	5.39	0.24	0.056	0.96	Good
-------------	----	------	-------	------	------	-------	------	------

ZScore



Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh
Page 9 of 22

This report is for use only by the intended participant.





Neu-QAP

(an EXTERNAL QUALITY ASSURANCE PROGRAMME)

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY



PC-1047

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

CHLORIDE

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	27	Not Recvd.	mmol/L	93.74	6.29	1.758		N/A

Authorised Signatory

Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor

Dr Venkatesh

Page 10 of 22

This report is for use only by the intended participant.



An external quality assurance program from
NEUBERG ANAND ACADEMY OF LABORATORY MEDICINE PVT.LTD.

Anand Tower, 54, Bowring Hospital Road,
Shivajinagar, Bangalore - 560001
+91-9902277355 · qap@naalm.com · www.naalm.com
CIN: U85300KA2018PTC115147

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY


Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022


Sample : JUL 2022

CHOLESTEROL

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	32	156.90	mg/dL	188.31	10.15	2.278	3.10	Unsatisfactory



Peer group (CHOD-PAP)	13	156.90	mg/dL	183.50	10.33		2.58	Questionable
-----------------------	----	---------------	-------	--------	-------	--	------	--------------

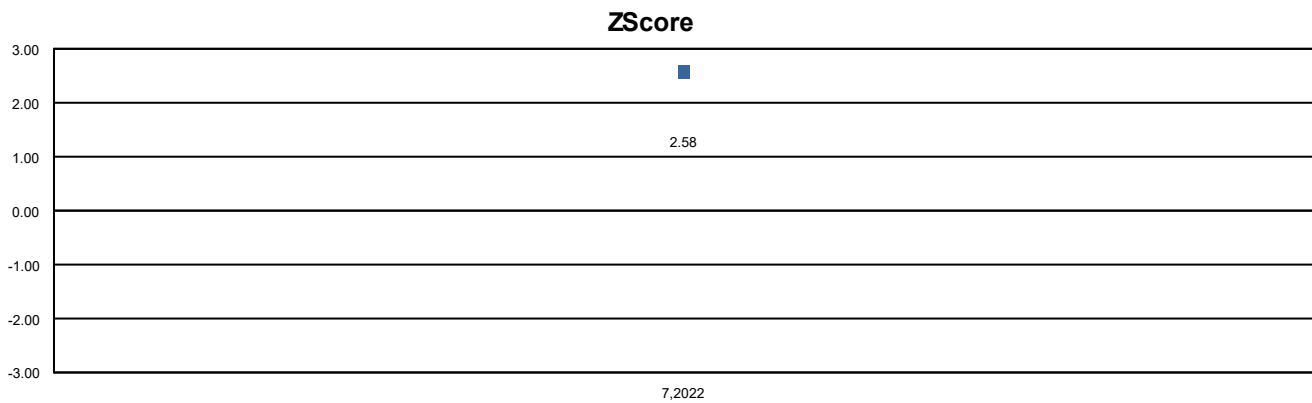

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 11 of 22


Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022


CREATININE

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	33	8.04	mg/dL	11.07	0.86	0.186	3.53	Unsatisfactory



Peer group (Modified Jaffe's)	1	8.04	mg/dL					N/A
----------------------------------	---	-------------	-------	--	--	--	--	-----

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh
Page 12 of 22

This report is for use only by the intended participant.



Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4


Report Date : 12/08/2022

Sample : JUL 2022

Direct Bilirubin


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (Diazotised Sulphanilic)	8	2.49	mg/dL	2.60	0.48		0.22	Good

ZScore




All Methods	30	2.49	mg/dL	2.84	0.65	0.148	0.54	Good
-------------	----	------	-------	------	------	-------	------	------

ZScore



Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 13 of 22



Neu-QAP

(an EXTERNAL QUALITY ASSURANCE PROGRAMME)

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY



PC-1047


Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

GGTP

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (IFCC)	10	144.50	U/L	203.50	10.19		5.79	Unsatisfactory

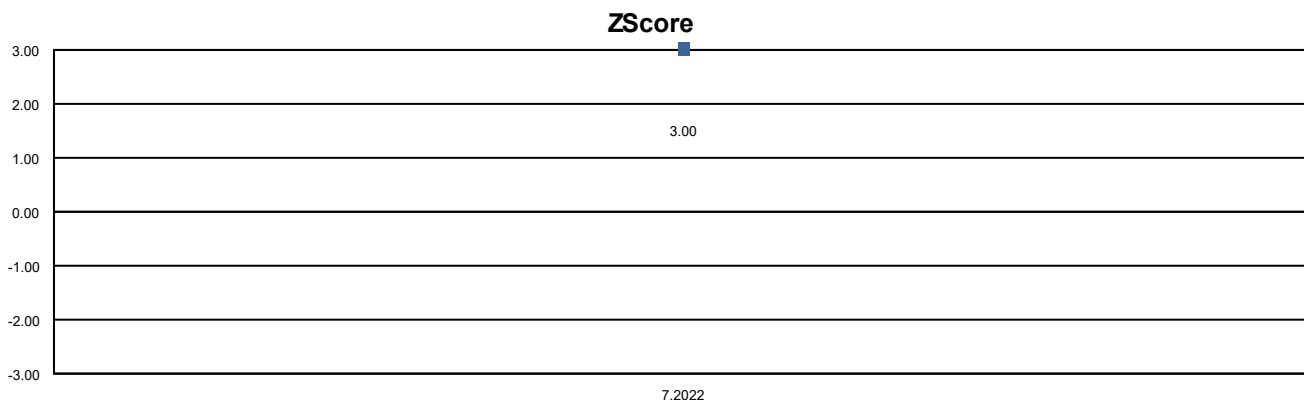

Authorised Signatory

Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor

Dr Venkatesh
Page 14 of 22

This report is for use only by the intended participant.



An external quality assurance program from
NEUBERG ANAND ACADEMY OF LABORATORY MEDICINE PVT.LTD.

Anand Tower, 54, Bowring Hospital Road,
Shivajinagar, Bangalore - 560001
+91-9902277355 · qap@naalm.com · www.naalm.com
CIN: U85300KA2018PTC115147

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4


Report Date : 12/08/2022

Sample : JUL 2022

GLUCOSE


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	33	609.80	mg/dL	572.85	50.07	14.751	0.74	Good

ZScore



Peer group (GOD-POD)	7	609.80	mg/dL	598.40	45.58		0.25	Good
----------------------	---	---------------	-------	--------	-------	--	------	------

ZScore



Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 15 of 22

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022


Sample : JUL 2022

HDL-CHOL


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (PEG modified enzymatic)	1	29.28	mg/dL					N/A

All Methods	26	29.28	mg/dL	140.80	24.63	6.565	4.53	Unsatisfactory
-------------	----	-------	-------	--------	-------	-------	------	----------------

ZScore



Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh
Page 16 of 22

This report is for use only by the intended participant.





Neu-QAP

(an EXTERNAL QUALITY ASSURANCE PROGRAMME)

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY



PC-1047

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

POTASSIUM

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	27	Not Recvd.	mmol/L	4.49	0.92	0.236		N/A

Authorised Signatory

Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor

Dr Venkatesh

Page 17 of 22

This report is for use only by the intended participant.



An external quality assurance program from
NEUBERG ANAND ACADEMY OF LABORATORY MEDICINE PVT.LTD.

Anand Tower, 54, Bowring Hospital Road,
Shivajinagar, Bangalore - 560001
+91-9902277355 · qap@naalm.com · www.naalm.com
CIN: U85300KA2018PTC115147



Neu-QAP

(an EXTERNAL QUALITY ASSURANCE PROGRAMME)

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY



PC-1047

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

SODIUM

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	27	Not Recvd.	mmol/L	119.29	10.69	2.850		N/A

Authorised Signatory

Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor

Dr Venkatesh

Page 18 of 22

This report is for use only by the intended participant.



An external quality assurance program from
NEUBERG ANAND ACADEMY OF LABORATORY MEDICINE PVT.LTD.

Anand Tower, 54, Bowring Hospital Road,
Shivajinagar, Bangalore - 560001
+91-9902277355 · qap@naalm.com · www.naalm.com
CIN: U85300KA2018PTC115147

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4


Report Date : 12/08/2022

Sample : JUL 2022

TOTAL PROTEIN


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (Biuret)	22	5.00	g/dL	5.38	0.41	0.112	0.94	Good

ZScore




All Methods	32	5.00	g/dL	5.48	0.44	0.100	1.09	Satisfactory
-------------	----	------	------	------	------	-------	------	--------------

ZScore



Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh
Page 19 of 22

This report is for use only by the intended participant.





Neu-QAP

(an EXTERNAL QUALITY ASSURANCE PROGRAMME)

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY



PC-1047


Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

TRIGLYCERIDES

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	28	453.30	mg/dL	556.63	24.08	6.567	4.29	Unsatisfactory

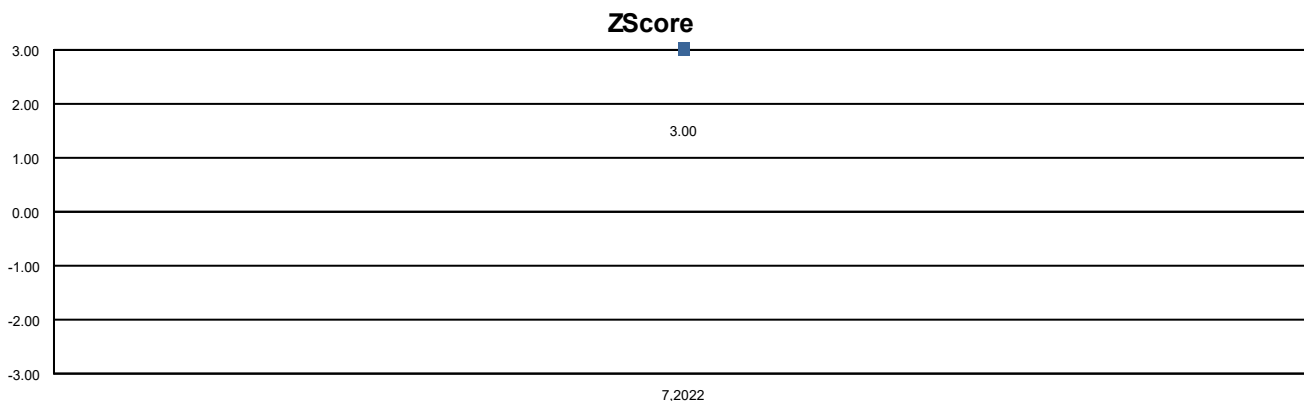

Peer group (GPO-Trinder)	3	453.30	mg/dL					N/A
--------------------------	---	--------	-------	--	--	--	--	-----

Authorised Signatory

Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor

Dr Venkatesh

Page 20 of 22

This report is for use only by the intended participant.



An external quality assurance program from
NEUBERG ANAND ACADEMY OF LABORATORY MEDICINE PVT.LTD.

Anand Tower, 54, Bowring Hospital Road,
Shivajinagar, Bangalore - 560001
+91-9902277355 · qap@naalm.com · www.naalm.com
CIN: U85300KA2018PTC115147

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4


Report Date : 12/08/2022

Sample : JUL 2022

UREA


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	33	118.60	mg/dL	125.42	8.95	1.948	0.76	Good

ZScore




Peer group (Urease/GLDH coupled reac)	5	118.60	mg/dL	124.90	8.48		0.74	Good
---	---	---------------	-------	--------	------	--	------	------

ZScore



Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 21 of 22



Neu-QAP

(an EXTERNAL QUALITY ASSURANCE PROGRAMME)

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY



PC-1047

Cycle No	C4
Ref.No.	NEUQAP549
Sample ID	NEUQAP BIO SERUM/2022/7/C4/S4

Report Date : 12/08/2022

Sample : JUL 2022

URIC ACID

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (Trinder Peroxidase)	1	13.49	mg/dL					N/A

All Methods	31	13.49	mg/dL	10.98	0.46	0.109	5.45	Unsatisfactory
-------------	----	-------	-------	-------	------	-------	------	----------------

ZScore



Note: Sample generation, homogeneity and stability testing activities are subcontracted to ISO 15189:2012 accredited laboratory . Lyophilisation of samples is subcontracted to ISO 9001:2015 manufacturing facility .

**End of report **

Authorised Signatory

Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor

Dr Venkatesh

Please refer to NEUQAP Web portal for all subcontracted activ
This report is for use only by the intended participant.



An external quality assurance program from
NEUBERG ANAND ACADEMY OF LABORATORY MEDICINE PVT.LTD.

Anand Tower, 54, Bowring Hospital Road,
Shivajinagar, Bangalore - 560001
+91-9902277355 · qap@naalm.com · www.naalm.com
CIN: U85300KA2018PTC115147