



October 29, 2021

*Calibration Certificate for Fully Automated Analyzer
Model: XL640 (Sr. No.: 640353)*


This is to certify that the Fully Automated Analyzer, Model: XL640 (Sr. No.: 640353) installed at REDCLIFFE LIFETECH PVT Ltd, Plotno: 144/C, Ground floor, Chandrasekharpur, Bhubaneswar, Odisha-751016 has been calibrated and the calibration value of all filters gains and all the required values are well within limit.

This calibration is valid till October 28, 2022

For, Transasia Bio-Medicals Ltd.

Shibananda Biswas

Dy. Regional Service Manager

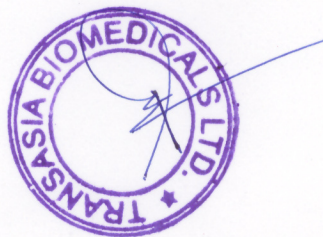

Result Reprint

Report Type : Controls 27-Aug-2022

Consumable: BIORAD L1

Sl #	Lot #	Consumable	Test	Result Unit	Flag	Curve #	Result Date	Mean	SD	Interval (3SD)
1	26491	BIORAD L1	Na	145.50 mmol/l		0	27-Aug-2022 09:35:12	146.747	3.440	136.427 - 157.067
2	26491	BIORAD L1	K	3.60 mmol/l	F,+1SD	0	27-Aug-2022 09:35:12	3.494	0.060	3.314 - 3.674
3	26491	BIORAD L1	Cl	102.20 mmol/l		0	27-Aug-2022 09:35:12	101.837	1.720	96.677 - 106.997
4	26491	BIORAD L1	SGPTD	26.6 U/L	-1SD	183039	27-Aug-2022 09:37:58	27.770	0.950	24.92 - 30.62
5	26491	BIORAD L1	ALPU	111 U/L		183043	27-Aug-2022 09:38:34	107.750	7.210	86.12 - 129.38
6	26491	BIORAD L1	GGT	64.7 U/L		183045	27-Aug-2022 09:38:52	66.300	6.600	46.5 - 86.1
7	26491	BIORAD L1	PHOS	4.03 mg/dl	+1SD	183047	27-Aug-2022 09:39:10	3.791	0.190	3.221 - 4.361
8	26491	BIORAD L1	BID	0.40 mg/dl		183049	27-Aug-2022 09:39:28	0.396	0.020	0.336 - 0.456
9	26491	BIORAD L1	BIT	0.94 mg/dl		183051	27-Aug-2022 09:39:46	0.958	0.080	0.718 - 1.198
10	26491	BIORAD L1	CRENZ	1.72 mg/dl		183055	27-Aug-2022 09:40:22	1.707	0.040	1.587 - 1.827
11	26491	BIORAD L1	GLU	86.1 mg/dl	+1SD	183057	27-Aug-2022 09:40:40	82.853	2.520	75.293 - 90.413
12	26491	BIORAD L1	CHOL	265 mg/dl	+1SD	183061	27-Aug-2022 09:41:16	252.400	7.210	230.77 - 274.03
13	26491	BIORAD L1	UA	5.2 mg/dl		183065	27-Aug-2022 09:41:52	5.194	0.210	4.564 - 5.824
14	26491	BIORAD L1	CA	9.5 mg/dl		183073	27-Aug-2022 09:43:04	9.217	0.370	8.107 - 10.327
15	26491	BIORAD L1	ALB	4.08 g/dl	+1SD	183075	27-Aug-2022 09:43:22	3.965	0.100	3.665 - 4.265
16	26491	BIORAD L1	PRO	6.82 g/dl	+1SD	183077	27-Aug-2022 09:43:41	6.469	0.310	5.539 - 7.399
17	26491	BIORAD L1	SGOTD	35.6 U/L		183087	27-Aug-2022 10:21:47	36.210	1.040	33.09 - 39.33

Print Date 27-Aug-2022



Result Reprint

Report Type : Controls 27-Aug-2022

Consumable: BIORAD L1

Sr #	Lot #	Consumable	Test	Result Unit	Flag	Curve #	Result Date	Mean	SD	Interval (3SD)
18	26491	BIORAD L1	UREA	34.4 mg/dl	+1SD	183094	27-Aug-2022 10:22:50	32.681	1.380	28.541 - 36.821
19	26491	BIORAD L1	TRIG	168.1 mg/dl	-1SD	183101	27-Aug-2022 10:23:53	179.873	7.120	158.513 - 201.233
20	26491	BIORAD L1	CHOL	261 mg/dl	+1SD	183102	27-Aug-2022 10:24:03	252.400	7.210	230.77 - 274.03
21	26491	BIORAD L1	HDLC	59.6 mg/dl	+1SD	183103	27-Aug-2022 10:24:11	57.243	2.020	51.183 - 63.303



27-8-22

Result Reprint

Report Type : Controls 27-Aug-2022 Consumable: BIORAD L2

SR #	Lot #	Consumable	Test	Result Unit	Flag	Curve #	Result Date	Mean	SD	Interval (3SD)
1	89702	BIORAD L2	Na	125.10 mmol/l		0	27-Aug-2022 09:35:59	124.000	6.250	105.25 - 142.75
2	89702	BIORAD L2	K	5.66 mmol/l	F	0	27-Aug-2022 09:35:59	5.680	0.280	4.84 - 6.52
3	89702	BIORAD L2	Cl	86.80 mmol/l		0	27-Aug-2022 09:35:59	85.900	4.350	72.85 - 98.95
4	89702	BIORAD L2	SGPTD	93.2 U/L		183040	27-Aug-2022 09:38:06	94.700	9.550	66.05 - 123.35
5	89702	BIORAD L2	SGOTD	186.1 U/L		183042	27-Aug-2022 09:38:25	187.000	18.000	133 - 241
6	89702	BIORAD L2	ALPU	500 U/L		183044	27-Aug-2022 09:38:43	517.000	51.000	364 - 670
7	89702	BIORAD L2	GGT	171.9 U/L		183046	27-Aug-2022 09:39:01	176.000	18.000	122 - 230
8	89702	BIORAD L2	PHOS	7.45 mg/dl		183048	27-Aug-2022 09:39:19	7.500	0.600	5.7 - 9.3
9	89702	BIORAD L2	BID	1.09 mg/dl	-1SD	183050	27-Aug-2022 09:39:37	1.280	0.160	0.8 - 1.76
10	89702	BIORAD L2	BIT	4.03 mg/dl		183052	27-Aug-2022 09:39:55	4.260	0.540	2.64 - 5.88
11	89702	BIORAD L2	UREA	112.0 mg/dl	+1SD	183054	27-Aug-2022 09:40:13	100.000	7.500	77.5 - 122.5
12	89702	BIORAD L2	CRENZ	5.10 mg/dl		183056	27-Aug-2022 09:40:31	5.200	0.450	3.85 - 6.55
13	89702	BIORAD L2	GLU	295.9 mg/dl		183058	27-Aug-2022 09:40:49	291.000	22.500	223.5 - 358.5
14	89702	BIORAD L2	TRIG	83.5 mg/dl		183060	27-Aug-2022 09:41:07	85.700	6.450	66.35 - 105.05
15	89702	BIORAD L2	CHOL	103 mg/dl		183062	27-Aug-2022 09:41:25	101.000	7.750	77.75 - 124.25
16	89702	BIORAD L2	HDLc	21.2 mg/dl		183064	27-Aug-2022 09:41:43	23.000	2.250	16.25 - 29.75
17	89702	BIORAD L2	UA	10.1 mg/dl		183066	27-Aug-2022 09:42:01	10.400	0.750	8.15 - 12.65

Print Date 27-Aug-2022

Result Reprint

Report Type : Controls 27-Aug-2022 Consumable: BIORAD L2

Sr #	Lot #	Consumable	Test	Result Unit	Flag	Curve #	Result Date	Mean	SD	Interval (3SD)
18	89702	BIORAD L2	CA	12.6 mg/dl		183074	27-Aug-2022 09:43:13	13.000	1.050	9.85 - 16.15
19	89702	BIORAD L2	ALB	2.71 g/dl		183076	27-Aug-2022 09:43:31	2.700	0.210	2.07 - 3.33
20	89702	BIORAD L2	PRO	4.71 g/dl		183078	27-Aug-2022 09:43:49	4.600	0.300	3.7 - 5.5

Print Date 27-Aug-2022

