

CALIBRATION CERTIFICATE

NAME OF CUSTOMER:
OLI CLINICAL LABORATORY
EAST MAIN ROAD,
PENNADAM-606105

DATE:13.09.2022

DESCRIPTION OF THE EQUIPMENT: CENTRIFUGE

MODEL NO: C854/4

S.NO: CGLC-1206

COMPANY: REMI

INSTRUMENT USED FOR CALIBRATION: DIGITAL TACHOMETER

MODEL NO:KUSAM-MECO&KM-2234BL


SL.NO: S1049947

CERTIFIED BY: MSIR INDIA PVT. LTD

<i>REGULATOR STEEPS</i>	<i>INSTRUMENT SPEED</i>	<i>TACHOMETER READING</i>	<i>ALLOWABLE ERROR</i>	<i>ERROR OBSERVED ±</i>	<i>RESULT</i>
1.	700	719	±50	19	OK
3.	2100	2074	±50	26	OK
5.	3500	3465	±50	35	OK

NEXT CALIBRATION DUE ON: 12.09.2023

TESTED BY: G DINESH

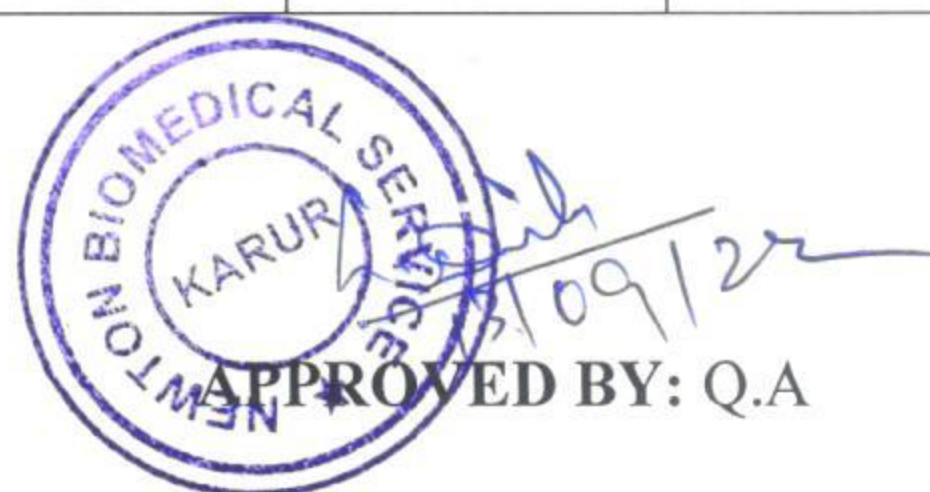

NOTE: 1) Calibration Points & due date is given as per customer request 2) This certificate refer only to particular item submitted for certificate 3) The calibration results reported are valid at the time of and under the stated conditions of the measurements 4) Any error in the certificate should be brought to our lab within 45 days from the date of issue of certificate.