

Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022


Clinical Path - Urine Routine Chemistry,Bilirubin (urine), -

	N
■ All Methods	254
■ Diazonium salt - (Your Method)	204
■ Manual - (Your Analyzer)	117

Evaluation Based On - Method wise Peer Grouping	
Your Result	Negative
Result Expected	+1,Neg

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

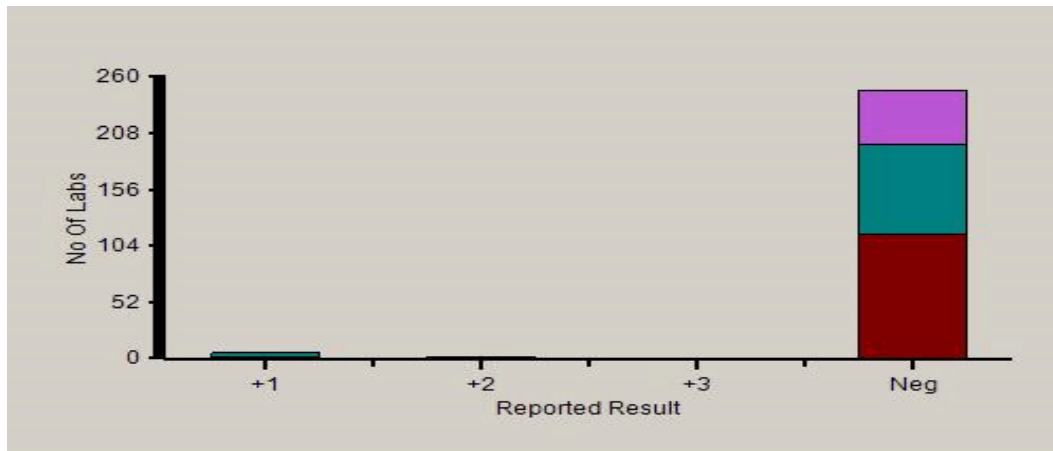

Analyte Methodwise Qualitative Result Report

Lab No.: 735
Lab Name : KGMT MULTISPECIALITY HOSPITAL
Report Date : 31/08/2022

Cycle No : 220207
Sample No : 1
Sample Date : 28-07-2022

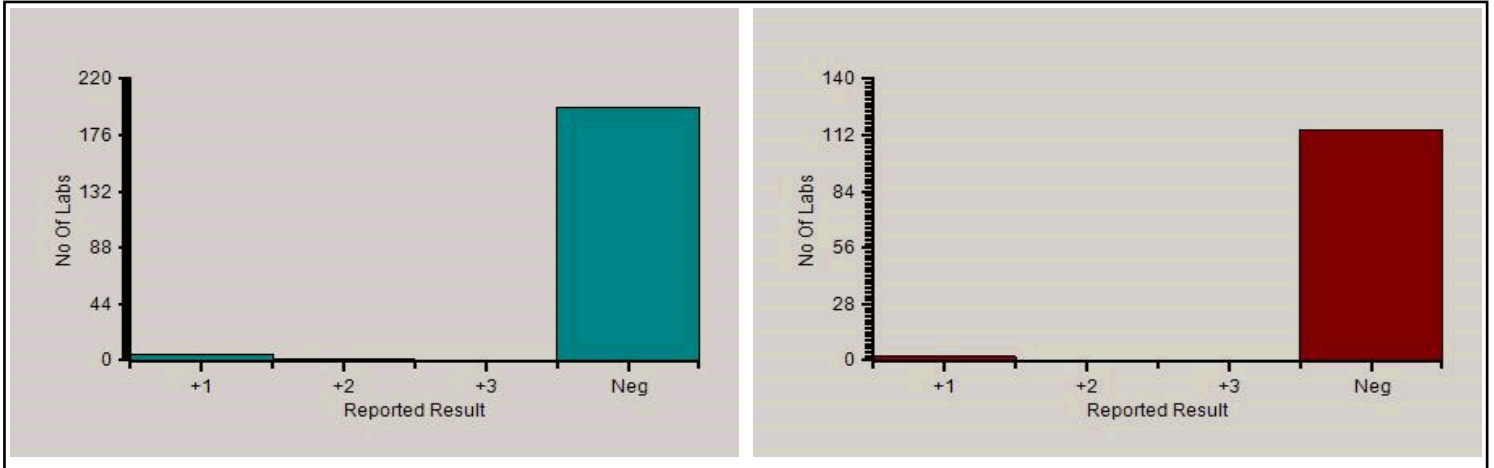

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022

Clinical Path - Urine Routine Chemistry,Blood (urine), -


	N
■ All Methods	256
■ Peroxidase enzyme - (Your Method)	129
■ Manual - (Your Analyzer)	118

Evaluation Based On - Method wise Peer Grouping

Your Result	Trace
Result Expected	+1,Neg,Tr

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

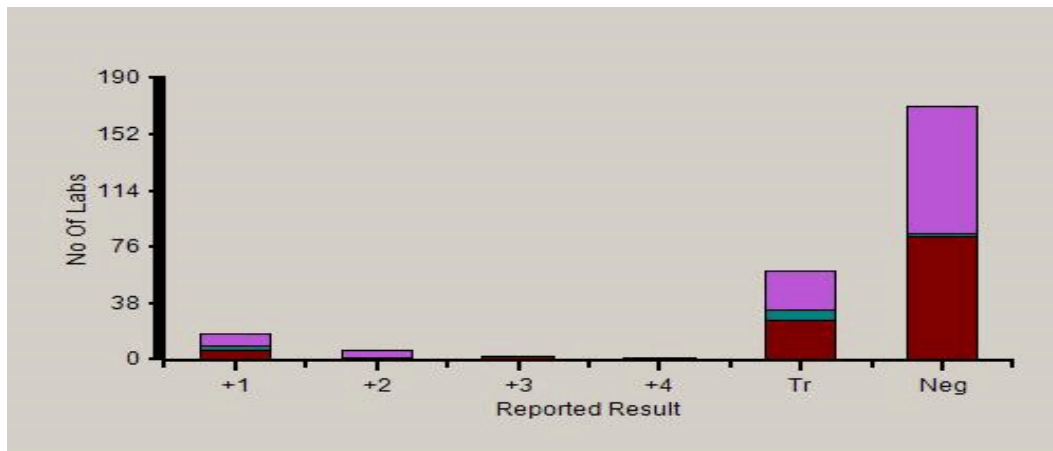

Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022

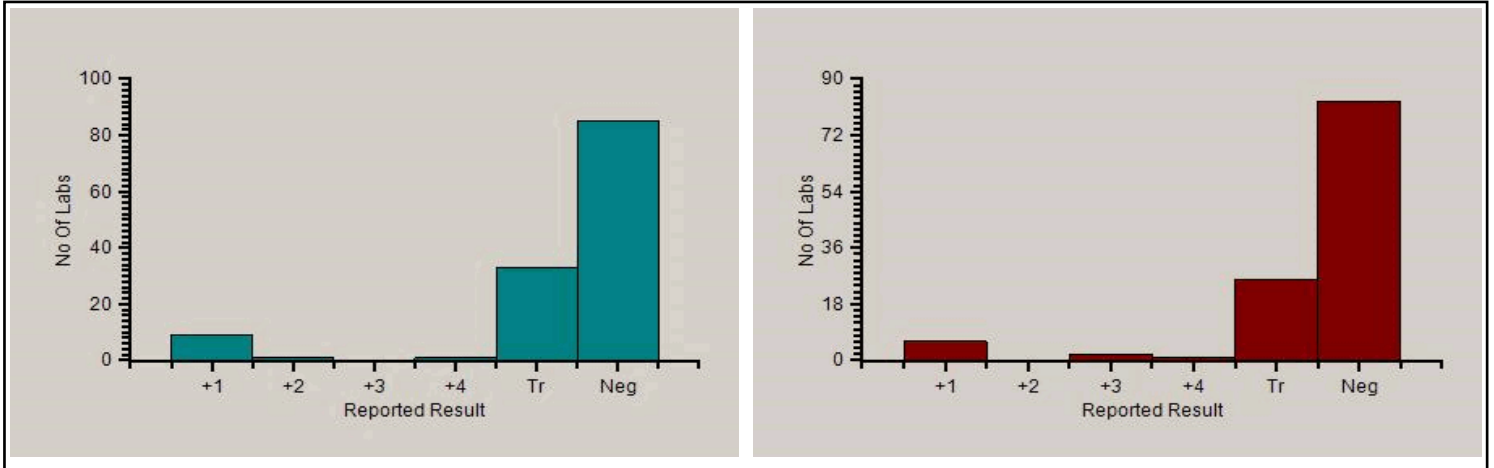

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+
Tr	: Trace
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022

Clinical Path - Urine Routine Chemistry, Glucose (urine), -


	N
■ All Methods	268
■ Glucose oxidase peroxidase - (Your Method)	179
■ Manual - (Your Analyzer)	127

Evaluation Based On - Method wise Peer Grouping

Your Result	4+
Result Expected	+2,+3,+4

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

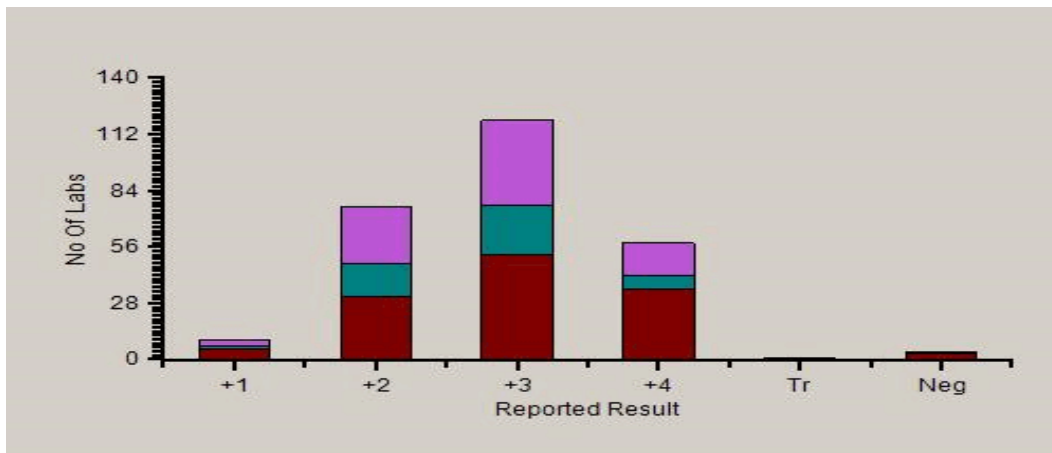

Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022

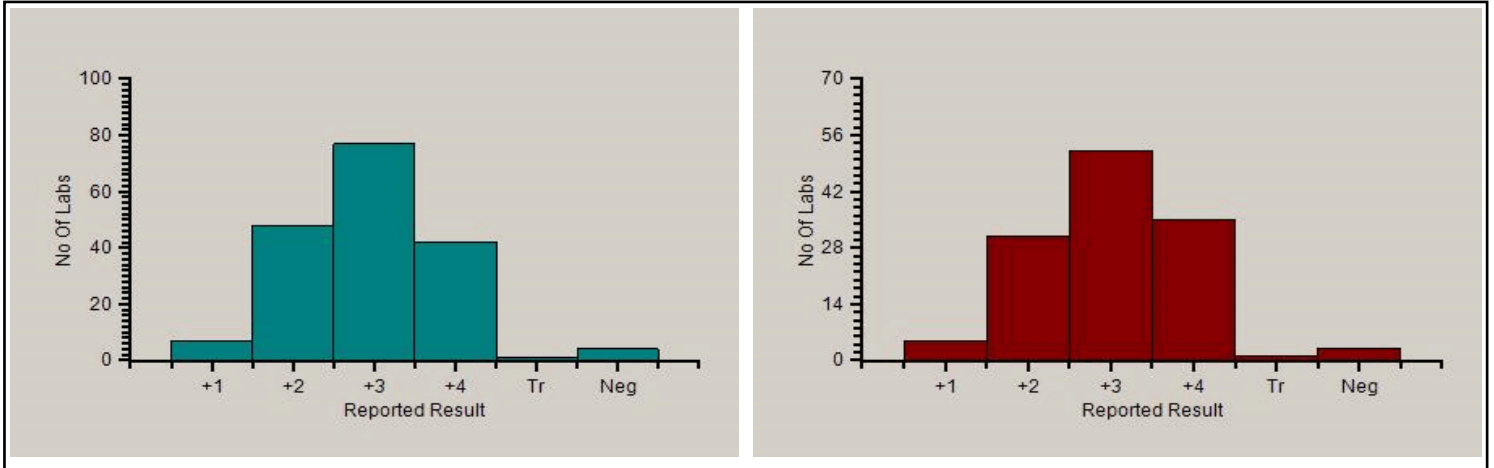

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+
Tr	: Trace
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022

Clinical Path - Urine Routine Chemistry, Ketone (urine), -


	N
■ All Methods	257
■ Hegal test - (Your Method)	13
■ Manual - (Your Analyzer)	120

Evaluation Based On - Method wise Peer Grouping

Your Result	Negative
Result Expected	+1, Neg, Tr

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

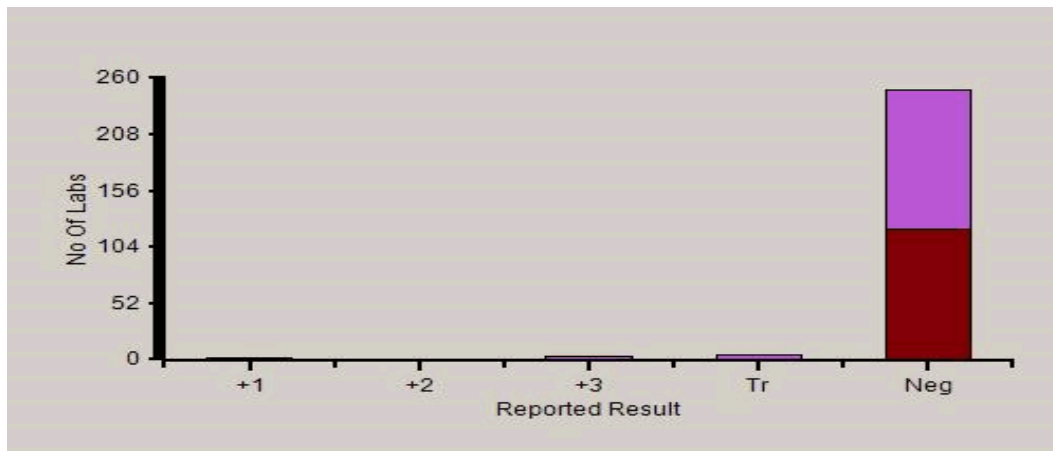

Analyte Methodwise Qualitative Result Report

Lab No.: 735
Lab Name : KGMT MULTISPECIALITY HOSPITAL
Report Date : 31/08/2022

Cycle No : 220207
Sample No : 1
Sample Date : 28-07-2022

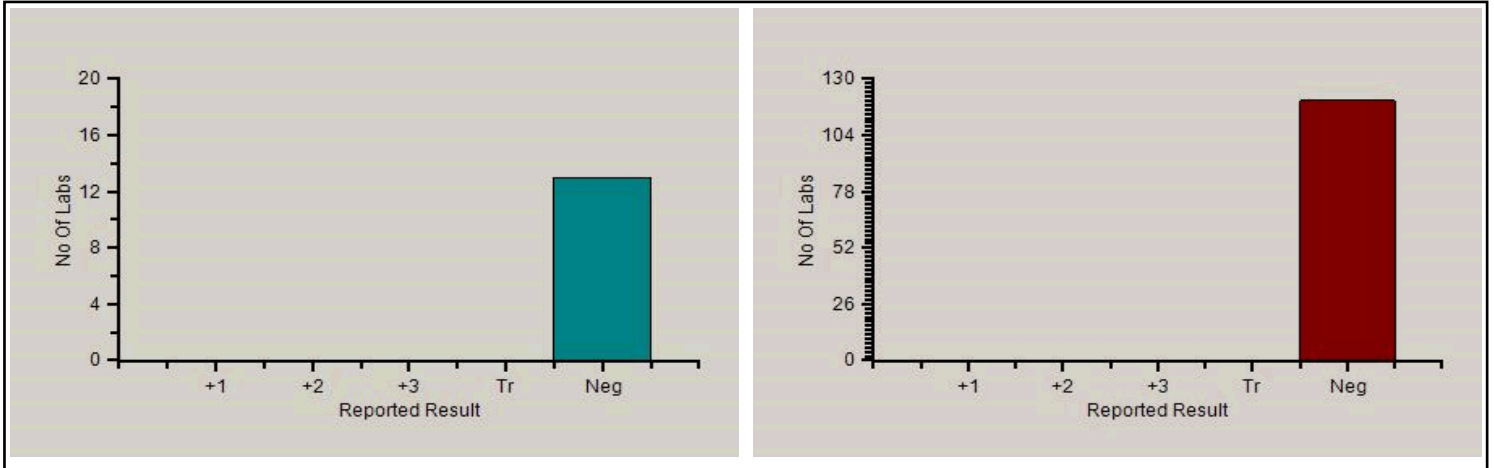

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
Tr	: Trace
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022


Clinical Path - Urine Routine Chemistry,Nitrite (urine), -

	All Methods	N
	Griess test - (Your Method)	256
	Manual - (Your Analyzer)	54
		117

Evaluation Based On - Method wise Peer Grouping	
Your Result	Absent
Result Expected	Abs

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

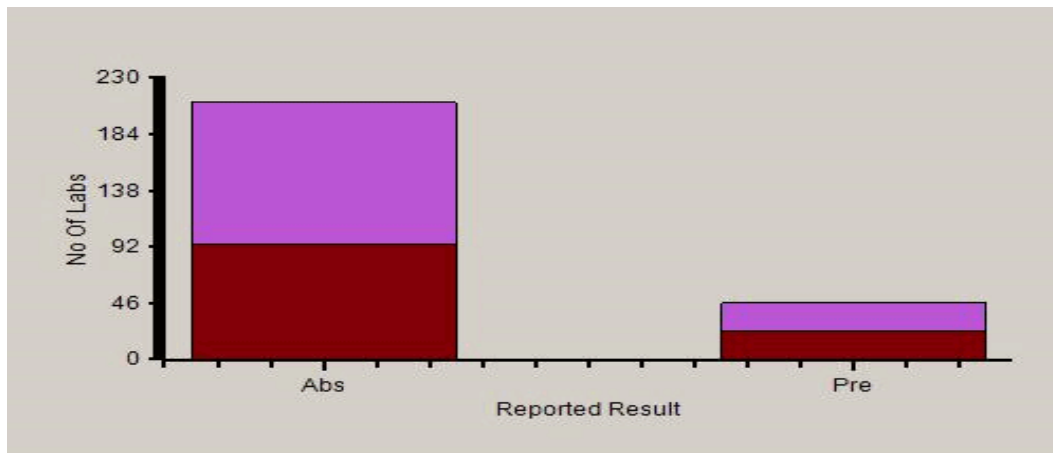


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 735
Lab Name : KGMT MULTISPECIALITY HOSPITAL
Report Date : 31/08/2022

Cycle No : 220207
Sample No : 1
Sample Date : 28-07-2022

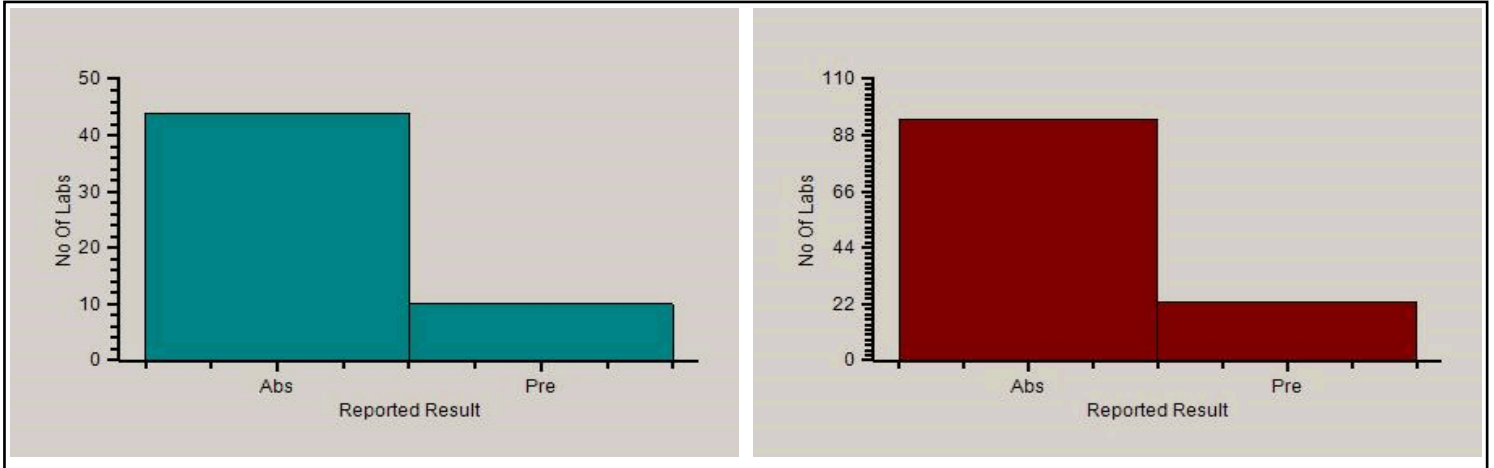

Reported Results Legends :-
 Abs : Absent
 Pre : Present

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022


Clinical Path - Urine Routine Chemistry,pH, -

	N
■ All Methods	260
■ Indicator Principle - (Your Method)	220
■ Manual - (Your Analyzer)	119

Evaluation Based On - Method wise Peer Grouping	
Your Result	6
Result Expected	6,6.5,7

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

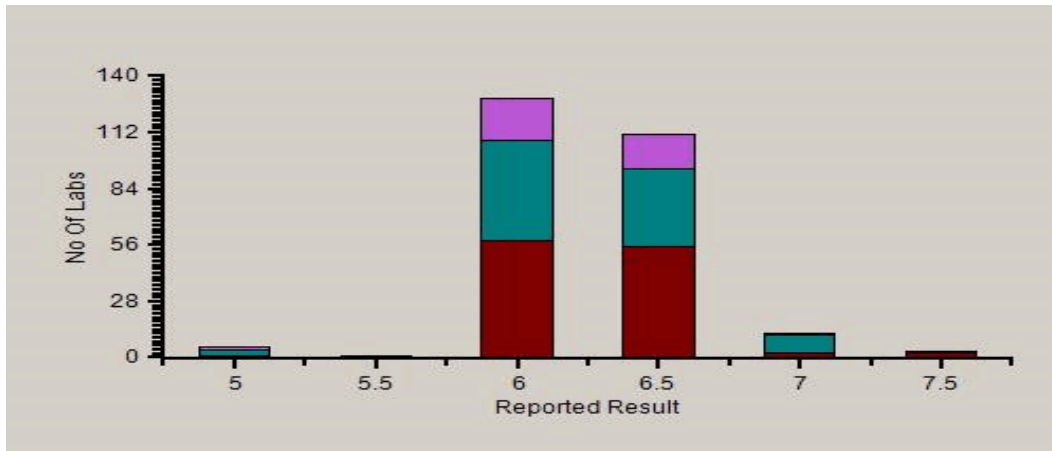

Analyte Methodwise Qualitative Result Report

Lab No.: 735
Lab Name : KGMT MULTISPECIALITY HOSPITAL
Report Date : 31/08/2022

Cycle No : 220207
Sample No : 1
Sample Date : 28-07-2022

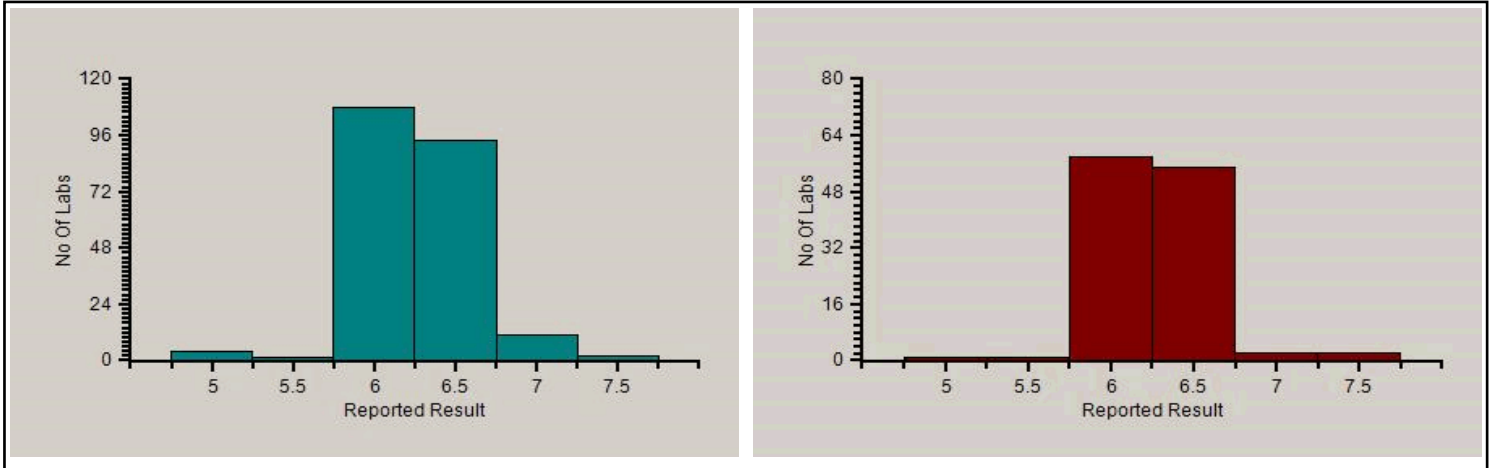

Reported Results Legends :-

5	: 5
5.5	: 5.5
6	: 6
6.5	: 6.5
7	: 7
7.5	: 7.5
8	: 8
8.5	: 8.5
9	: 9

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022


Clinical Path - Urine Routine Chemistry,Protein (Urine), -

	N
■ All Methods	265
■ Protein error principle of indicator - (Your Method)	126
■ Manual - (Your Analyzer)	124

Evaluation Based On - Method wise Peer Grouping	
Your Result	Trace
Result Expected	+1,Neg,Tr

Note : # is an indication that this parameter has not been evaluated



Frequency Histogram

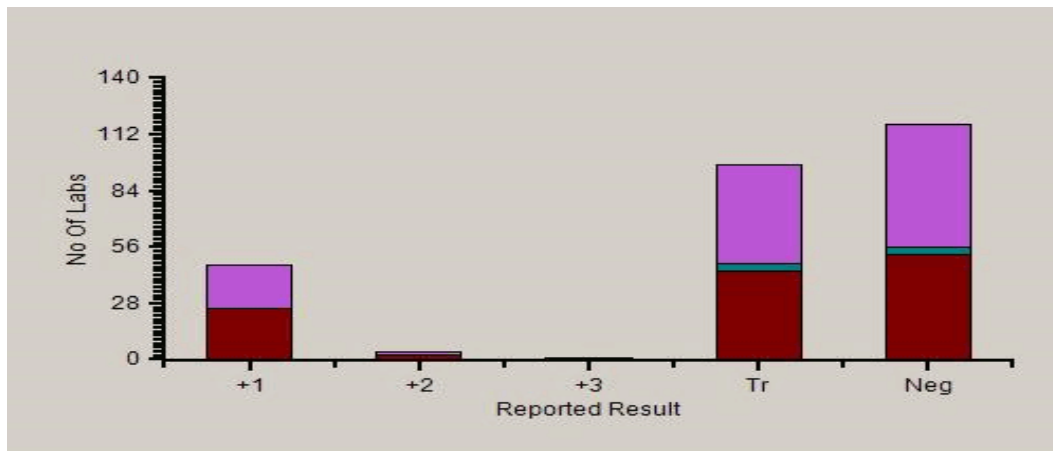

Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022

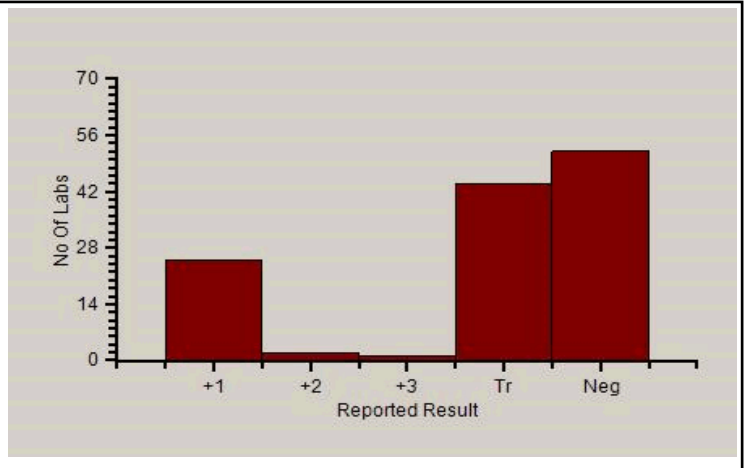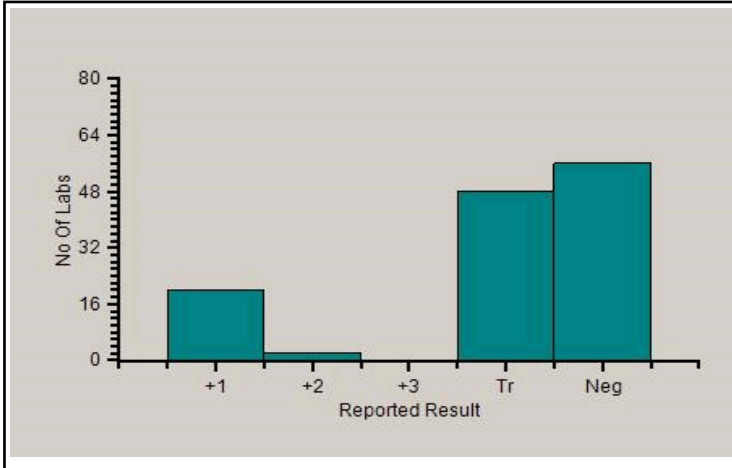

Reported Results Legends :-

+1	: 1+
+2	: 2+
+3	: 3+
Tr	: Trace
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022


Clinical Path - Urine Routine Chemistry, Specific Gravity, -

	N
■ All Methods	260
■ Ionic Concentration - (Your Method)	128
■ Manual - (Your Analyzer)	119

Evaluation Based On - Method wise Peer Grouping	
Your Result	1.015
Result Expected	1.015,1.020,1.025

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

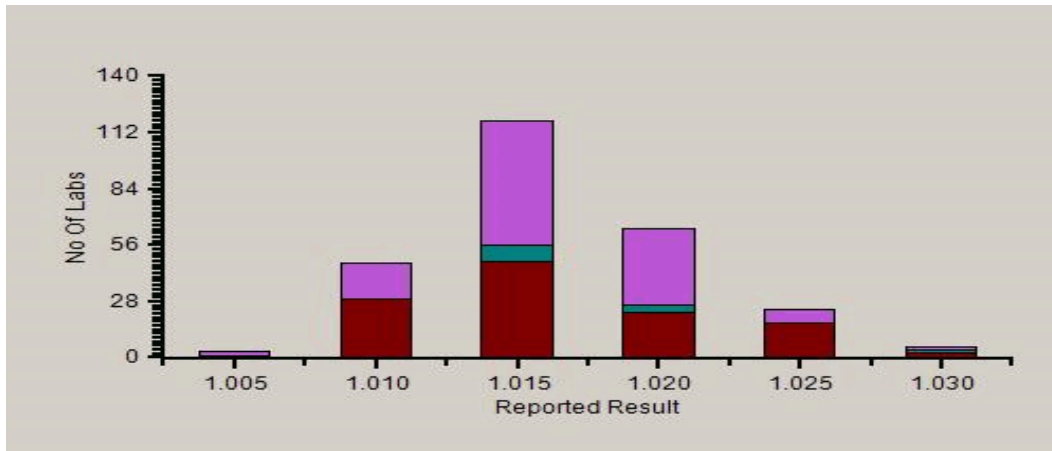

Analyte Methodwise Qualitative Result Report

Lab No.: 735
Lab Name : KGMT MULTISPECIALITY HOSPITAL
Report Date : 31/08/2022

Cycle No : 220207
Sample No : 1
Sample Date : 28-07-2022

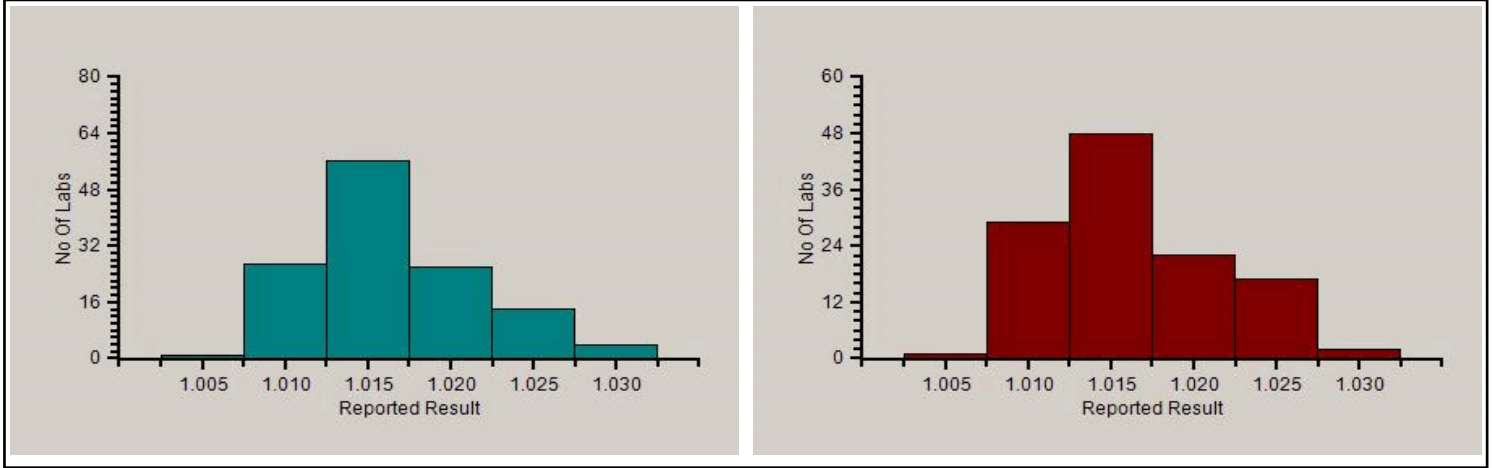

Reported Results Legends :-

1.005	: 1.005
1.010	: 1.010
1.015	: 1.015
1.020	: 1.020
1.025	: 1.025
1.030	: 1.030
1.035	: 1.035

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022

Clinical Path - Urine Routine Chemistry,Urine Pregnancy Test, -


	All Methods	N
	Immunochromatography - (Your Method)	180
	- - (Your Analyzer)	180

Evaluation Based On - Method wise Peer Grouping

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

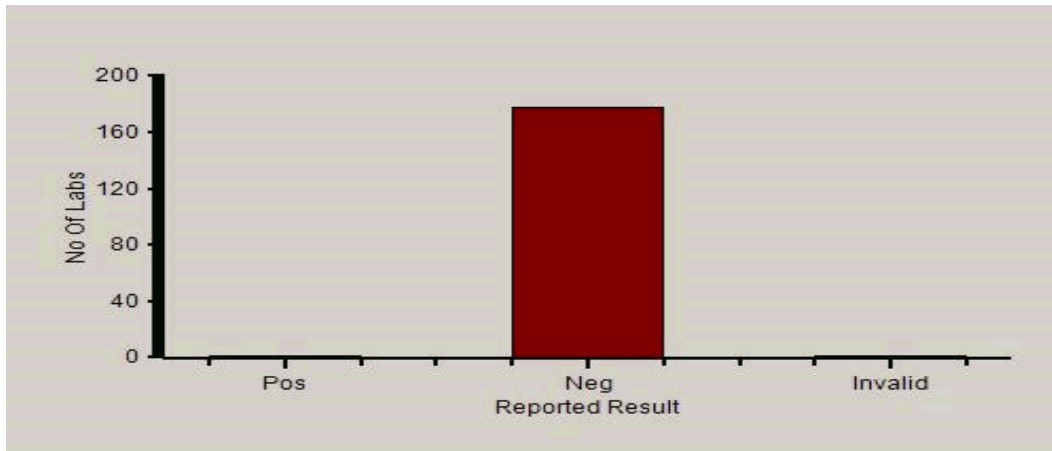

Analyte Methodwise Qualitative Result Report

Lab No.: 735
Lab Name : KGMT MULTISPECIALITY HOSPITAL
Report Date : 31/08/2022

Cycle No : 220207
Sample No : 1
Sample Date : 28-07-2022

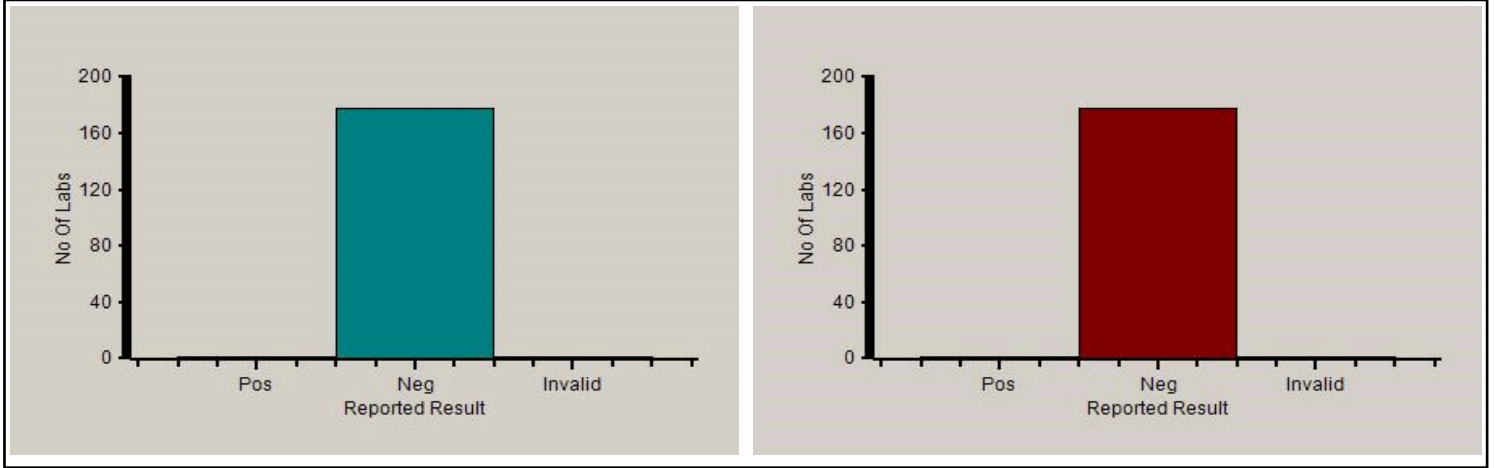

Reported Results Legends :-
 Pos : Positive
 Neg : Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 735
 Lab Name : KGMT MULTISPECIALITY HOSPITAL
 Report Date : 31/08/2022

Cycle No : 220207
 Sample No : 1
 Sample Date : 28-07-2022


Clinical Path - Urine Routine Chemistry,Urobilinogen (urine), -

	N
■ All Methods	245
■ Diethyleaminobenzaldehyde - (Your Method)	114
■ Manual - (Your Analyzer)	111

Evaluation Based On - Method wise Peer Grouping	
Your Result	Normal
Result Expected	+1,Nor

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

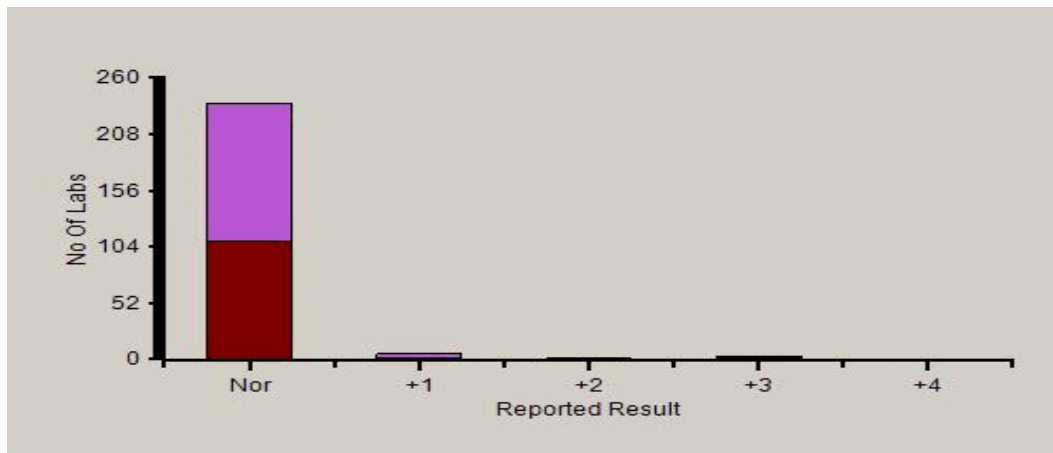

Analyte Methodwise Qualitative Result Report

Lab No.: 735
Lab Name : KGMT MULTISPECIALITY HOSPITAL
Report Date : 31/08/2022

Cycle No : 220207
Sample No : 1
Sample Date : 28-07-2022

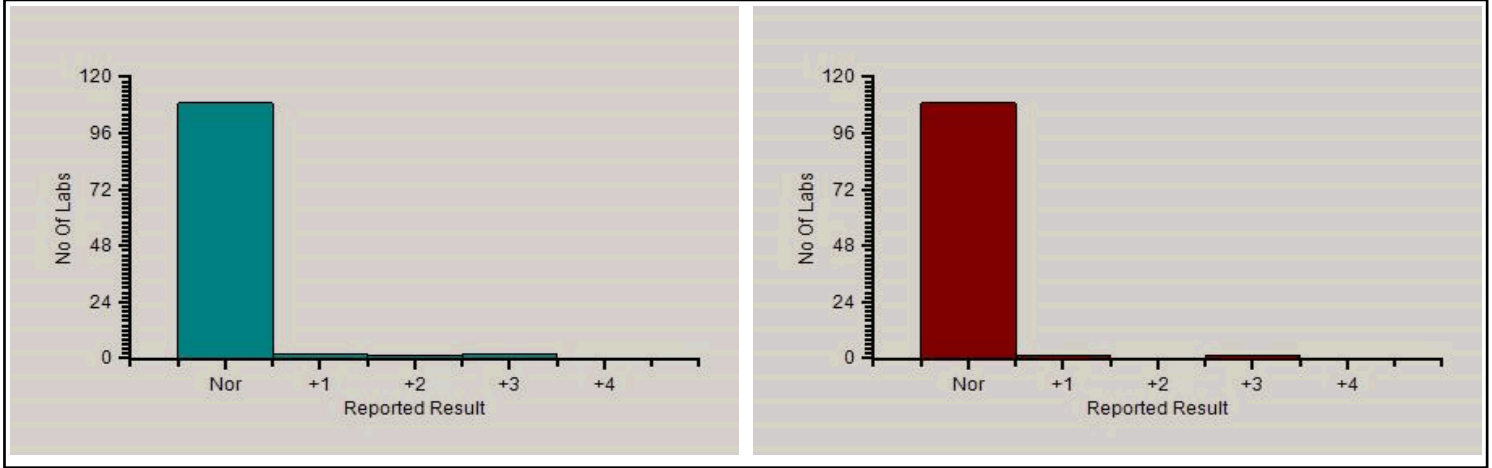

Reported Results Legends :-

Nor	: Normal
+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kiroi Road, Kurla (W),
 Mumbai - 400070

