

Analyte Methodwise Qualitative Result Report

Lab No.: 775
Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
Report Date : 10/12/2022

Cycle No : 220309
Sample No : 1
Sample Date : 30-09-2022

Immunoassay Extended,C-Reactive Protein Qualitative, mg/L


| | | |
|---|---|-----------------|
| | All Methods | N 109 |
| | Immunoturbidimetric - (Your Method) | 48 |
| | Beckman Coulter AU680 - (Your Analyzer) | 2 |

Your Result Normal

Result Expected #

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram



Analyte Methodwise Qualitative Result Report

Lab No.: 775
Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
Report Date : 10/12/2022

Cycle No : 220309
Sample No : 1
Sample Date : 30-09-2022



Reported Results Legends :-
 Nor : Normal
 Abn : Abnormal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 775
 Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
 Report Date : 10/12/2022

Cycle No : 220309
 Sample No : 1
 Sample Date : 30-09-2022


Immunoassay Extended,Dengue IgG, -

| | | |
|---|--------------------------------------|----------------|
| | All Methods | N 45 |
| | Immunochromatography - (Your Method) | 31 |
| | Manual - (Your Analyzer) | 38 |

| | |
|------------------------|----------|
| Your Result | Negative |
| Result Expected | Neg |

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

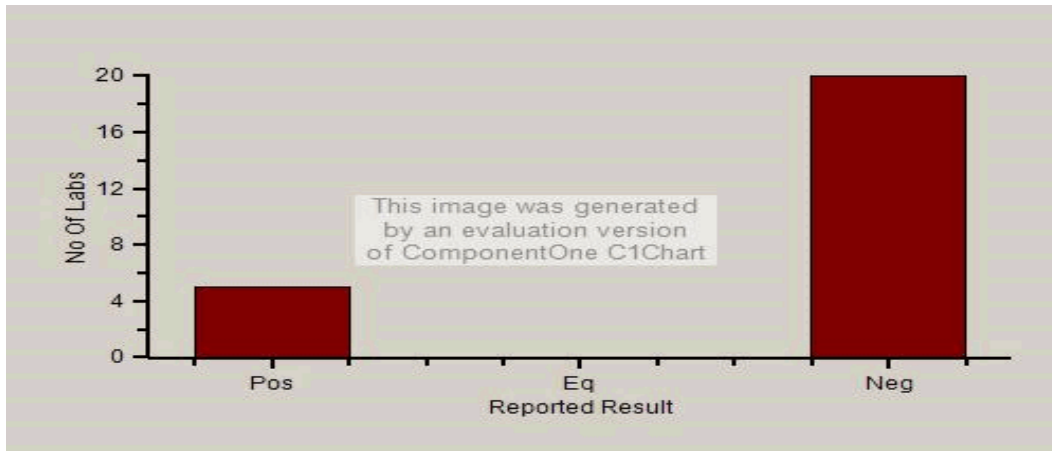

Analyte Methodwise Qualitative Result Report

Lab No.: 775
Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
Report Date : 10/12/2022

Cycle No : 220309
Sample No : 1
Sample Date : 30-09-2022

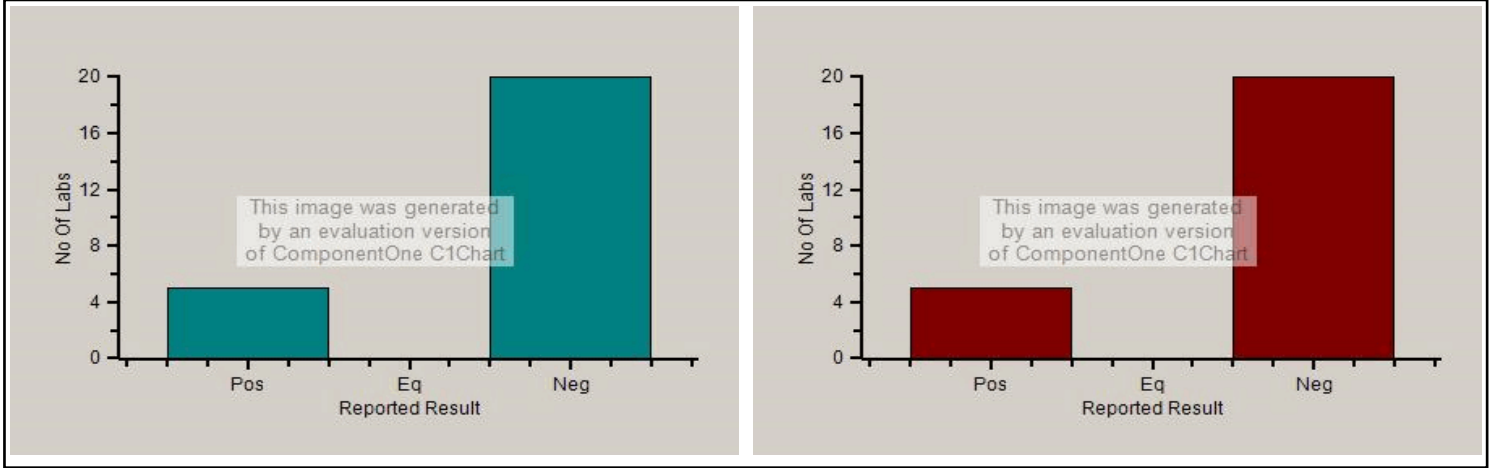

Reported Results Legends :-

| | |
|-----|--------------|
| Pos | : Positive |
| Eq | : Equivocal |
| BL | : Borderline |
| Neg | : Negative |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Analyte Methodwise Qualitative Result Report

Lab No.: 775
 Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
 Report Date : 10/12/2022

Cycle No : 220309
 Sample No : 1
 Sample Date : 30-09-2022


Immunoassay Extended,Dengue IgM, -

| | |
|--|----------|
| | N |
| ■ All Methods | 45 |
| ■ Immunochromatography - (Your Method) | 31 |
| ■ Manual - (Your Analyzer) | 38 |

| | |
|------------------------|----------|
| Your Result | Negative |
| Result Expected | Neg |

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

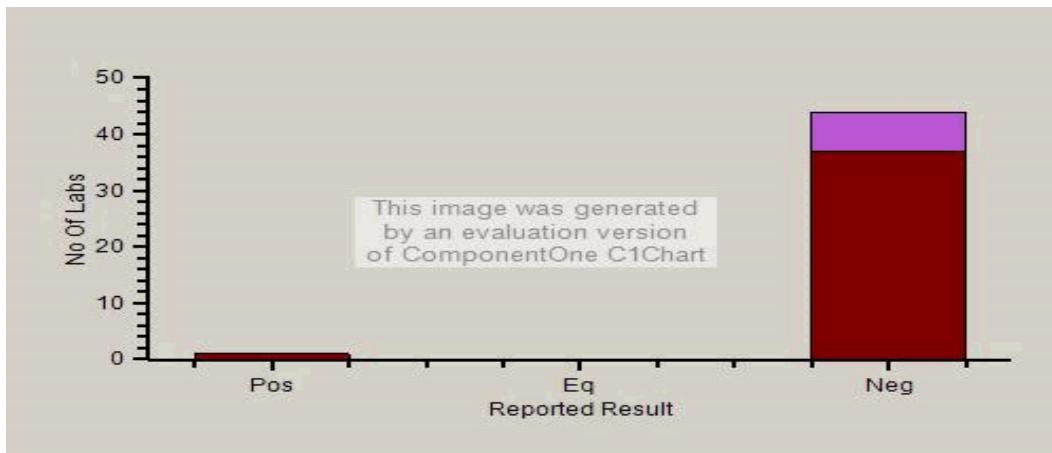

Analyte Methodwise Qualitative Result Report

Lab No.: 775
Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
Report Date : 10/12/2022

Cycle No : 220309
Sample No : 1
Sample Date : 30-09-2022

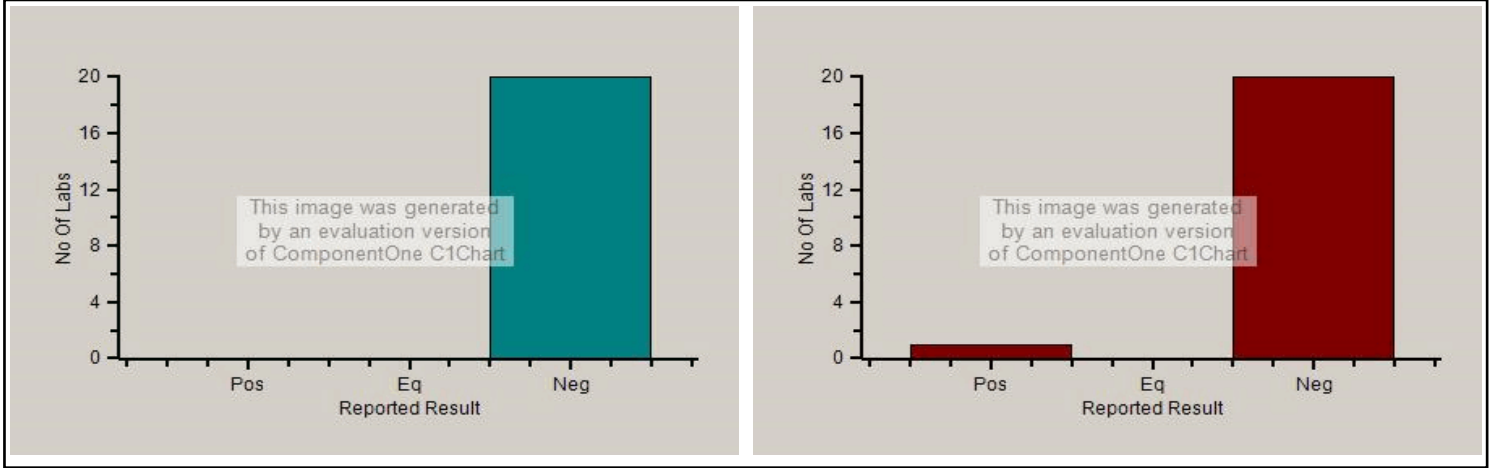

Reported Results Legends :-

| | |
|-----|--------------|
| Pos | : Positive |
| Eq | : Equivocal |
| BL | : Borderline |
| Neg | : Negative |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Analyte Methodwise Qualitative Result Report

Lab No.: 775
 Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
 Report Date : 10/12/2022

Cycle No : 220309
 Sample No : 1
 Sample Date : 30-09-2022


Immunoassay Extended,Dengue NS 1, -

| | |
|--|----------|
| | N |
| ■ All Methods | 156 |
| ■ Immunochromatography - (Your Method) | 133 |
| ■ Manual - (Your Analyzer) | 145 |

| | |
|------------------------|----------|
| Your Result | Negative |
| Result Expected | Neg |

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

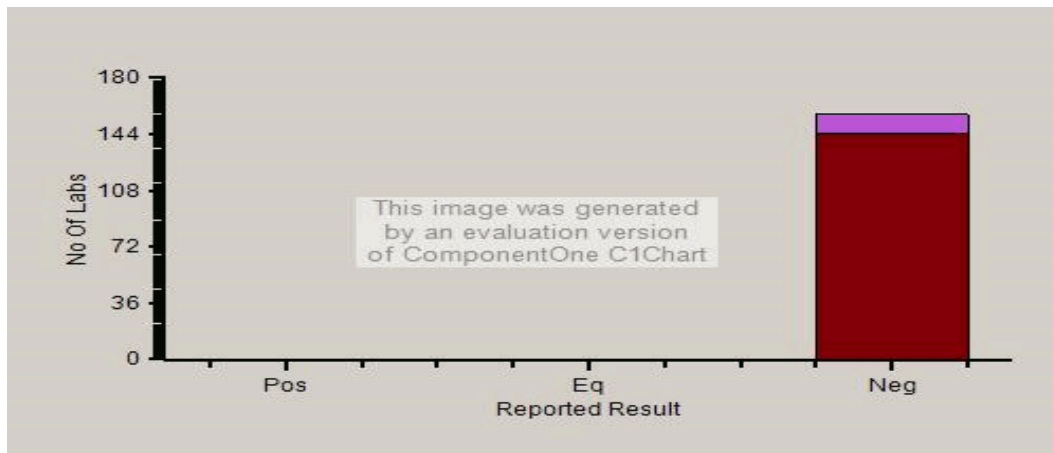


PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 775
Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
Report Date : 10/12/2022

Cycle No : 220309
Sample No : 1
Sample Date : 30-09-2022



Reported Results Legends :-

| | |
|-----|--------------|
| Pos | : Positive |
| Eq | : Equivocal |
| BL | : Borderline |
| Neg | : Negative |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 775
 Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
 Report Date : 10/12/2022

Cycle No : 220309
 Sample No : 1
 Sample Date : 30-09-2022


Immunoassay Extended,HBsAg, Nil

| | |
|--|----------|
| | N |
| ■ All Methods | 214 |
| ■ Immunochromatography - (Your Method) | 155 |
| ■ Manual - (Your Analyzer) | 135 |

| | |
|------------------------|--------------|
| Your Result | Non-reactive |
| Result Expected | NR |

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram




PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 775
Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
Report Date : 10/12/2022

Cycle No : 220309
Sample No : 1
Sample Date : 30-09-2022



Reported Results Legends :-

- R : Reactive
- NR : Non-reactive
- Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 775
 Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
 Report Date : 10/12/2022

Cycle No : 220309
 Sample No : 1
 Sample Date : 30-09-2022


Immunoassay Extended,HCV, -

| | |
|--|----------|
| | N |
| ■ All Methods | 121 |
| ■ Immunochromatography - (Your Method) | 96 |
| ■ Manual - (Your Analyzer) | 88 |

| | |
|------------------------|--------------|
| Your Result | Non-reactive |
| Result Expected | NR |

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

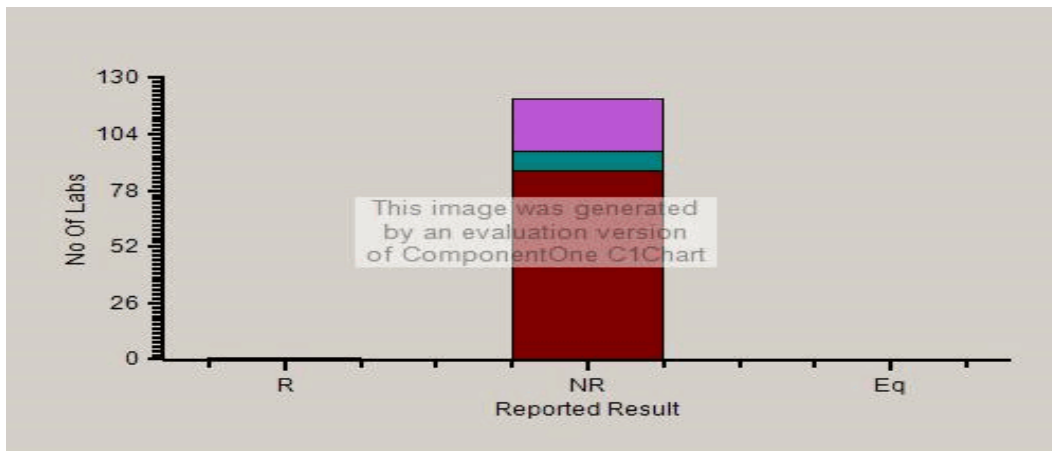

Analyte Methodwise Qualitative Result Report

Lab No.: 775
Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
Report Date : 10/12/2022

Cycle No : 220309
Sample No : 1
Sample Date : 30-09-2022



Reported Results Legends :-

| | |
|----|----------------|
| R | : Reactive |
| NR | : Non-reactive |
| Eq | : Equivocal |

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 775
 Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
 Report Date : 10/12/2022

Cycle No : 220309
 Sample No : 1
 Sample Date : 30-09-2022


Immunoassay Extended,HIV Ab, -

| | |
|--|----------|
| | N |
| ■ All Methods | 132 |
| ■ Immunochromatography - (Your Method) | 119 |
| ■ Manual - (Your Analyzer) | 113 |

| | |
|------------------------|--------------|
| Your Result | Non-reactive |
| Result Expected | NR |

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram



Analyte Methodwise Qualitative Result Report

Lab No.: 775
Lab Name : DR AMRISH MEHTA'S APPLE DIAGNOSTIC
Report Date : 10/12/2022

Cycle No : 220309
Sample No : 1
Sample Date : 30-09-2022



Reported Results Legends :-

| | |
|-------|---------------------|
| R | : Reactive |
| NR | : Non-reactive |
| Eq | : Equivocal |
| Indet | : Indeterminate |
| HIV-1 | : HIV-1 Ab Reactive |
| HIV-2 | : HIV-2 Ab Reactive |

Comments :

- Interpretation when an analyte is reported for multiple samples in a Round:
- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
 - b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kiroi Road, Kurla (W),
 Mumbai - 400070

