

Calibration Certificate

Name	Annapurna Pathology
Address of Customer	Bandariba, Charbagh, Lucknow
City	Lucknow
State	Uttar Pradesh
PIN	226004
Phone	9839131582
Email	Anubhaagarwal0706@gmail.com
Name of Instrument	Meril CliniQuant Micro Instrument
Type	Biochemistry Analyzer
Serial No	CM0901106
Calibration Date	14-12-2022
Calibration Valid upto	13-12-2023

This is to Certify that Biochemistry Analyzer Meril CliniQuant Micro Instrument Sr.No. CM0901106 Installed at Annapurna Pathology calibrated by our engineer on 14-12-2022 with appropriate and sophisticated tools.

TEST ITEMS AND RESULT

Appearance	OK
AD Value Range (120<AD<350)	OK
Temperature Checking (at 37°C)	OK
Printer Test	OK
Aspiration Volume Range	OK
Stability of Pot. Dichromate	OK
Absorbency Linearity at 340	OK
PC Communication Checking	OK

Engineer Name: **Mr. Virendra Verma**

Engineer Sign

Stamp



(Handwritten signature)



Meril
Diagnostics

Results of Internal Quality Control

Test	Qc Range (Level 1)	Result	Qc Range (Level 2)	Result
ALP	75 - 109	107.1	184 - 266	204.34
Albumin	2.48 - 3.56	3.27	4.06 - 5.84	4.4
SGOT	39.4 - 56.6	51.09	118.3 - 170.3	129.38
SGPT	36.2 - 52.2	43.79	112.8 - 162.4	142.03
Total Bil	1.44 - 2.08	1.86	5.21 - 7.49	5.65
Calcium	7.57-9.63	8.32	10.60 - 13.50	10.83
Creatinine	0.75 - 1.07	1.05	2.39 - 3.43	3.23
HDL	25 - 35	26.68	35 - 45	36.94
Triglycerides	86 - 120	114.14	157 - 217	164.75
Uric Acid	5.03 - 6.81	5.45	10.29 - 13.93	12.62

Remarks:

We hereby certify that Instrument standardization / calibrations have been carried. Verified by evaluating controls before processing patients Samples and obtained results are satisfactory. Instrument is ready for regular use.










Engineer Name: **Mr. Virendra Verma**

Engineer Sign

Stamp











Snapshots of controls: (Level 1)

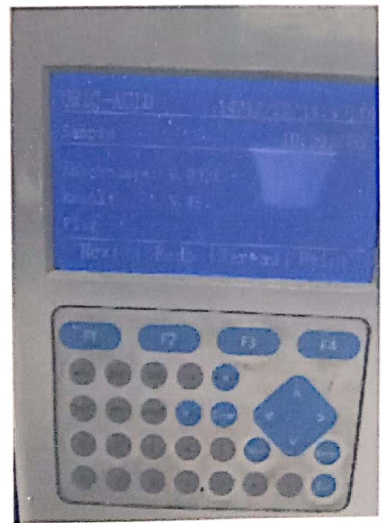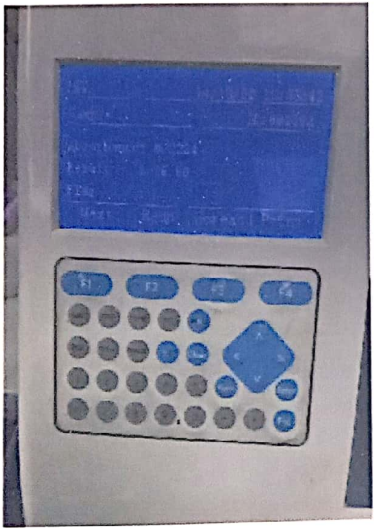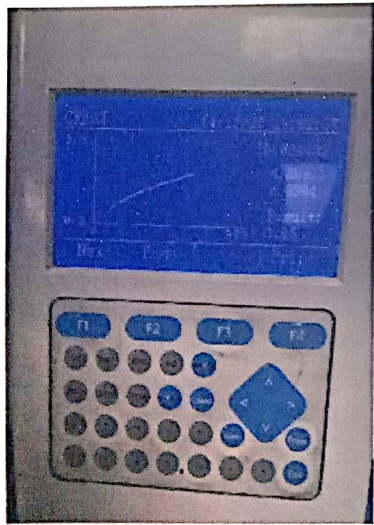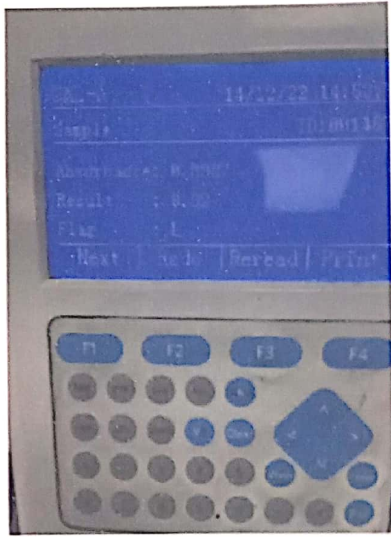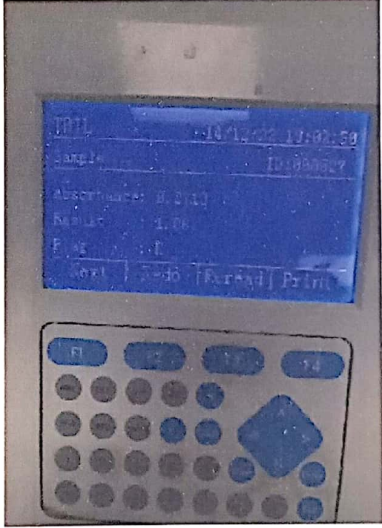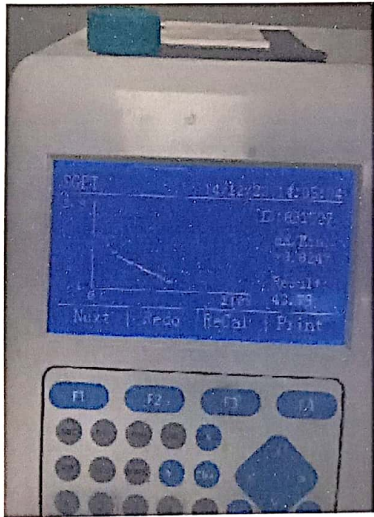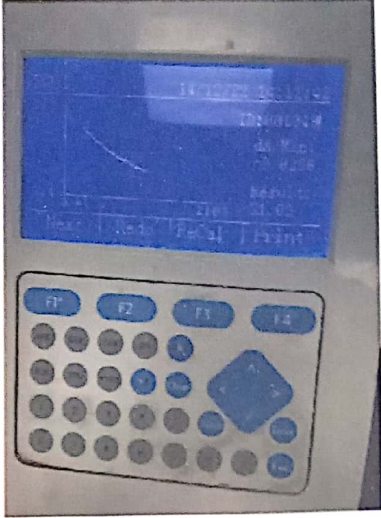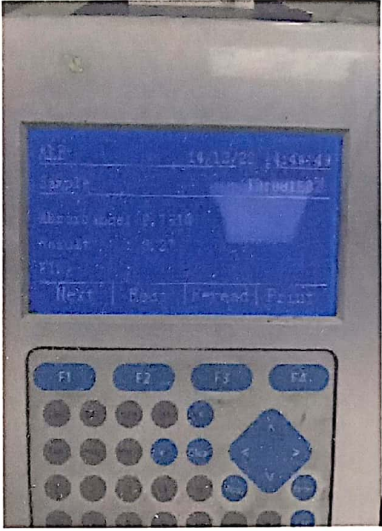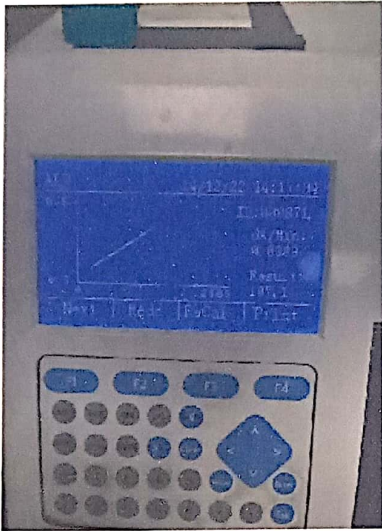

Dr. A. H. T +91 260 3052100
+91 260 3052125
www.merilife.com

Meril Diagnostics Pvt. Ltd.
Survey No 135/2/B, Biakhia House
Muktanand Marg Chala
Vap - 396191, Gujarat, India

Snapshots of controls: (Level 2)

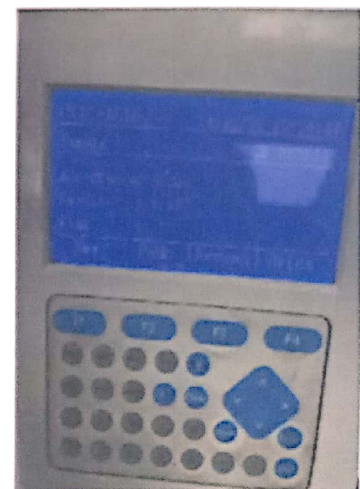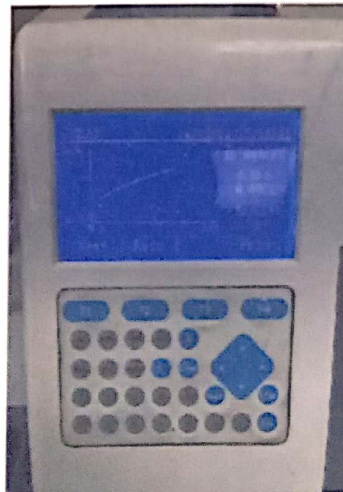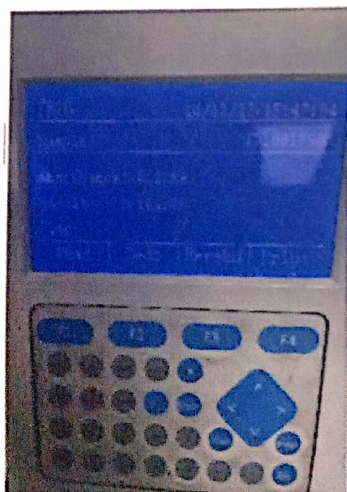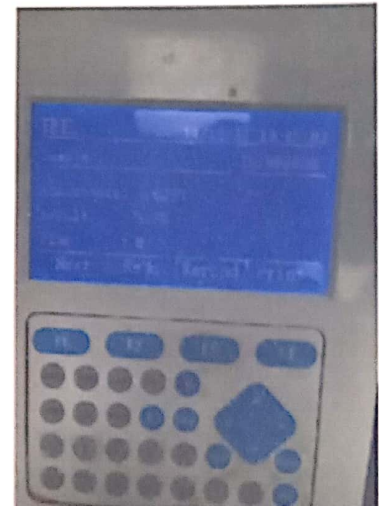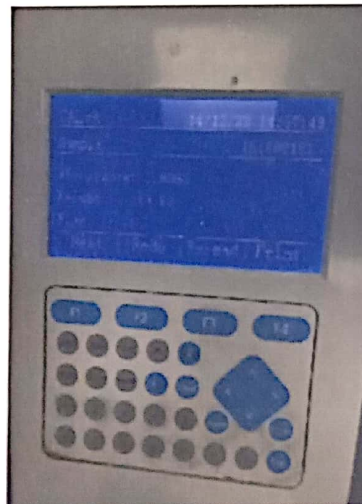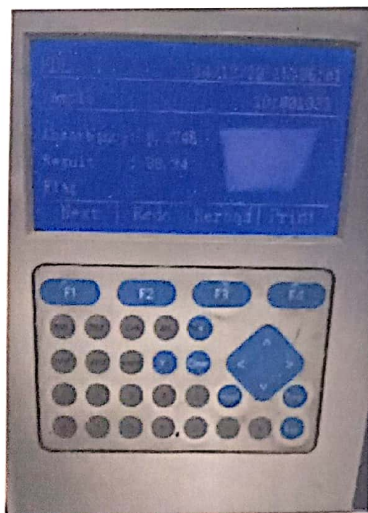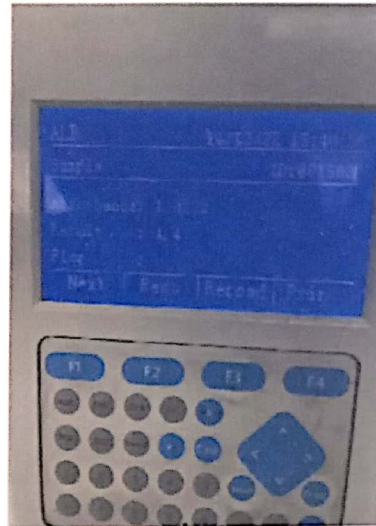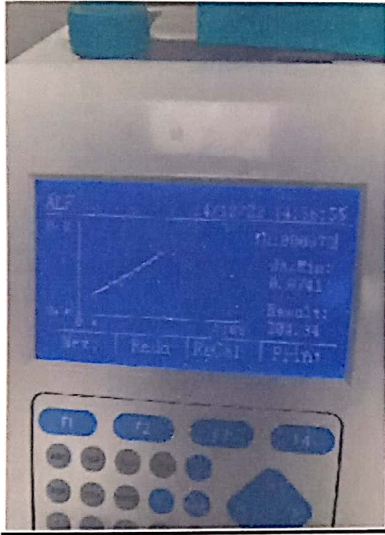

Handwritten signature

T +91 260 3052100
 F +91 260 3052125
 www.merilite.com

Meril Diagnostics Pvt. Ltd
 Survey No 135/2/B, Birakhia House
 Muktanand Marg, Chela
 Vap. 396191, Gujarat, India