

Analyte Methodwise Qualitative Result Report

Lab No.: 456
Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, BANSWARA
Report Date : 10/12/2022

Cycle No : 220309
Sample No : 1
Sample Date : 30-09-2022


Clinical Path - Urine Sediment Analysis Image, Crystal, -

	All Methods	N 163
	- - (Your Method)	164
	- - (Your Analyzer)	164

Your Result	Bilirubin crystals
Result Expected	BC

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram

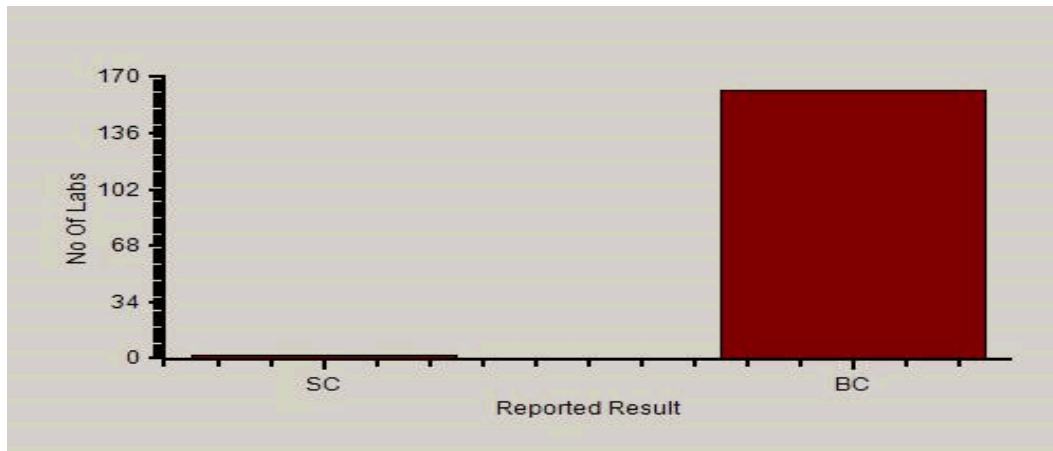

Analyte Methodwise Qualitative Result Report

Lab No.: 456
 Lab Name : MEDICENTRE SONOGRAPHY & CLINICAL LAB, BANSWARA
 Report Date : 10/12/2022

Cycle No : 220309
 Sample No : 1
 Sample Date : 30-09-2022

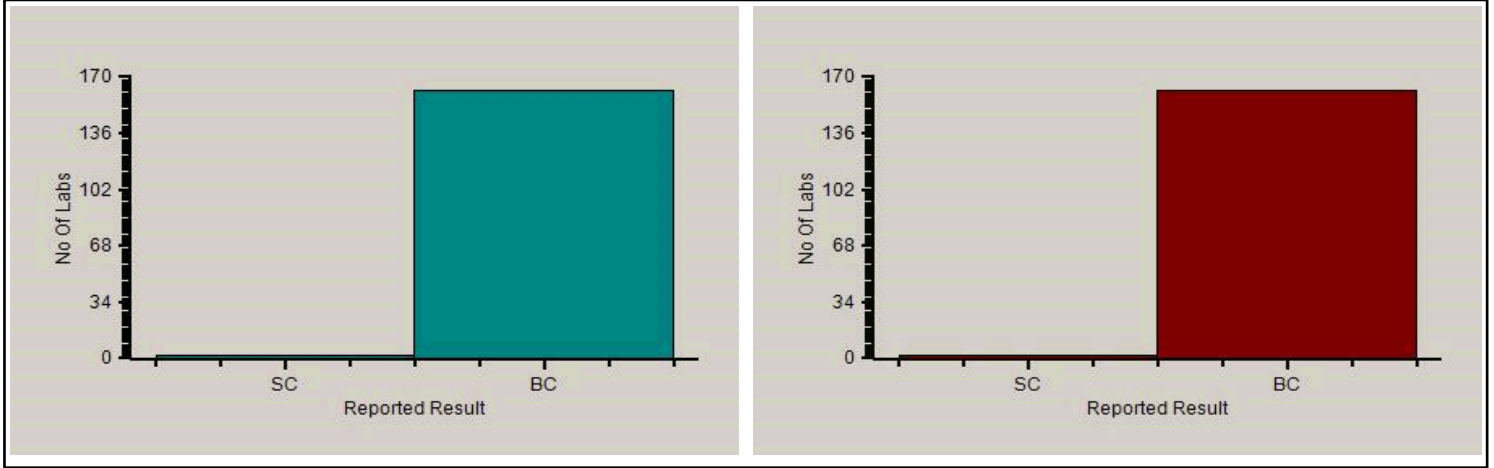

Reported Results Legends :-

TPC	: Triple phosphate crystal
UAC	: Uric acid crystal
CC	: Cystine crystal
SC	: Sulfonamide crystal
UC	: Urate crystal
CaOx	: Calcium oxalate crystal
BC	: Bilirubin crystals
CHC	: Cholesterol crystals
ABC	: Ammonium Biurate crystal
NCS	: No crystal seen
APC	: Ammonium phosphate crystal
APC	: Amorphous Phosphate Crystal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
 PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kiroi Road, Kurla (W),
 Mumbai - 400070

