

**Analyte Methodwise Qualitative Result Report**

**Lab No.:** 454  
**Lab Name :** MEDICENTRE SONOGRAPHY AND CLINICAL LAB, CHITTORGARH  
**Report Date :** 10/12/2022

**Cycle No :** 220309  
**Sample No :** 1  
**Sample Date :** 30-09-2022


**Clinical Path - Urine Sediment Analysis Image, Crystal, -**

	All Methods	<b>N</b> 163
	- - (Your Method)	164
	- - (Your Analyzer)	164

<b>Your Result</b>	Bilirubin crystals
<b>Result Expected</b>	BC

**Note :** # is an indication that this parameter has not been evaluated


**Frequency Histogram**

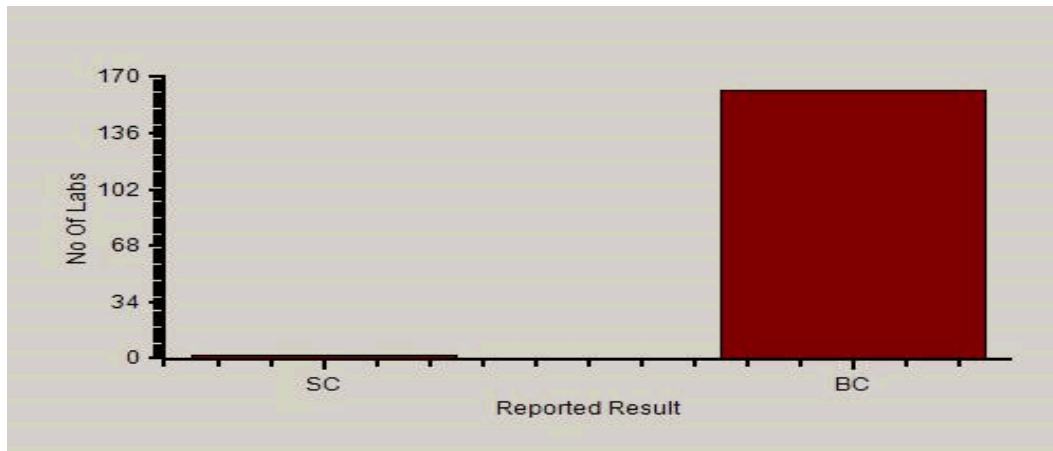

**Analyte Methodwise Qualitative Result Report**

Lab No.: 454  
 Lab Name : MEDICENTRE SONOGRAPHY AND CLINICAL LAB, CHITTORGARH  
 Report Date : 10/12/2022

Cycle No : 220309  
 Sample No : 1  
 Sample Date : 30-09-2022

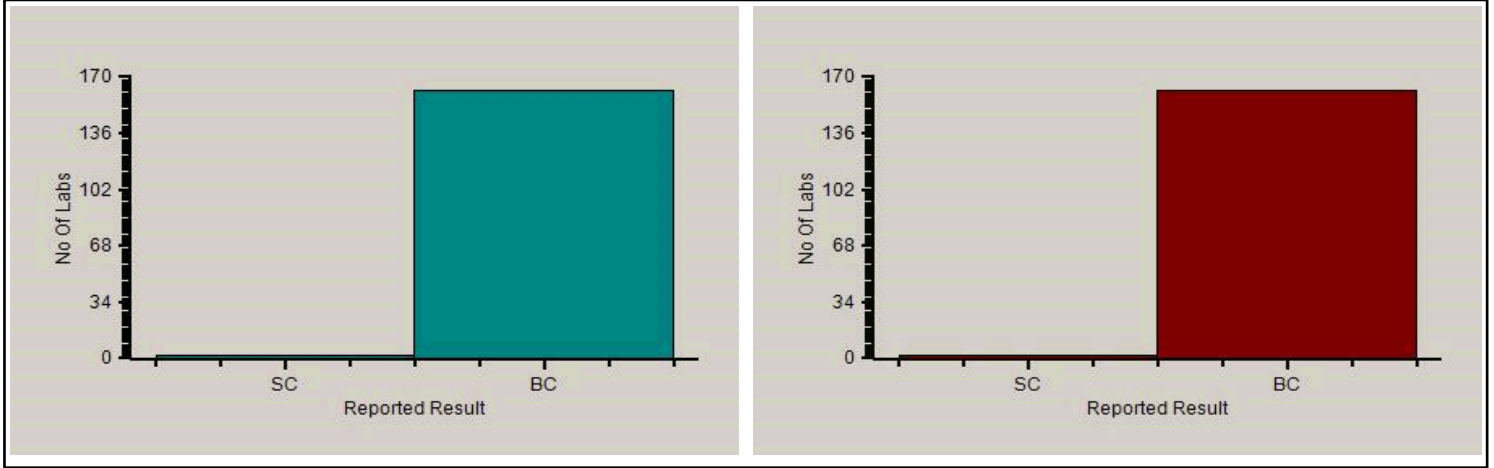

**Reported Results Legends :-**

TPC	: Triple phosphate crystal
UAC	: Uric acid crystal
CC	: Cystine crystal
SC	: Sulfonamide crystal
UC	: Urate crystal
CaOx	: Calcium oxalate crystal
BC	: Bilirubin crystals
CHC	: Cholesterol crystals
ABC	: Ammonium Biurate crystal
NCS	: No crystal seen
APC	: Ammonium phosphate crystal
APC	: Amorphous Phosphate Crystal

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance. Review for systematic error

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
 PT coordinator & Technical Manager, MHL EQAS  
 Unit No. 409-416.  
 Commercial Building - 1A,  
 Kohinoor Mall, Kiroi Road, Kurla (W),  
 Mumbai - 400070

