

CALIBRATION / TESTING REPORT


CUSTOMER DETAILS: KAMALA SPECIALITY HOSPITAL PRIVATE LIMITED, KOVILPATTI, TAMIL NADU		CERTIFICATE NO	TICS/23/01/003
		EQUIPMENT NAME	SEMI AUTO ANALYSER
		MANUFACTURE	ERBA
		MODEL	CHEM 7
CALIBRATION DATE	09/01/2023	SERIAL NO	81201
CALIBRATION DUE DATE	08/01/2024	INSTALLED DEPARTMENT	LAB
LOCATION OF CALIBRATION	SITE	ASSET NUMBER	KSH-LAB-002

- | | | |
|------------------------------------|------------------------------|--|
| 1. General maintenance required | <input type="checkbox"/> Yes | <input checked="" type="checkbox"/> No |
| 2. Any Physical damage observed | <input type="checkbox"/> Yes | <input checked="" type="checkbox"/> No |
| 3. Spare Replacement (if required) | <input type="checkbox"/> Yes | <input checked="" type="checkbox"/> No |

TEST EQUIPMENT	MANUFACTURE	SERIAL NUMBER	CERTIFICATE NUMBER/VALIDITY
ELECTRICAL SAFTY ANALYZER	DATREND	VPM 18040011	ACCS221441/28-07-2023

*The above mentioned instrument has been tested using standards manufactures recommended protocols, using equipments having traceability to National/International standards.

ACCEPTABLE FOR USE
 CORRECTIVE MAINTENANCE REQUIRED
 REMOVED FROM USE

Calibrated By : 
 Mandrananthu

Authorized Sign With Seal



*Electrical safety test result attached

CERTIFICATE NO: TICS/23/01/003

TESTING REPORT			
TEST EQUIPMENT	MANUFACTURE	MODEL	SERIAL NUMBER
ELECTRICAL SAFTY ANALYZER	DATREND	V Pad-mini	VPM 18040011

TEST REPORT –Electrical Safety


Test Standard: IEC 62353

Parameter	Units	Value	Limits	Status
Main Voltage L1-L2	V	233.3	240±10	PASS
Main Voltage L1-G(PE)	V	234.1	240±10	PASS
Main Voltage L2-G(PE)	V	3.1	<5	PASS
Load Current	A	2.13	As per unit	PASS
Protective Earth Resistance	Ω	0	<0.3	PASS
Point-to-Point Resistance	Ω	0	<0.5	PASS
Equipment Leakage	μA	2.3	Class I - < 500 Class II - < 100	PASS
Applied Part Leakage	μA	0	Type BF - < 5mA Type CF- <50μA*	PASS

* Note: Defibrillator paddles 100 μA, per IEC 60601-2-4

The above mentioned instrument has been tested using standards manufactures recommended protocols, using equipments having traceability to National/International standards.

M
Mandua monthly

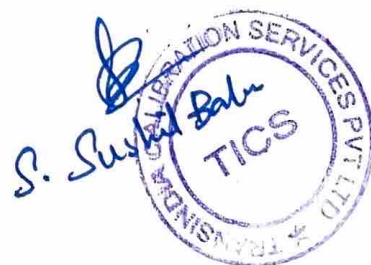

PAGE NO : 2/2