

**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022


**Clinical Path - Urine Routine Chemistry,Bilirubin (urine), -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	229
<span style="color: teal;">■</span> Photoelectric colorimetry - (Your Method)	17
<span style="color: red;">■</span> Urometer 120 - (Your Analyzer)	6

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	Negative
<b>Result Expected</b>	+1,Neg

**Note :** # is an indication that this parameter has not been evaluated


Frequency Histogram

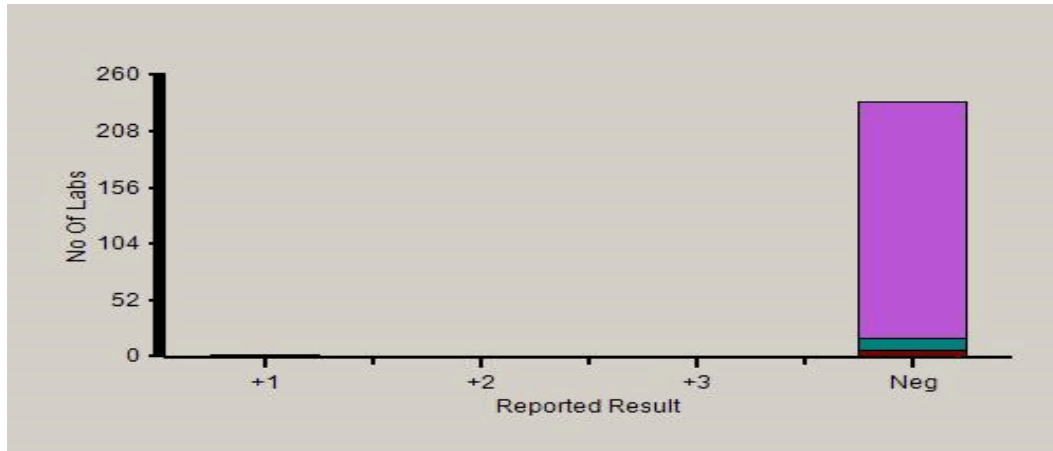

**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022

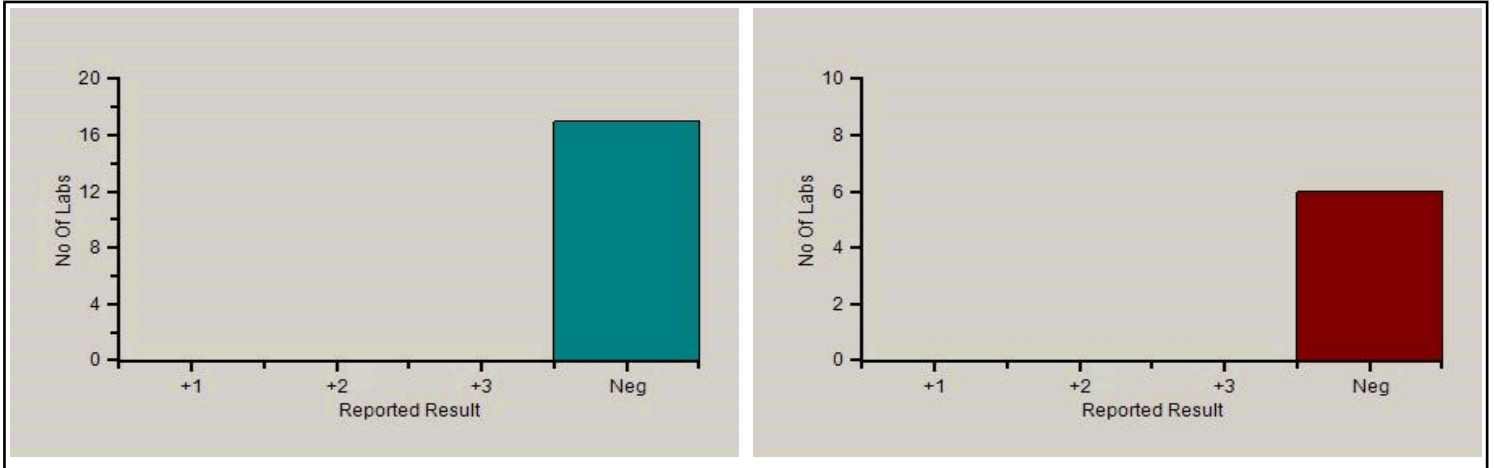

**Reported Results Legends :-**

+1	: 1+
+2	: 2+
+3	: 3+
Neg	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error



**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022


**Clinical Path - Urine Routine Chemistry,Blood (urine), -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	232
<span style="color: teal;">■</span> Photoelectric colorimetry - (Your Method)	19
<span style="color: red;">■</span> Urometer 120 - (Your Analyzer)	6

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	2+
<b>Result Expected</b>	+1,+2,Tr

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

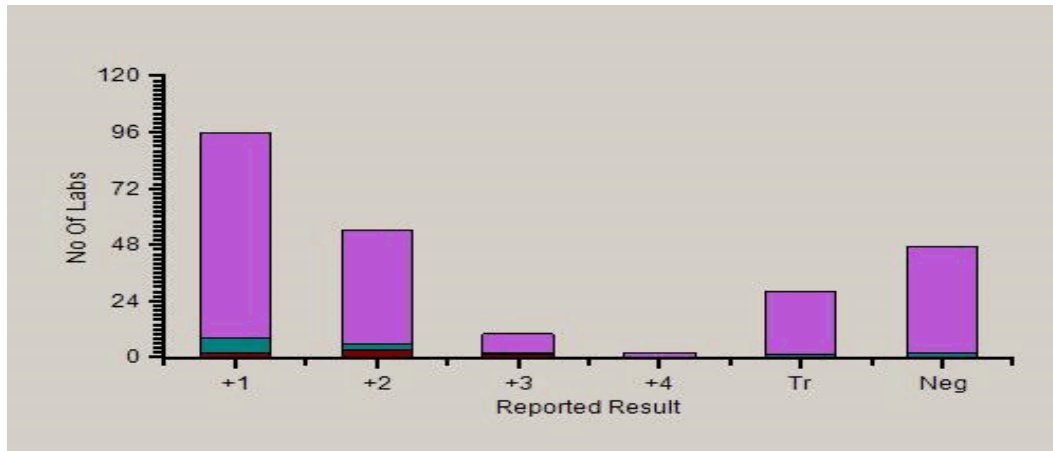


PC-1022

**Analyte Methodwise Qualitative Result Report**

**Lab No.:** 596  
**Lab Name :** HEALTH HORIZON DIAGNOSTICS  
**Report Date :** 25/01/2023

**Cycle No :** 220412  
**Sample No :** 1  
**Sample Date :** 27-12-2022

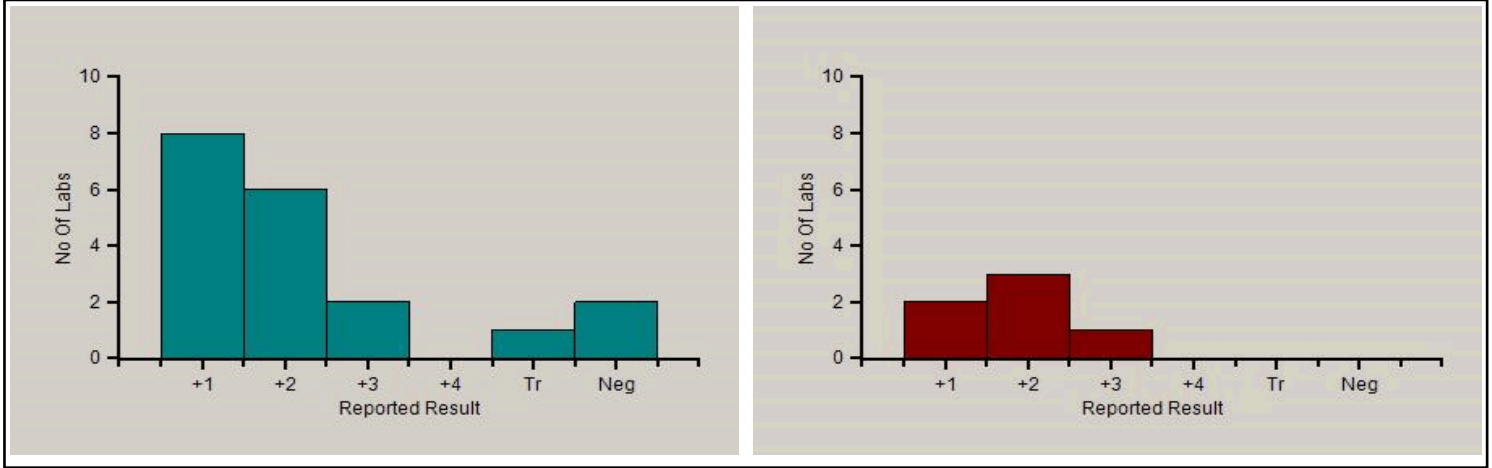

**Reported Results Legends :-**

+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+
Tr	: Trace
Neg	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance. Review for systematic error



**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022


**Clinical Path - Urine Routine Chemistry,Glucose (urine), -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	238
<span style="color: teal;">■</span> Photoelectric colorimetry - (Your Method)	17
<span style="color: red;">■</span> Urometer 120 - (Your Analyzer)	6

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	3+
<b>Result Expected</b>	+2,+3,+4

**Note :** # is an indication that this parameter has not been evaluated



Frequency Histogram

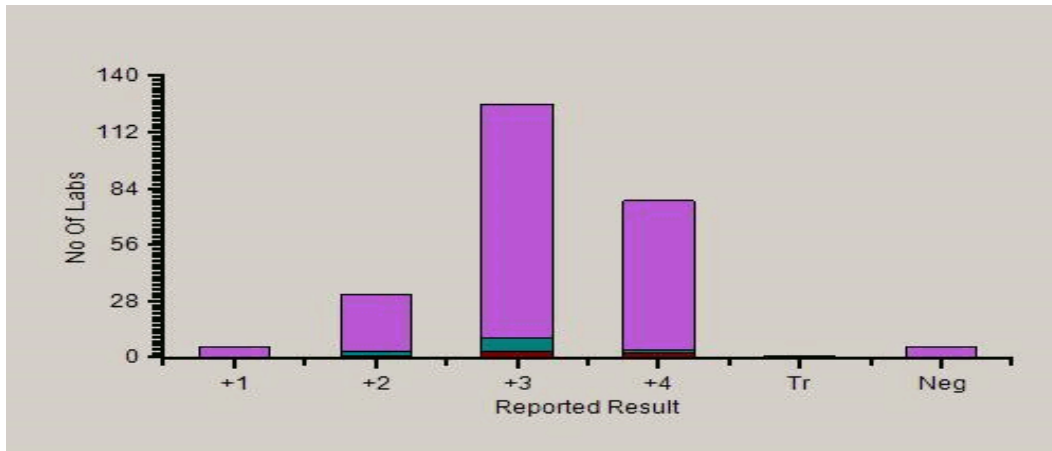

**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022

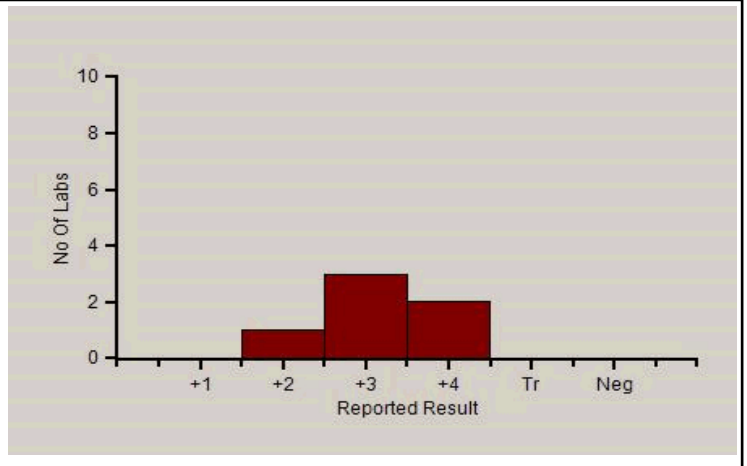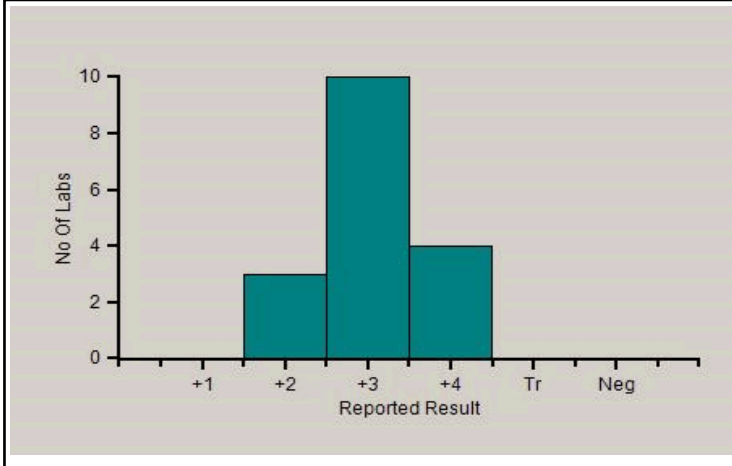

**Reported Results Legends :-**

+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+
Tr	: Trace
Neg	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance. Review for systematic error



**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022

**Clinical Path - Urine Routine Chemistry, Ketone (urine), -**


	<b>N</b>
<span style="color: purple;">■</span> All Methods	234
<span style="color: teal;">■</span> Photoelectric colorimetry - (Your Method)	18
<span style="color: red;">■</span> Urometer 120 - (Your Analyzer)	6

**Evaluation Based On - Method wise Peer Grouping**

<b>Your Result</b>	Negative
<b>Result Expected</b>	Neg, Tr

**Note :** # is an indication that this parameter has not been evaluated


Frequency Histogram

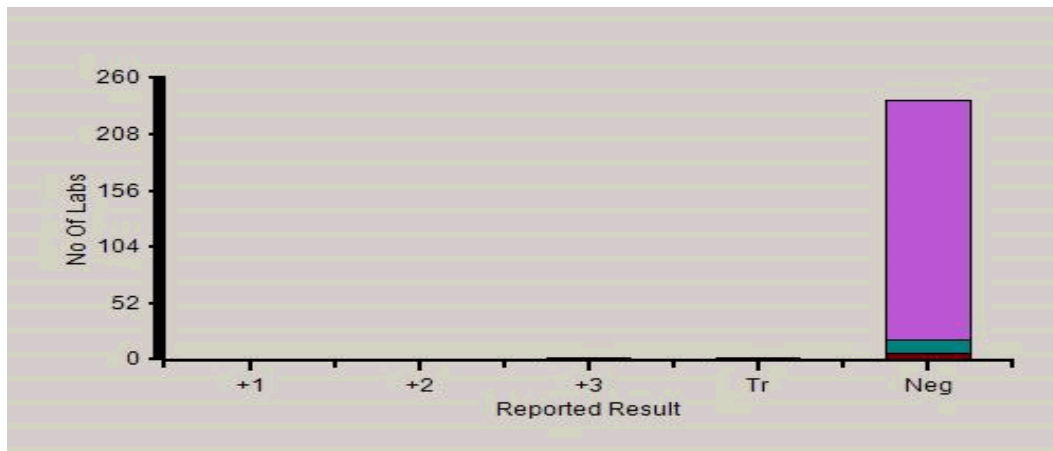

**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022

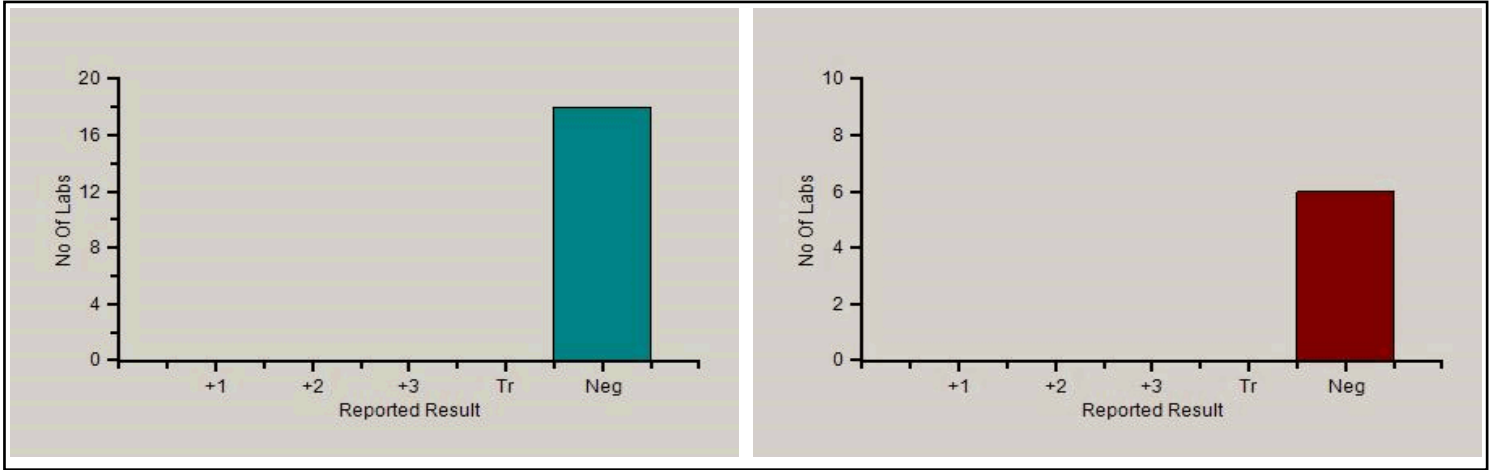

**Reported Results Legends :-**

+1	: 1+
+2	: 2+
+3	: 3+
Tr	: Trace
Neg	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
- Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
- All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance. Review for systematic error





**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022


**Clinical Path - Urine Routine Chemistry,Nitrite (urine), -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	233
<span style="color: teal;">■</span> Photoelectric colorimetry - (Your Method)	19
<span style="color: red;">■</span> Urometer 120 - (Your Analyzer)	6

Evaluation Based On - Method wise Peer Grouping	
Your Result	Absent
Result Expected	Abs

**Note :** # is an indication that this parameter has not been evaluated


Frequency Histogram

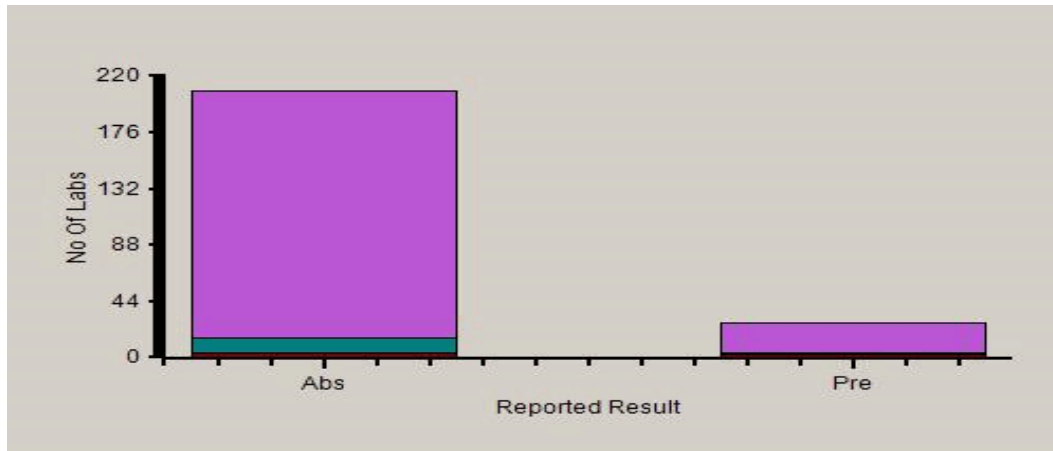

**Analyte Methodwise Qualitative Result Report**

**Lab No.:** 596  
**Lab Name :** HEALTH HORIZON DIAGNOSTICS  
**Report Date :** 25/01/2023

**Cycle No :** 220412  
**Sample No :** 1  
**Sample Date :** 27-12-2022

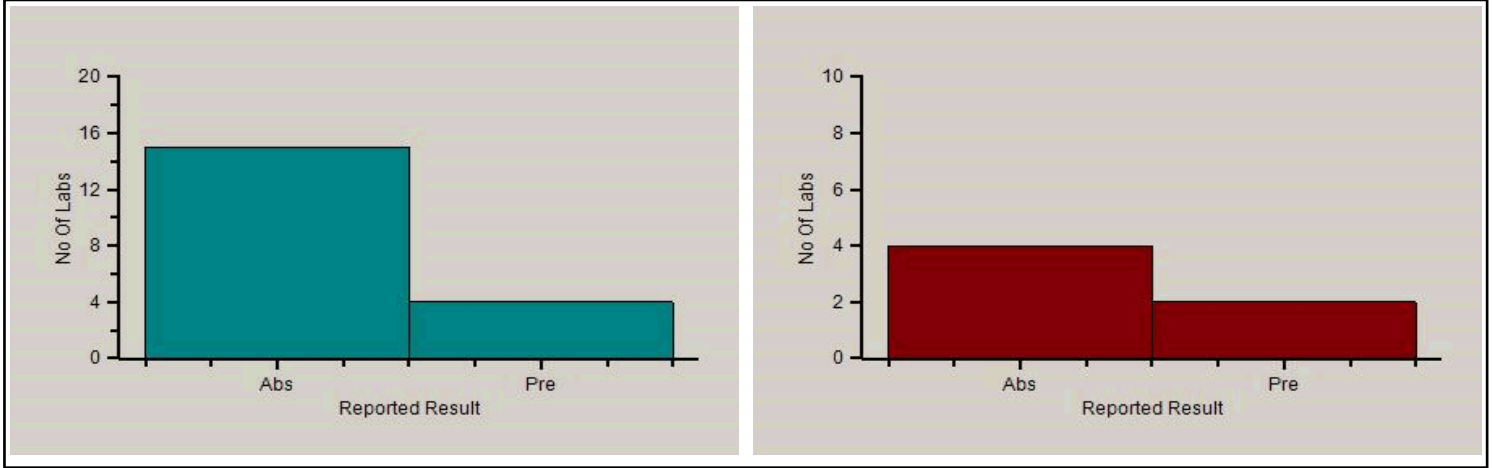

**Reported Results Legends :-**  
 Abs : Absent  
 Pre : Present

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance. Review for systematic error

**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022


**Clinical Path - Urine Routine Chemistry,pH, -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	236
<span style="color: teal;">■</span> Photoelectric colorimetry - (Your Method)	17
<span style="color: red;">■</span> Urometer 120 - (Your Analyzer)	6

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	6.5
<b>Result Expected</b>	6,6.5,7

**Note** : # is an indication that this parameter has not been evaluated


Frequency Histogram

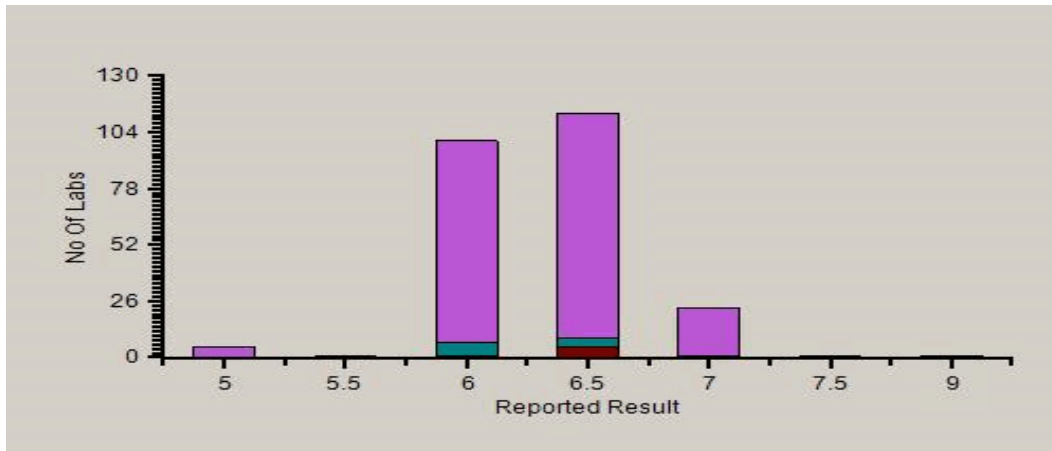

**Analyte Methodwise Qualitative Result Report**

**Lab No.:** 596  
**Lab Name :** HEALTH HORIZON DIAGNOSTICS  
**Report Date :** 25/01/2023

**Cycle No :** 220412  
**Sample No :** 1  
**Sample Date :** 27-12-2022

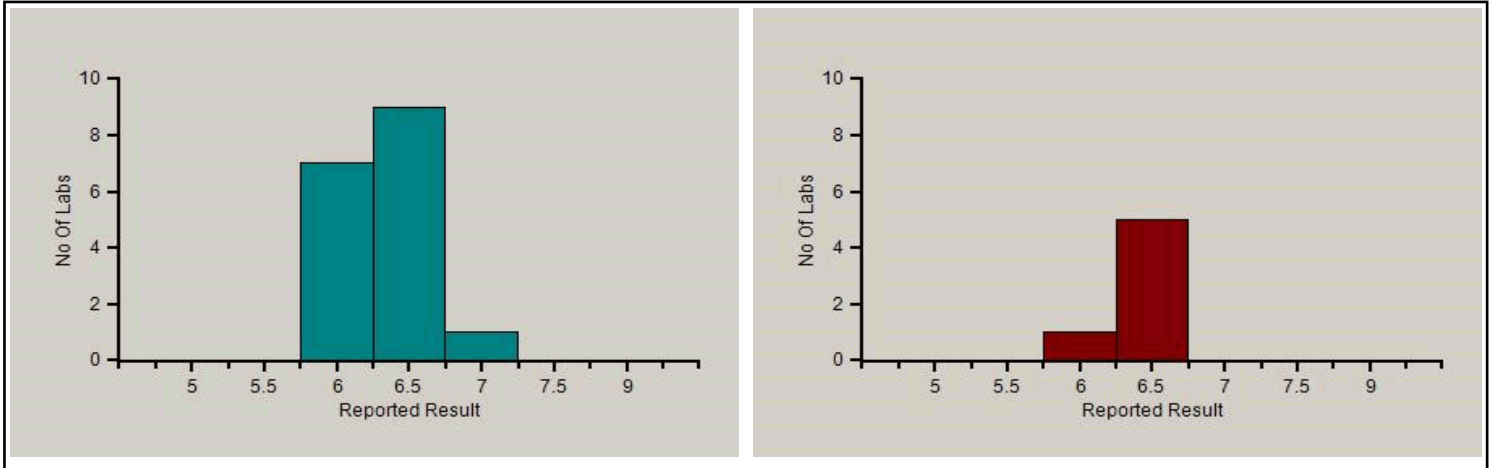

**Reported Results Legends :-**

5	: 5
5.5	: 5.5
6	: 6
6.5	: 6.5
7	: 7
7.5	: 7.5
8	: 8
8.5	: 8.5
9	: 9

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error



**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022


**Clinical Path - Urine Routine Chemistry,Protein (Urine), -**

<span style="color: purple;">■</span> All Methods	N
<span style="color: teal;">■</span> Photoelectric colorimetry - (Your Method)	238
<span style="color: red;">■</span> Urometer 120 - (Your Analyzer)	19
	6

Evaluation Based On - Method wise Peer Grouping	
Your Result	Trace
Result Expected	+1,Neg,Tr

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram


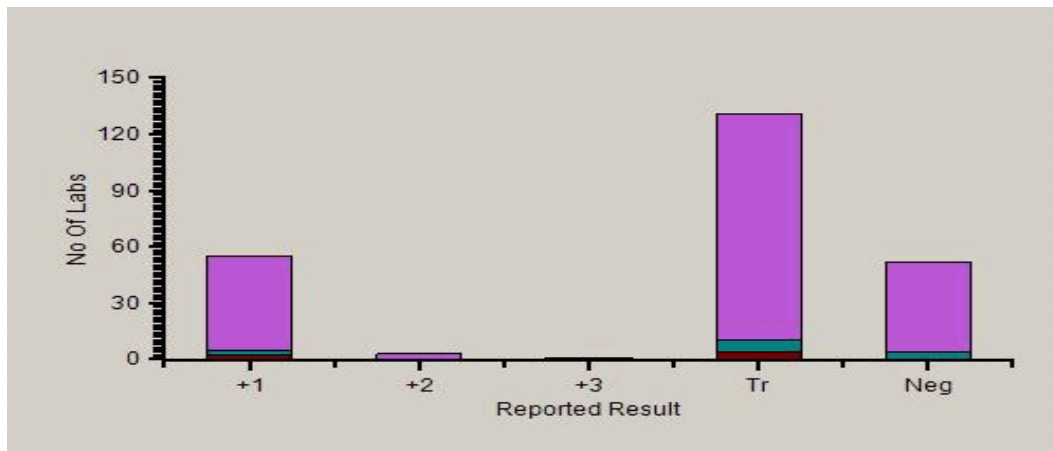


PC-1022

**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022

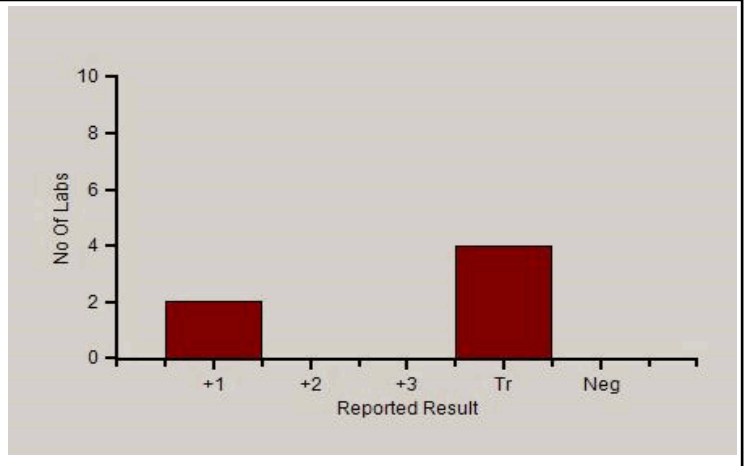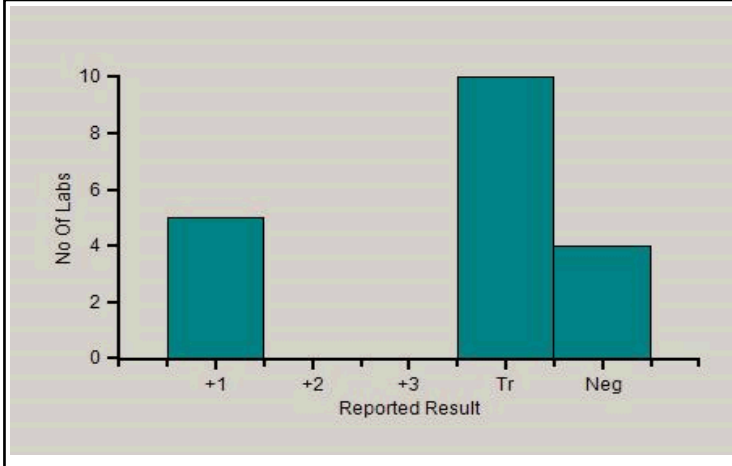

**Reported Results Legends :-**

+1	: 1+
+2	: 2+
+3	: 3+
Tr	: Trace
Neg	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance. Review for systematic error



**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022


**Clinical Path - Urine Routine Chemistry, Specific Gravity, -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	235
<span style="color: teal;">■</span> Photoelectric colorimetry - (Your Method)	17
<span style="color: red;">■</span> Urometer 120 - (Your Analyzer)	6

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	1.020
<b>Result Expected</b>	1.010,1.015,1.020

**Note :** # is an indication that this parameter has not been evaluated


Frequency Histogram

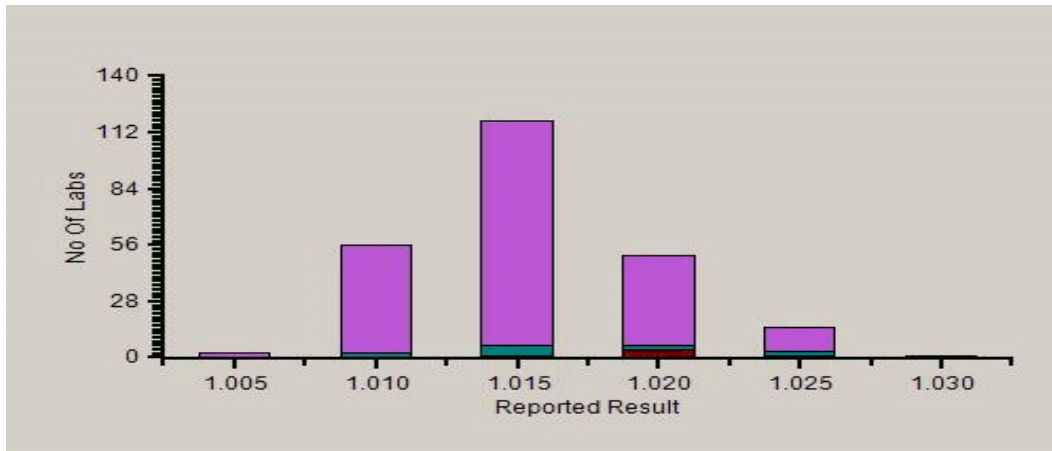

**Analyte Methodwise Qualitative Result Report**

**Lab No.:** 596  
**Lab Name :** HEALTH HORIZON DIAGNOSTICS  
**Report Date :** 25/01/2023

**Cycle No :** 220412  
**Sample No :** 1  
**Sample Date :** 27-12-2022

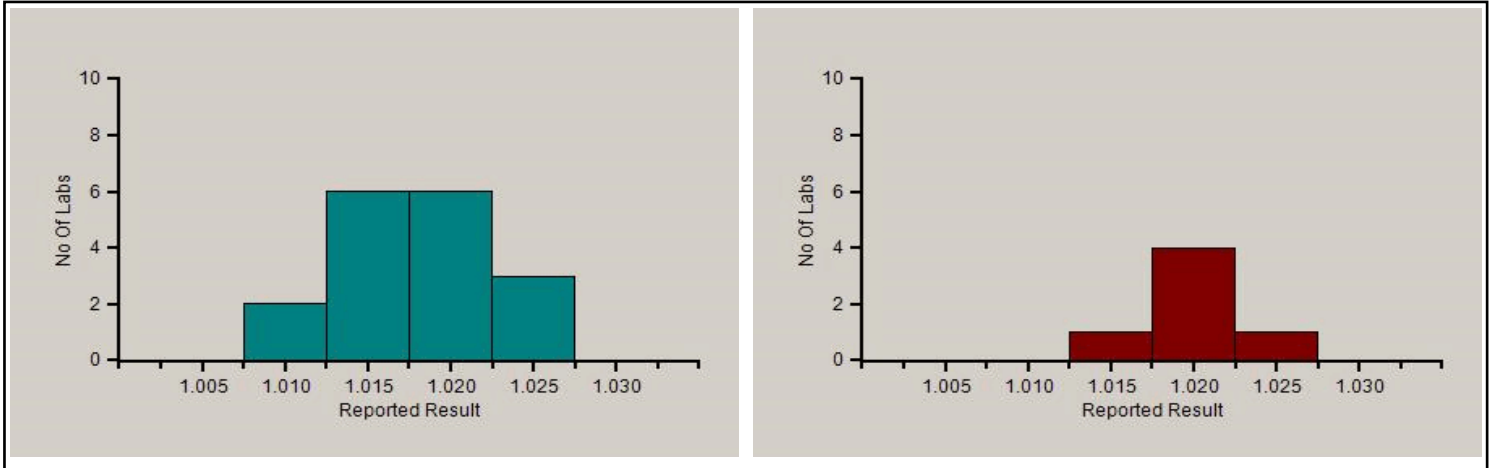

**Reported Results Legends :-**

1.005	: 1.005
1.010	: 1.010
1.015	: 1.015
1.020	: 1.020
1.025	: 1.025
1.030	: 1.030
1.035	: 1.035

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance. Review for systematic error





**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
 Lab Name : HEALTH HORIZON DIAGNOSTICS  
 Report Date : 25/01/2023

Cycle No : 220412  
 Sample No : 1  
 Sample Date : 27-12-2022


**Clinical Path - Urine Routine Chemistry,Urobilinogen (urine), -**

	<b>N</b>
<span style="color: purple;">■</span> All Methods	223
<span style="color: teal;">■</span> Photoelectric colorimetry - (Your Method)	16
<span style="color: red;">■</span> Urometer 120 - (Your Analyzer)	6

Evaluation Based On - Method wise Peer Grouping	
Your Result	Normal
Result Expected	Nor

**Note :** # is an indication that this parameter has not been evaluated



Frequency Histogram

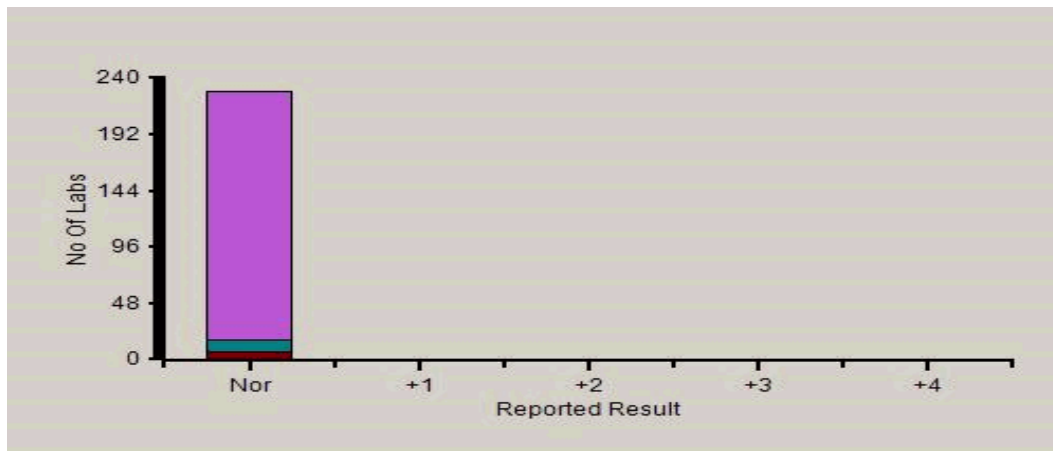

**Analyte Methodwise Qualitative Result Report**

Lab No.: 596  
Lab Name : HEALTH HORIZON DIAGNOSTICS  
Report Date : 25/01/2023

Cycle No : 220412  
Sample No : 1  
Sample Date : 27-12-2022

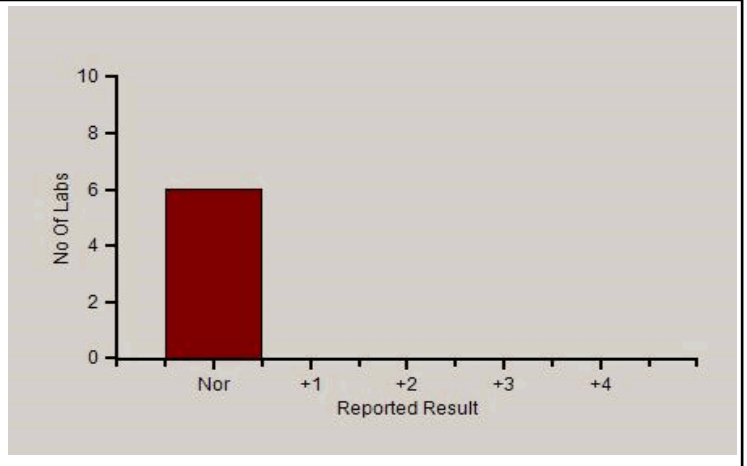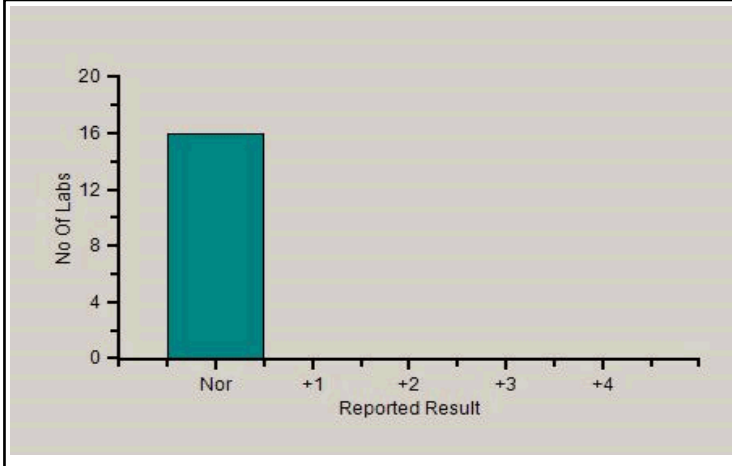

**Reported Results Legends :-**

Nor	: Normal
+1	: 1+
+2	: 2+
+3	: 3+
+4	: 4+

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance. Review for systematic error

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
Unit No. 409-416.  
Commercial Building - 1A,  
Kohinoor Mall, Kiroi Road, Kurla (W),  
Mumbai - 400070

