

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 1
 Sample Date : 27-12-2022


Immunoassay Extended,HBsAg, Nil

	N
■ All Methods	179
■ Immunochromatography - (Your Method)	119
■ Manual - (Your Analyzer)	104

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 1
 Sample Date : 27-12-2022

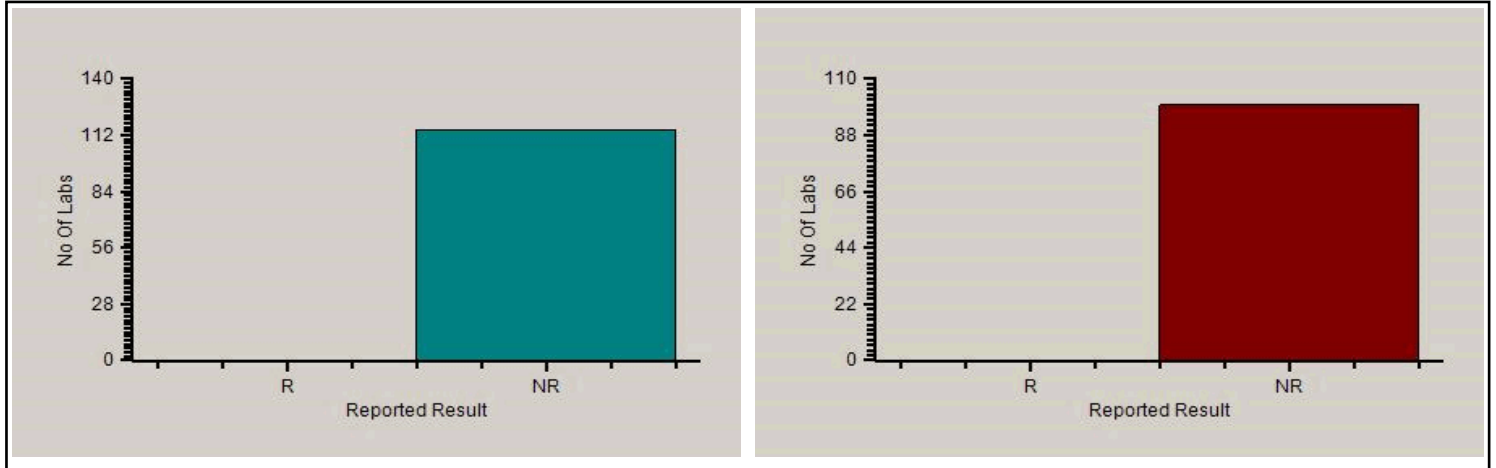

Reported Results Legends :-

- R : Reactive
- NR : Non-reactive
- Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 1
 Sample Date : 27-12-2022


Immunoassay Extended,HCV, -

	N
■ All Methods	159
■ Immunochromatography - (Your Method)	107
■ Manual - (Your Analyzer)	98

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 1
 Sample Date : 27-12-2022



Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 1
 Sample Date : 27-12-2022


Immunoassay Extended,HIV Ab, -

	N
■ All Methods	108
■ Immunochromatography - (Your Method)	96
■ Manual - (Your Analyzer)	93

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram




PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : HEALTH HORIZON DIAGNOSTICS
Report Date : 25/01/2023

Cycle No : 220412
Sample No : 1
Sample Date : 27-12-2022



Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
Eq	: Equivocal
Indet	: Indeterminate
HIV-1	: HIV-1 Ab Reactive
HIV-2	: HIV-2 Ab Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 1
 Sample Date : 27-12-2022


Immunoassay Extended,RPR (Syphilis Serology), -

	N
■ All Methods	150
■ Agglutination - (Your Method)	56
■ Manual - (Your Analyzer)	154

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram



Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : HEALTH HORIZON DIAGNOSTICS
Report Date : 25/01/2023

Cycle No : 220412
Sample No : 1
Sample Date : 27-12-2022

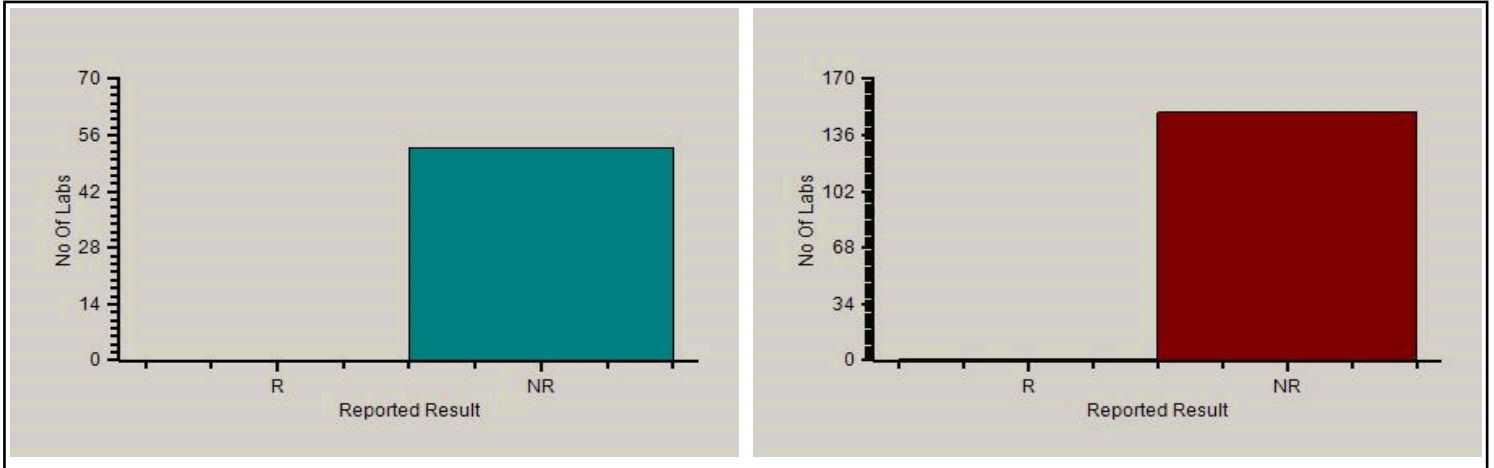

Reported Results Legends :-

R : Reactive
NR : Non-reactive
WR : Weak Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416.
Commercial Building - 1A,
Kohinoor Mall, Kiroi Road, Kurla (W),
Mumbai - 400070



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 2
 Sample Date : 27-12-2022


Immunoassay Extended,HBsAg, Nil

	N
■ All Methods	174
■ Immunochromatography - (Your Method)	115
■ Manual - (Your Analyzer)	101

Your Result	Reactive
Result Expected	R

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram



Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : HEALTH HORIZON DIAGNOSTICS
Report Date : 25/01/2023

Cycle No : 220412
Sample No : 2
Sample Date : 27-12-2022



Reported Results Legends :-

- R : Reactive
- NR : Non-reactive
- Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 2
 Sample Date : 27-12-2022

Immunoassay Extended,HCV, -


■ All Methods	N
■ Immunochromatography - (Your Method)	154
■ Manual - (Your Analyzer)	102
	94

Your Result Reactive

Result Expected #

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram



Analyte Methodwise Qualitative Result Report

Lab No.: 596
Lab Name : HEALTH HORIZON DIAGNOSTICS
Report Date : 25/01/2023

Cycle No : 220412
Sample No : 2
Sample Date : 27-12-2022



Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 Eq : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 2
 Sample Date : 27-12-2022


Immunoassay Extended,HIV Ab, -

	All Methods	N
	Immunochromatography - (Your Method)	98
	Manual - (Your Analyzer)	91
		89

Your Result	HIV-1 Ab Reactive
Result Expected	HIV-1

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram





PC-1022

Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 2
 Sample Date : 27-12-2022

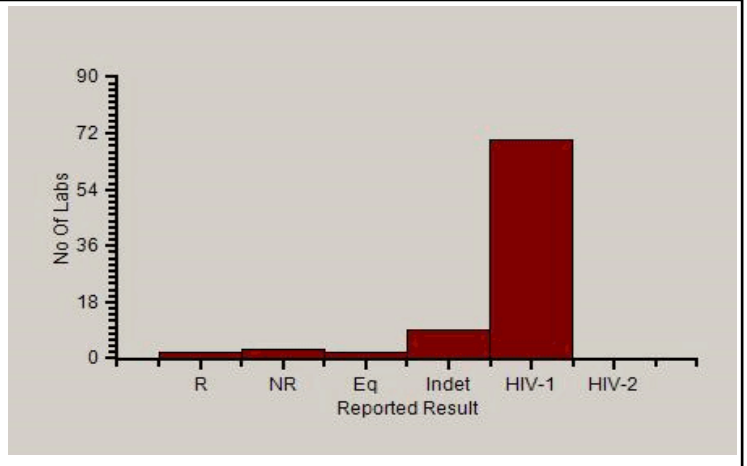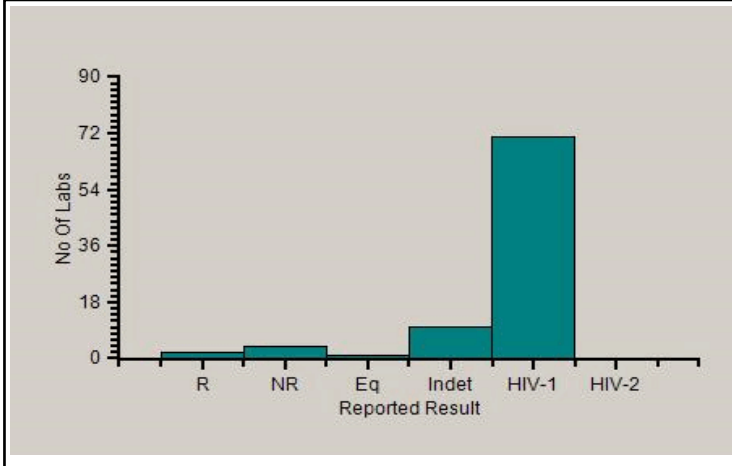

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
Eq	: Equivocal
Indet	: Indeterminate
HIV-1	: HIV-1 Ab Reactive
HIV-2	: HIV-2 Ab Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance. Review for systematic error



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 2
 Sample Date : 27-12-2022


Immunoassay Extended,RPR (Syphilis Serology), -

	N
■ All Methods	150
■ Agglutination - (Your Method)	57
■ Manual - (Your Analyzer)	155

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated


Frequency Histogram



Analyte Methodwise Qualitative Result Report

Lab No.: 596
 Lab Name : HEALTH HORIZON DIAGNOSTICS
 Report Date : 25/01/2023

Cycle No : 220412
 Sample No : 2
 Sample Date : 27-12-2022



Reported Results Legends :-

R : Reactive
 NR : Non-reactive
 WR : Weak Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr. Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A,
 Kohinoor Mall, Kiroi Road, Kurla (W),
 Mumbai - 400070

