



COMMITTED TO THE
CUSTOMER SINCE - 1996

Vaidyanatheshwara INSTRUMENTS



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com



NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page 1 of 2

1 Name and Address of the Customer

M/s: Acharya Tulsi Diagnostic Centre and Dental Care,
#228/12, MSP Plaza, Magadi Road,
(Near Magadi Road Metro Station), Bangalore - 560 203.

2 Customer Reference

- 2.1 ULR No. : CC247322500043070F
- 2.2 SRF No : 2125
- 2.3 Certificate No. : VI/22-23/2125-02
- 2.4 Format No. : VI-FRM-ME-046 & VI-FRM-ET-011
- 2.5 Date of issue : 21-11-2022

3 Details Of Device Under Calibration(DUC).

- 3.1 Nomenclature : Centrifuge
- 3.2 Make / Model : Remi / R-8C
- 3.3 SI.No. / Id.No. : ATDC/CF-01
- 3.4 DUC Condition : Satisfactory
- 3.5 Calibration Procedure No. : SOP-16-42 & SOP-37-11
- 3.6 No.of Pages : 2
- 3.7 Calibration Date : 17-11-2022
- 3.8 Calibration Due : 16-11-2023
- 3.9 Calibration done at : Onsite
- 3.10 Instrument Location : Laboratory
- 3.11 Discipline : Mechanical & Electro-Technical

4 Environmental Condition

Temperature 24.3 °C Humidity 53 %RH

5 Standards Used for calibration

Sl. No.	Nomenclature	Make & Model	Sl. No.	Cal Agency	Certificate No.	Validity
1	Time Totalizer	Beltronics & 501	251	VI, Bangalore	VI/21-22/INT-ETH-426	22-02-2023
2	Digital Tachometer	SENTRY / ST723	SN1323004225	Sansel Lab Chennai	CC287922000003276F	16-08-2023

6 Notes:

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab.
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7. The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

Vinay
Vinay

(Calibration Engineer)

Checked By

Guruprasad S C
Guruprasad S C

(Lab In-Charge)





COMMITTED TO THE
CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com



NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No.

VI/22-23/2125-02

Page No: 2 of 2

Results: Timer

Range: 0 to 99 min

Resolution: 1 min

Sl. No.	Std Reading (hr:min:sec:msec)	DUC Reading (min)	Error Observed (hr:min:sec:msec)	Measurement Uncertainty in (±) (%)	k Factor
1	00:00:00:000	0	00:00:00:000	--	--
2	00:10:00:018	10	-00:00:00:018	0.05	2.0
3	00:30:00:029	30	-00:00:00:029	0.05	2.0
4	01:00:00:036	60	-00:00:00:036	0.05	2.0
5	01:30:00:052	90	-00:00:00:052	0.05	2.0
6	02:00:50:068	120	-00:00:00:068	0.05	2.0
7	02:30:65:075	150	-00:00:00:075	0.05	2.0

Results: RPM

Range : 0 to 5500 RPM

Resolution: 10 RPM

Sl. No.	Range.	DUC Reading (RPM)	STD Reading (RPM)	Error Observed (RPM)	Measurement Uncertainty in (±) (%)	k Factor
1	0 to 5500 RPM	500	500.5	-0.5	1.2	2.0
2		1000	1000.8	-0.8	1.2	2.0
3		2000	2001.2	-1.2	1.2	2.0
4		3000	3001.5	-1.5	1.2	2.0
5		4000	4002.0	-2.0	1.2	2.0
5		5500	5502.7	-2.7	1.2	2.0

Conclusion :-

- Measurement uncertainty reported is at 95.45 % confidence level.

Calibrated By

Vinay

Vinay

(Calibration Engineer)

Checked By

Guruprasad S C

Guruprasad S C
(Lab In-Charge)





COMMITTED TO THE
CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nanahani Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9886586789 / 9832221171 / 9964308118 | Email : info@vipgroup.com Web : www.vipgroup.com



NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of the Customer

M/s: Acharya Tuls Diagnostic Centre and Dental Care,
#228/12, MSP Plaza, Magadi Road,
(Near Magadi Road Metro Station), Bangalore - 560 203.

2 Customer Reference

- 2.1 ULR No. : CC247322500043071F
- 2.2 SRF No : 2125
- 2.3 Certificate No. : VI/22-23/2125-03
- 2.4 Format No. : VI-FRM-ME-046 & VI-FRM-ET-011
- 2.5 Date of issue : 21-11-2022

3 Details Of Device Under Calibration(DUC),

- 3.1 Nomenclature : Centrifuge
- 3.2 Make / Model : Remi / R-8C
- 3.3 SI.No. / Id.No. : ATDC/CF-02
- 3.4 DUC Condition : Satisfactory
- 3.5 Calibration Procedure No. : SOP-16-42 & SOP-37-11
- 3.6 No.of Pages : 2
- 3.7 Calibration Date : 17-11-2022
- 3.8 Calibration Due : 16-11-2023
- 3.9 Calibration done at : Onsite
- 3.10 Instrument Location : Laboratory
- 3.11 Discipline : Mechanical & Electro-Technical

4 Environmental Condition

Temperature 24.3 °C Humidity 53 %RH

5 Standards Used for calibration


Sl. No.	Nomenclature	Make & Model	Sl. No.	Cal Agency	Certificate No.	Validity
1	Time Totalizer	Beltronics & 501	251	VI, Bangalore	VI/21-22/INT-ETH-426	22-02-2023
2	Digital Tachometer	SENTRY / ST723	SN1323004225	Sansel Lab Chennai	CC287922000003276F	16-08-2023

6 Notes:

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab.
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7. The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By
Vinay
Vinay
(Calibration Engineer)

Checked By
Guruprasad S C
Guruprasad S C
(Lab In-Charge)



This report refers only to the item/gauge submitted and may not be reproduced except in full without written permission from Vaidyanatheshwara Instruments Bangalore - 560096.

This report refers only to the item/gauge submitted and may not be reproduced except in full without written permission from Vaidyanatheshwara Instruments Bangalore - 560096.

CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com



NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. **VII/22-23/2125-03**

Page No: 2 of 2

Results: Timer

Range: 0 to 99 min

Resolution: 1 min

Sl. No.	Std Reading (hr:min:sec:msec)	DUC Reading (min)	Error Observed (hr:min:sec:msec)	Measurement Uncertainty in (±) (%)	k Factor
1	00:00:00:000	0	00:00:00:000	--	--
2	00:10:00:015	10	-00:00:00:015	0.05	2.0
3	00:30:00:032	30	-00:00:00:032	0.05	2.0
4	01:00:00:045	60	-00:00:00:045	0.05	2.0
5	01:30:00:058	90	-00:00:00:058	0.05	2.0
6	02:00:50:072	120	-00:00:00:072	0.05	2.0
7	02:30:65:083	150	-00:00:00:083	0.05	2.0

Results: RPM

Range : 0 to 5500 RPM

Resolution: 10 RPM

Sl. No.	Range.	DUC Reading (RPM)	STD Reading (RPM)	Error Observed (RPM)	Measurement Uncertainty in (±) (%)	k Factor
1	0 to 5500 RPM	500	500.7	-0.7	1.2	2.0
2		1000	1001.0	-1.0	1.2	2.0
3		2000	2001.6	-1.6	1.2	2.0
4		3000	3002.3	-2.3	1.2	2.0
5		4000	4002.8	-2.8	1.2	2.0
5		5500	5503.5	-3.5	1.2	2.0

Conclusion :-

1. Measurement uncertainty reported is at 95.45 % confidence level.

Calibrated By

Vinay
Vinay

(Calibration Engineer)

Checked By

Guruprasad S C
Guruprasad S C
(Lab In-Charge)





COMMITTED TO THE
CUSTOMER SINCE - 1996

Vaidyanatheshwara INSTRUMENTS



CERTIFICATE OF CALIBRATION

CC-2473



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of the Customer

M/s.: Acharya Tulsi Diagnostic Centre and Dental Care,
#228/12, MSP Plaza, Magadi Road,
(Near Magadi Road Metro Station), Bangalore - 560 203.

2 Customer Reference

- 2.1 ULR No. : CC247322500043069F
- 2.2 SRF No. : 2125
- 2.3 Certificate No. : VI/22-23/2125-01
- 2.4 Format No. : VI-FRM-TH-006
- 2.5 Date of Issue : 21-11-2022

3 Details Of Device Under Calibration(DUC).

- 3.1 Nomenclature : Refrigerator
- 3.2 Make / Model : Frost Free Godrej / RT EON 245B
- 3.3 Id.No. : ATDC/REF-01
- 3.4 Range : 2 to 8 °C
- 3.5 DUC Condition : Satisfactory
- 3.6 Calibration Procedure No. : SOP-38-06
- 3.7 No.of Pages : 2
- 3.8 Calibration Date : 17-11-2022
- 3.9 Calibration Due : 16-11-2023
- 3.10 Calibration done at : Onsite
- 3.11 Instrument Location : Laboratory
- 3.12 Discipline : Thermal

4 Environmental Condition

Temperature 23.1 °C

Humidity 52 %RH

5 Standards Used for Temperature Calibration

Sl. No.	Nomenclature	Make / Model	Id. No.	Cal Agency	Certificate. No.	Validity
1	Paperless Recorder	Brain Child & VR-18	VI/OS/PR-04	VI, Bangalore	VI/21-22/INT-56-01	30-12-2022
2	RTD Sensor	Frontier & ----	VI-RTD-01	VI, Bangalore	VI/22-23/INT-TH-100-001	17-02-2023

6 Note:

- 6.1.The Calibration Certificate relates only to the above DUC
- 6.2.Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI.
- 6.3.Corrections/erasing, invalidate the Calibration Certificate.
- 6.4.Calibration of the DUC are traceable to National standards/International Standards
- 6.5.Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6.Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7.The usage of NABL Symbol is as per NABL guidelines given in NABL-133

Calibrated By

Vinay
Vinay

(Calibration Engineer)

Checked By

Guruprasad S.e
Guruprasad S.e
(Lab In-Charge)





COMMITTED TO THE CUSTOMER SINCE - 1996

Vaidyanatheshwara INSTRUMENTS



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com



NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No. VI/22-23/2125-01


Page: 2 of 2

Results:

Range : 2 to 8 °C

Sl. No.	STD Reading (°C)	DUC Reading (°C)	Error Observed (°C)	Measurement Uncertainty ± (°C)	k Factor
1	2.0	2.0	0.0	0.95	2.0
2	3.0	3.0	0.0	0.95	2.0
3	4.0	4.0	0.0	0.95	2.0
4	5.9	6.0	0.1	0.95	2.0
5	7.9	8.0	0.1	0.95	2.0

Pictorial Representation of Sensors Placement

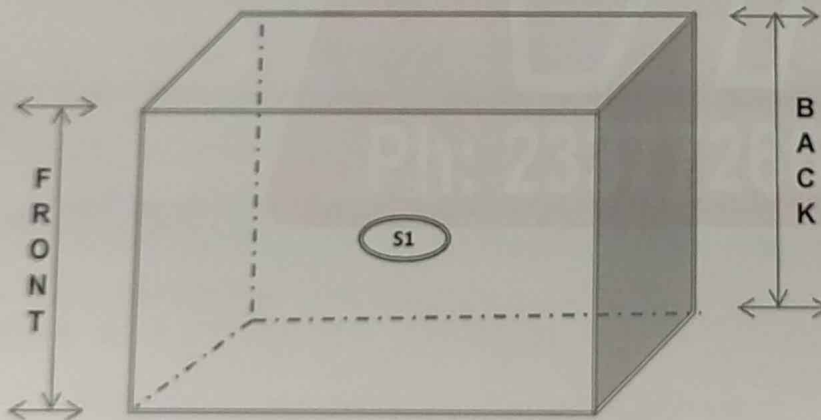

Note :

1. S1 Indicates Placement of Standard Sensor

Conclusion / Remarks:

- 1 Measurement Uncertainty reported is at 95.45% confidence level with $k = 2$.

Calibrated By

Vinay
Vinay

(Calibration Engineer)

Checked By

Guruprasad S.C
Guruprasad S.C

(Lab In-Charge)



CALIBRATION CERTIFICATE

SANS/FT/01(7.8/01)	Page No : 1 of 2
Certificate/ULR No : CC287922000003276F	Date of issue : 19.08.2022
Date of Calibration : 17.08.2022	Due date : 16.08.2023

Customer Details:

M/s.VAIDYANATHESHWARA INSTRUMENTS	SRF No	: 15057
No.301/A, 9 th Main Road, 3rd Cross, Rajiv Gandhi Nagar,	Date of Receipt	: 16.08.2022
J.B. Kaval, Nandhini Layout Post,	Cond of Receipt	: Satisfactory
Bangalore-560 096.	Calibrated at	: LAB

Details of UUC

Instrument Name	: Digital Tachometer (Contact) & (Non - Contact)		
Make	: SENTRY		
Model	: ST723		
S.No	: SN1323004225	ID No.	: VIME/DT/01
Cal . Range	: 100 to 8000 rpm (Contact) & 12 to 90000 rpm (Non- Contact)		
Resolution	: 0.1/1 rpm		
Accuracy	: ---		

Environmental Details	Method of Calibration	Work Instruction : SANS/M/L-02
Ambient Temperature : 24.1°C	Comparison Method	Discipline : Mechanical
Relative Humidity : 50.3%RH		Group : Acceleration and Speed

Details of Standards Used

Nomenclature	SI.No	Certificate No	Validity	Traceability
Digital Tachometer	109-0591V	HT/CC/210916-20/001	15.09.2022	National Standard
Digital Tachometer	168-0093	FCRI/EQL/21-22/219	25.10.2022	National standard
RPM Source	RPMC11160798	---	---	---

Mohammed Nazeem

S.Mohammed Nazeem
Calibration Engineer



Anand.B

Authorised Signatory





Vaidyanatheshwara INSTRUMENTS



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
 Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@vipgroup.com Web : www.vipgroup.com



NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of the Customer : M/s. ACHARYA TULSI® DENTAL CARE & DIAGNOSTIC CENTRE
 #25, JP Arcade , 8th Main , Binny Layout , 1st Stage ,
 Vijayanagar ,Bangalore -40,

2 Customer Reference
 2.1 ULR No : CC247322100020680F
 2.2 SRF No : 5099
 2.3 Certificate No. : VI/22-23/5099-02
 2.4 Format No. : VI-FRM-ME-105
 2.5 Receipt Date : 18-11-2022
 2.6 DC No. / DC Date : -- & 17-11-2022
 2.7 Date Of Issue : 21-11-2022

3 Details Of Device Under Calibration(DUC).
 3.1 Nomenclature : MicroPipette
 3.2 Make/Model : Biohit/Proline
 3.3 Range : 100 - 1000 µl
 3.4 Sl.No. : 11514898
 3.5 DUC Condition : Satisfactory
 3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
 3.7 No.of Pages : 2
 3.8 Calibration Date : 21-11-2022
 3.9 Calibration Due : 20-11-2023
 3.10 Calibration done at : VI Volumetric Lab
 3.11 Discipline : Mechanical (Mass & volume)

4 Environmental Condition
 Temperature 20.4 °C Humidity 51 %Rh

5 Standards Used for calibration

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/22-23/INT-ME-121	15-09-2023
2	E1 Class Weights	LCGC	VI-E1-ME-001	200g to 1mg	TVCSPL22/03/527-01	30 - 03 - 2025

- 6 Note:**
- The Calibration Certificate relates only to the above DUC
 - Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
 - Corrections/erasing, invalidate the Calibration Certificate.
 - Calibration of the DUC are traceable to National standards/International Standards
 - Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
 - Results Reported are valid at the time of and under the stated conditions of measurements.
 - The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By

Checked By

Ranjith Kumar P
 (Calibration Engineer)

P. Santhosh Kumar
 (Lab- In-Charge)





CERTIFICATE OF CALIBRATION

CC-2473



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.

Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/22-23/5099-02

Page 2 of 2

Range: 100 - 1000 μ l

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty \pm
	μ l	μ l	μ l
100 - 1000 μ l	100	100.784	0.62
	500	500.937	3.10
	1000	1001.751	6.20

Note:

1. Visual Inspection : Found Well.
2. Tripple Distilled water is used to Calibrate the MicroPipette.

Conclusion /Remarks:

1. Ref. standard used are traceable to National/International Standard.
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Checked By

Ranjith kumar P
(Calibration Engineer)

P. Santhosh Kumar
(Lab- In-Charge)





CERTIFICATE OF CALIBRATION



COMMITTED TO THE CUSTOMER SINCE - 1996

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com



NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

1 Name and Address of the Customer : M/s. ACHARYA TULSI* DENTAL CARE & DIAGNOSTIC CENTRE
#25, JP Arcade , 8th Main , Binny Layout , 1st Stage ,
Vijayanagar ,Bangalore -40.

2 Customer Reference

2.1 ULR No : CC247322100020682F
2.2 SRF No : 5099
2.3 Certificate No. : VI/22-23/5099-04
2.4 Format No. : VI-FRM-ME-105
2.5 Receipt Date : 18-11-2022
2.6 DC No. / DC Date : -- & 17-11-2022
2.7 Date Of Issue : 21-11-2022

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : MicroPipette
3.2 Make/Model : Vertex
3.3 Range : 500 µl
3.4 SLNo . : 041801873
3.5 DUC Condition : Satisfactory
3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
3.7 No.of Pages : 2
3.8 Calibration Date : 21-11-2022
3.9 Calibration Due : 20-11-2023
3.10 Calibration done at : VI Volumetric Lab
3.11 Discipline : Mechanical (Mass & volume)

4 Environmental Condition

Temperature 20.4 °C Humidity 51 %Rh

5 Standards Used for calibration

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/22-23/INT-ME-121	15-09-2023
2	E1 Class Weights	LCGC	VI-E1-ME-001	200g to 1mg	TVCSPL22/03/527-01	30 - 03 - 2025

6 Note:

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By

Ranjith Kumar P
(Calibration Engineer)

Checked By

P. Santhosh Kumar
(Lab- In-Charge)





COMMITTED TO THE CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com



NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/22-23/5099-04

Page 2 of 2

Range: 500 µl

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty ±
	µl	µl	µl
500 µl	500	492.754	3.10
	500	492.741	3.10
	500	492.759	3.10

Note:

1. Visual Inspection : Found Well.
2. Tripple Distilled water is used to Calibrate the MicroPipette.

Conclusion /Remarks:

1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Ranjith Kumar P
Ranjith Kumar P
(Calibration Engineer)

Checked By

P. Santhosh Kumar
P. Santhosh Kumar
(Lab- In-Charge)





COMMITTED TO THE
CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com



NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page 1 of 2

1 Name and Address of the Customer : M/s. ACHARYA TULSI* DENTAL CARE & DIAGNOSTIC CENTRE
#25, JP Arcade , 8th Main , Binny Layout , 1st Stage ,
Vijayanagar ,Bangalore -40,

2 Customer Reference

2.1 ULR No : CC247322100020679F
2.2 SRF No : 5099
2.3 Certificate No. : VI/22-23/5099-01
2.4 Format No. : VI-FRM-ME-105
2.5 Receipt Date : 18-11-2022
2.6 DC No. / DC Date : -- & 17-11-2022
2.7 Date Of Issue : 21-11-2022

3 Details Of Device Under Calibration(DUC).

3.1 Nomenclature : Micro Pipette
3.2 Make / Model : Biohit
3.3 Range : 20 - 200µl
3.4 SI.No. : YE4A246436
3.5 DUC Condition : Satisfactory
3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
3.7 No.of Pages : 2
3.8 Calibration Date : 21-11-2022
3.9 Calibration Due : 20-11-2023
3.10 Calibration done at : VI Volumetric Lab
3.11 Discipline : Mechanical (Mass & volume)

4 Environmental Condition

Temperature 20.3 °C Humidity 53 %Rh

5 Standards Used for calibration

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/22-23/INT-ME-121	15-09-2023
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSP22/03/527-01	30 - 03 - 2025

6 Note:

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By

Checked By

P. Ranjith kumar
(Calibration Engineer)

P. Santosh Kumar
(Lab- In-Charge)





COMMITTED TO THE
CUSTOMER SINCE - 1996

Vaidyanatheshwara INSTRUMENTS



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9988586789 / 9632221171 / 9964308118 | Email : info@vigiigroup.com Web : www.vigiigroup.com



NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page 1 of 2

1 Name and Address of the Customer : M/s. ACHARYA TULSI* DENTAL CARE & DIAGNOSTIC CENTRE
#25, JP Arcade , 8th Main , Binny Layout , 1st Stage ,
Vijayanagar ,Bangalore -48,

2 Customer Reference

2.1 ULR No : CC247322100020681F
2.2 SRF No : 5099
2.3 Certificate No. : VI/22-23/5099-03
2.4 Format No. : VI-FRM-ME-105
2.5 Receipt Date : 18-11-2022
2.6 DC No / DC Date : -- & 17-11-2022
2.7 Date Of Issue : 21-11-2022

3 Details Of Device Under Calibration(DUC),

3.1 Nomenclature : Micro Pipette
3.2 Make : Biohit / Proline
3.3 Range : 5 - 50 µl
3.4 SL No. : 10047236
3.5 DUC Condition : Satisfactory
3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
3.7 No.of Pages : 2
3.8 Calibration Date : 21-11-2022
3.9 Calibration Due : 20-11-2023
3.10 Calibration done at : VI Volumetric Lab
3.11 Discipline : Mechanical (Mass & volume)

4 Environmental Condition

Temperature 20.4 °C Humidity 52 %Rh

5 Standards Used for calibration

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/22-23/INT-ME-121	15-09-2023
2	E1 Class Weights	LCGC	VI-E1-ME-001	1mg to 200g	TVCSP22/03/527-01	30 - 03 - 2025

6 Note:

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab.
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By

Ranjith Kumar P
(Calibration Engineer)

Checked By

P. Santhosh Kumar
(Lab. In Charge)



VAN/
ERT
rd Cros
3789 /
on La
stom



VAIDYANATHESHWARA INSTRUMENTS

CERTIFICATE OF CALIBRATION



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/22-23/5099-03

Page 2 of 2

Range: 5 - 50 μ l

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty \pm
5 - 50 μ l	μ l	μ l	μ l
	5	4.937	0.02
	20	19.423	0.04
	50	49.091	0.20

Note:

- 1. Visual Inspection : Found Well.
- 2. Tripple Distilled water is used to Calibrate the MicroPipette.

Conclusion /Remarks:

- 1. Ref. standard used are traceable to National/International Standard
- 2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Ranjith kumar P
(Calibration Engineer)

Checked By

P. Santhosh Kumar
(Lab- In-Charge)



CERTIFICATE OF CALIBRATION

No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Page 1 of 2

1 Name and Address of the Customer : M/s. ACHARYA TULSI® DENTAL CARE & DIAGNOSTIC CENTRE
#25, JP Arcade , 8th Main , Binny Layout , 1st Stage ,
Vijayanagar ,Bangalore -40,

2 Customer Reference

2.1 ULR No : CC247322100020683F
2.2 SRF No : 5099
2.3 Certificate No. : VI/22-23/5099-05
2.4 Format No. : VI-FRM-ME-105
2.5 Receipt Date : 16-11-2022
2.6 DC No. / DC Date : -- & 17-11-2022
2.7 Date Of Issue : 21-11-2022

3 Details Of Device Under Calibration(DUC),

3.1 Nomenclature : MicroPipette
3.2 Make/Model : Biohit/Proline
3.3 Range : 100 - 1000 µl
3.4 SI.No. : YE5E428280
3.5 DUC Condition : Satisfactory
3.6 Calibration Procedure No. : SOP-16-71 Based On ISO 8655-6:2002 E
3.7 No.of Pages : 2
3.8 Calibration Date : 21-11-2022
3.9 Calibration Due : 20-11-2023
3.10 Calibration done at : VI Volumetric Lab
3.11 Discipline : Mechanical (Mass & volume)

4 Environmental Condition

Temperature 20.4 °C Humidity 51 %Rh

5 Standards Used for calibration

Sl. No.	Nomenclature	Make & Model	Sl. No	Range	Traceable to /Cert. No.	Validity
1	Digital Weighing Balance	RADWAG/MYA5.4Y	544953	0.1mg to 5g	VI/22-23/INT-ME-121	15-09-2023
2	E1 Class Weights	LCGC	VI-E1-ME-001	200g to 1mg	TVCSP22/03/527-01	30 - 03 - 2025

6 Note:

- 6.1. The Calibration Certificate relates only to the above DUC
- 6.2. Publication or reproduction of this Certificate in any form other than by complete set of the whole report & in the language, written, is not permitted without the written consent of VI Lab..
- 6.3. Corrections/erasing, invalidate the Calibration Certificate.
- 6.4. Calibration of the DUC are traceable to National standards/International Standards
- 6.5. Any error in this Certificate should be brought to our knowledge within 30 days from the date of this Cert.
- 6.6. Results Reported are valid at the time of and under the stated conditions of measurements.
- 6.7. The usage of NABL symbol is as per NABL guidelines given in NABL-133.

Calibrated By

Ranjith Kumar P
(Calibration Engineer)

Checked By

P. Santhosh Kumar
(Lab- In-Charge)





COMMITTED TO THE CUSTOMER SINCE - 1996

VAIDYANATHESHWARA INSTRUMENTS



CERTIFICATE OF CALIBRATION

CC-2473



No. 301/A, 9th Main Road, 3rd Cross, Rajiv Gandhi Nagar, J.B. Kaval, Nandhini Layout Post, Bangalore - 560 096.
Ph : 080-23377266, Mob : 9986586789 / 9632221171 / 9964308118 | Email : info@viplgroup.com Web : www.viplgroup.com

NABL Accredited Calibration Lab as per ISO/IEC 17025 : 2017 With vide Certificate No: CC-2473

Certificate No: VI/22-23/5099-05

Page 2 of 2

Range: 100 - 1000 µl

Results:

Range	Cal Point	Volume observed	Expanded Uncertainty ±
	µl	µl	µl
100 - 1000 µl	100	100.873	0.62
	500	501.937	3.10
	1000	1002.878	6.20

Note:

1. Visual Inspection : Found Well.
2. Trippl Distilled water is used to Calibrate the MicroPipette.

Conclusion /Remarks:

1. Ref. standard used are traceable to National/International Standard
2. The Expanded Uncertainty of associated with measurement at approximate 95.45% confidence level with coverage factor k=2

Calibrated By

Ranjith kumar P
(Calibration Engineer)

Checked By

P. Santhosh Kumar
(Lab- In-Charge)

