



EXCELLAS CLINICS

External Quality Assurance Program-RML

SECTION : CLPTH

EQAS:RML (LAB CODE:2539)

ROUND NO. : 12 MONTH : DEC-2022

Date	Test Parameters	Sample Type	Date of EQAS run	Report Received on	Findings	Corrective Action Taken	Remark LD/QM
10/01/2023	Sp.Gravity pH Leukocytes Nitrite Protein Glucose Ketone Urobilinogen Bilirubin Blood(Hemoglobin)	Urine	07/12/2022	04/01/2023	All parameters are within consensus	NA	Result Satisfactory
FORM NO: 04							
FORM NAME : EQAS EVALUTION FORM-URINE FM/EQAS-EVAL-URINE/QM/TP/04							
ISSUE NO: 01							
ISSUE DATE: 01/06/2022							
AMN NO :00							
AMMENDED DATE :00							
ISSUE BY : QM							
APPROVED BY: LD							



*Handwritten signature*

LAB DIRECTOR



# RML – Quality Assurance Program (RML – QAP)



## Urine Routine Analysis

### ALL METHOD REPORT

Cycle - 11/2022  
Round No -12

Date: 20/12/2022

Lab Code: 2539

Parameters	Units	No.of. Participants	Consensus		Consensus Result	Your Value	Remark
			Number	%			
Specific Gravity	-	266	243	91%	1.010-1.020	1.010	Within Consensus
pH	-	266	255	88%	6.0	6.0	Within Consensus
Leukocytes	/μl	260	259	100%	Negative	.	-
Nitrite	-	253	245	97%	Negative	.	-
Protein	mg/dl	265	256	97%	Negative	Negative	Within Consensus
Glucose	mg/dl	266	263	99%	Negative	Negative	Within Consensus
Ketones	-	267	263	99%	Negative	Negative	Within Consensus
Urobilinogen	mg/dl	262	257	98%	Negative	Negative	Within Consensus
Bilirubin	mg/dl	265	262	99%	Negative	Negative	Within Consensus
Blood (Hemoglobin)	/μl	263	258	98%	Negative	Negative	Within Consensus

Legends	≥ 60% Consensus	(*) Outside Consensus	(@) No Consensus	(.) Not Reported	(#) Late Result Submission
---------	-----------------	-----------------------	------------------	------------------	----------------------------

Chief Coordinator

Dr. Sanjay Mehrotra

Checked By

Prepared By: SK

Programme Director

Dr. Bandana Mehrotra

Page 1 of 4



QUALITY MANAGER

Doc. No.: ASS/PC/10/R/01/Dt.: 05.01.2022

**RML**  
Research Foundation

Address: B-171 Nirala Nagar, Lucknow - 226 020 Ph: 405-001301, 407-80, 2788-4414 (05-212788333)

Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

Continuous Efforts And Execution Leads To Quality Excellence



# RML – Quality Assurance Program (RML – QAP)







## URINE ROUTINE ANALYSIS

### GRAPHICAL REPORT

Cycle - 11/2022  
Round-12

Date:20/12/2022

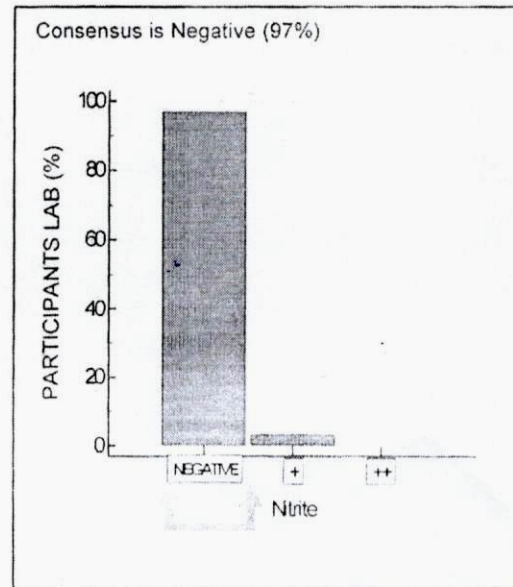

*[Signature]*  
**QUALITY MANAGER**









## URINE ROUTINE ANALYSIS

### GRAPHICAL REPORT

Cycle - 11/2022  
Round-12

Date:20/12/2022



Doc. No.: ASS / FR / 02 / R 00 / Dt.: 01.07.2012



*Handwritten Signature*  
**QUALITY MANAGER**



Address: B-171, Nirala Nagar, Lucknow - 226 020. Ph. : 4034100-130 (30 Lines), 4077180, 2788444 Fax : (0522)2788555

Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com





URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-12

Date:20/12/2022

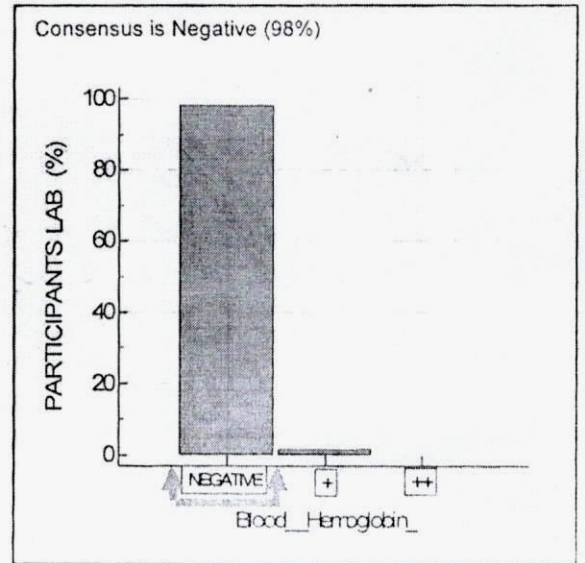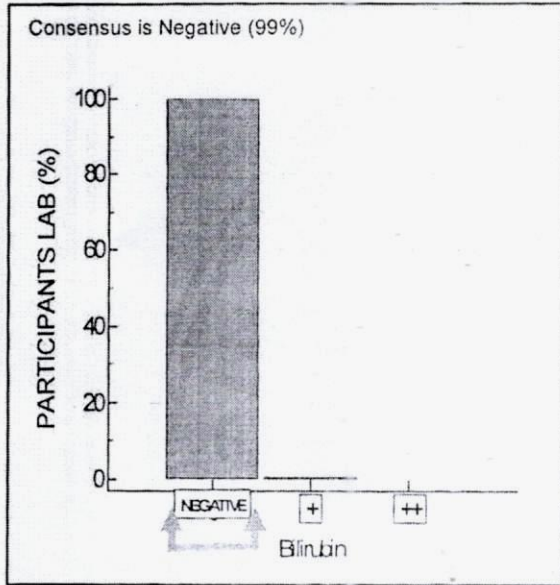

Doc. No.: ASS / FR / 02 / R 00 / Dt. 01.07.2012



*Pandi L*  
**QUALITY MANAGER**



Address: B-171, Nirala Nagar, Lucknow - 226 020. Ph. : 4034100-130 (30 Lines), 4077180, 2788444 Fax : (0522)2788555

Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

RML GAP - 2022  
Round - 12  
Date - 07/12/2022  
Urine Routine Analysis

Urobilinogen - Negative  
Protein - Negative  
pH - 6.0  
Blood - Absent  
Specific Gravity - 1.015  
Ketone - Negative  
Bilirubin - Negative  
Glucose - Negative.

Univar Diagnostics



Done by  
*[Signature]*

QUALITY MANAGER

*[Signature]*

LAB DIRECTOR

*[Signature]*



# RML – Quality Assurance Program (RML – QAP)

Result Sheet



## Urine Routine Analysis

(Filled by Participant)

Lab Code No. 2539

Sample Testing Date: 7/12/2022

(Filled by QAP Provider)

Cycle No.:11

Round No.:12

Last Date for Result Submission: 10.12.2022

S. No.	Name of the Test	Result	Units
1.	Specific gravity	<input type="radio"/> 1.000 <input type="radio"/> 1.005 <input checked="" type="radio"/> 1.010 <input type="radio"/> 1.020 <input type="radio"/> 1.030	NA
2	pH	<input type="radio"/> 5.0 <input checked="" type="radio"/> 6.0 <input type="radio"/> 7.0 <input type="radio"/> 8.0 <input type="radio"/> 9.0	NA
3	Leukocytes	<input type="radio"/> Negative <input type="radio"/> +=25 <input type="radio"/> +++=100 <input type="radio"/> +++=500	/μl
4	Nitrite	<input type="radio"/> Positive <input type="radio"/> Negative	NA
5	Protein	<input checked="" type="radio"/> Negative <input type="radio"/> +=25 <input type="radio"/> +=75 <input type="radio"/> +++=150 <input type="radio"/> +++=500	mg/dl
6	Glucose	<input checked="" type="radio"/> Negative <input type="radio"/> +=50 <input type="radio"/> +=100 <input type="radio"/> +++=300 <input type="radio"/> +++=1000	mg/dl
7	Ketones	<input checked="" type="radio"/> Negative <input type="radio"/> +=5 <input type="radio"/> +=15 <input type="radio"/> +++=50 <input type="radio"/> +++=150	NA
8	Urobilinogen	<input checked="" type="radio"/> Negative <input type="radio"/> +=1 <input type="radio"/> +=4 <input type="radio"/> +++=8 <input type="radio"/> +++=12	mg/dl
9	Bilirubin	<input checked="" type="radio"/> Negative <input type="radio"/> +=1 <input type="radio"/> +=3 <input type="radio"/> +++=6	mg/dl
10	Blood (Hemoglobin)	<input checked="" type="radio"/> Negative <input type="radio"/> +=10 <input type="radio"/> +=25 <input type="radio"/> +++=50 <input type="radio"/> +++=150 <input type="radio"/> +++=250	/μl

NP

NP



*Handwritten signature*


Note: -

**DONE BY QUALITY MANAGER LAB DIRECTOR**

You are request to report the result only given format. You may also send your results through mail, to a valid email id in result submission.

Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com





<p style="text-align: center;"><b>EXCELLAS CLINICS</b></p> <p style="text-align: center;">External Quality Assurance Program-RML</p> <p style="text-align: center;">SECTION : CLPTH</p> <p style="text-align: center;">EQAS:RML (LAB CODE:2539)</p> <p style="text-align: center;">MONTH : NOV-2022</p>		<p style="text-align: center;">ROUND NO. : 11</p>		<p style="text-align: center;">FORM NAME : EQAS EVALUATION FORM-URINE</p>		<p style="text-align: center;">FM/EQAS-EVAL-URINE/QM/TP/04</p>					
								<p style="text-align: center;">Date</p>		<p style="text-align: center;">Sample Type</p>	
								<p style="text-align: center;">20/12/2022</p>		<p style="text-align: center;">Urine</p>	
								<p style="text-align: center;">Test Parameters</p> <p>Sp.Gravity</p> <p>pH</p> <p>Leukocytes</p> <p>Nitrite</p> <p>Protein</p> <p>Glucose</p> <p>Ketone</p> <p>Urobilinogen</p> <p>Bilirubin</p> <p>Blood(Hemoglobin)</p>		<p style="text-align: center;">Date of EQAS run</p> <p style="text-align: center;">07/11/2022</p>	
<p style="text-align: center;">Report Received on</p> <p style="text-align: center;">20/12/2022</p>		<p style="text-align: center;">Findings</p> <p style="text-align: center;">All parameters are within consensus</p>		<p style="text-align: center;">Corrective Action Taken</p> <p style="text-align: center;">NA</p>		<p style="text-align: center;">Remark LD/QM</p> <p style="text-align: center;">Result Satisfactory</p>					
<p style="text-align: center;">FORM NO: 04</p>				<p style="text-align: center;">ISSUE NO: 01</p>							
<p style="text-align: center;">AMN NO :00</p>				<p style="text-align: center;">AMMENDED DATE :00</p>							
<p style="text-align: center;">ISSUE BY : QM</p>				<p style="text-align: center;">APPROVED BY: LD</p>							





## Urine Routine Analysis

### ALL METHOD REPORT

Cycle - 11/2022  
Round No -11

Date: 28/11/2022

Lab Code: 2539

Parameters	Units	No.of. Participants	Consensus		Consensus Result	Your Value	Remark
			Number	%			
Specific Gravity	-	274	210	77%	1.010-1.020	1.020	Within Consensus
pH	-	270	228	84%	7.0-8.0	7.0	Within Consensus
Leukocytes	/μl	263	195	74%	2+3+	.	-
Nitrite	-	262	213	81%	Positive	.	-
Protein	mg/dl	271	207	76%	2+3+	3+	Within Consensus
Glucose	mg/dl	271	173	64%	3+4+	3+	Within Consensus
Ketones	-	268	167	62%	2+3+	2+	Within Consensus
Urobilinogen	mg/dl	267	190	71%	2+3+	2+	Within Consensus
Bilirubin	mg/dl	266	243	91%	2+3+	2+	Within Consensus
Blood (Hemoglobin)	/μl	268	191	71%	3+4+	4+	Within Consensus

Legends	≥ 60% Consensus	(*) Outside Consensus	(@) No Consensus	(.) Not Reported	(#)Late Result Submission
---------	-----------------	-----------------------	------------------	------------------	---------------------------

Chief Coordinator

Dr. Sanjay Mehrotra

Checked By:

Prepared By: RK

Programme Director

Dr. Bandana Mehrotra

Page 1 of 4








### URINE ROUTINE ANALYSIS

### GRAPHICAL REPORT

Cycle - 11/2022  
Round-11

Date:28/11/2022

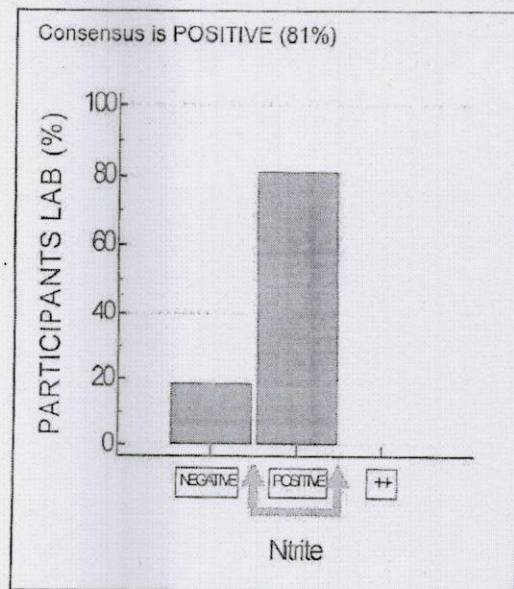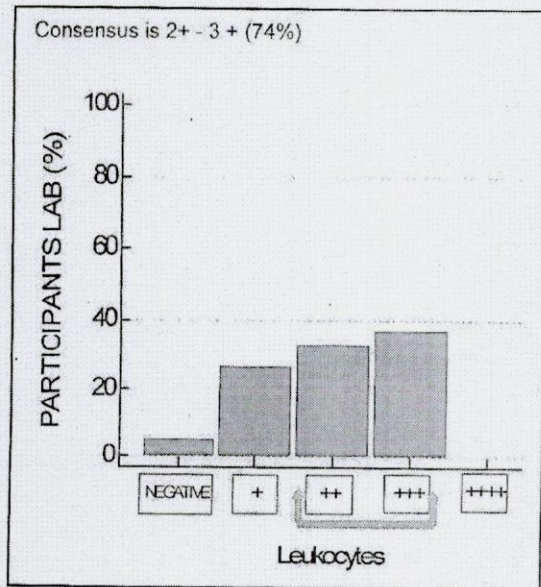








URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-11

Date:28/11/2022

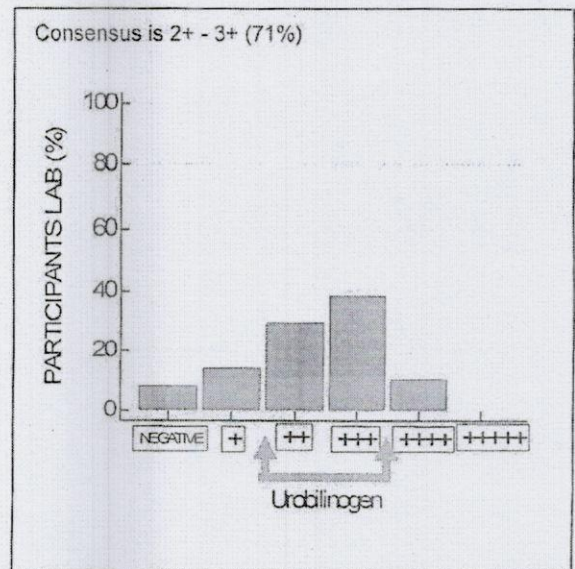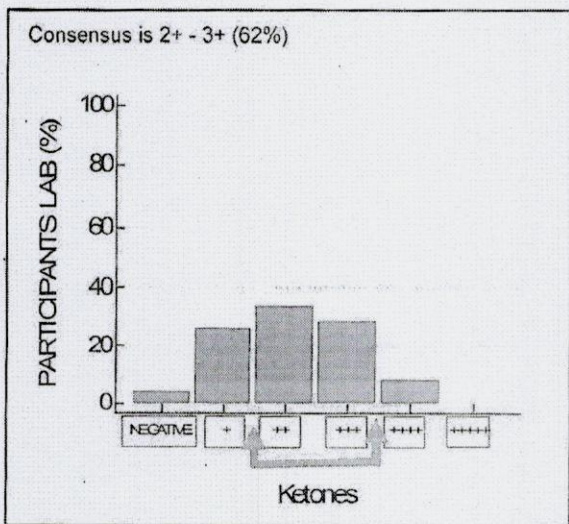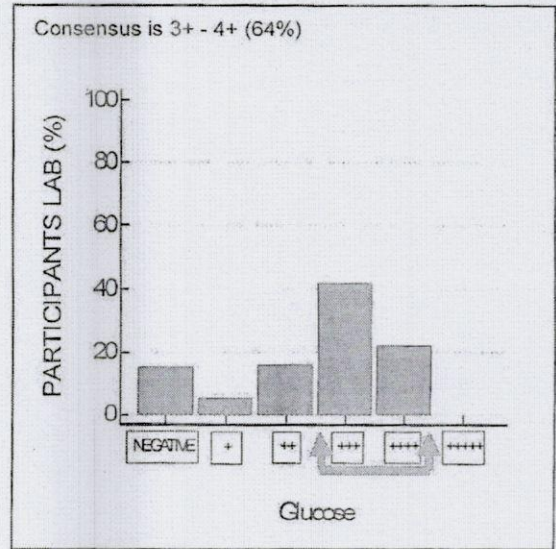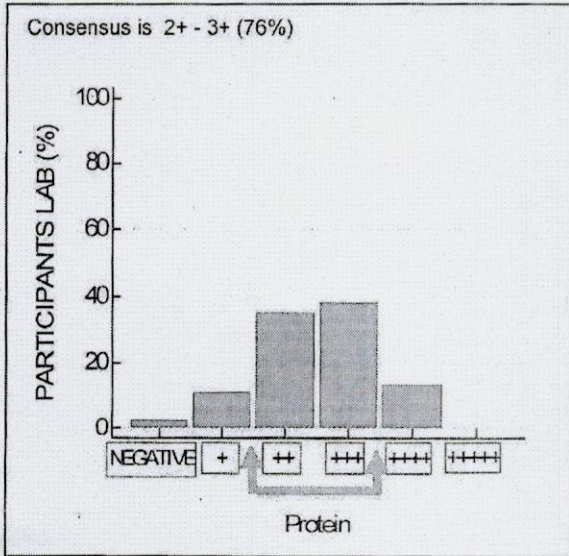






### URINE ROUTINE ANALYSIS

#### GRAPHICAL REPORT

Cycle - 11/2022  
Round-11

Date:28/11/2022

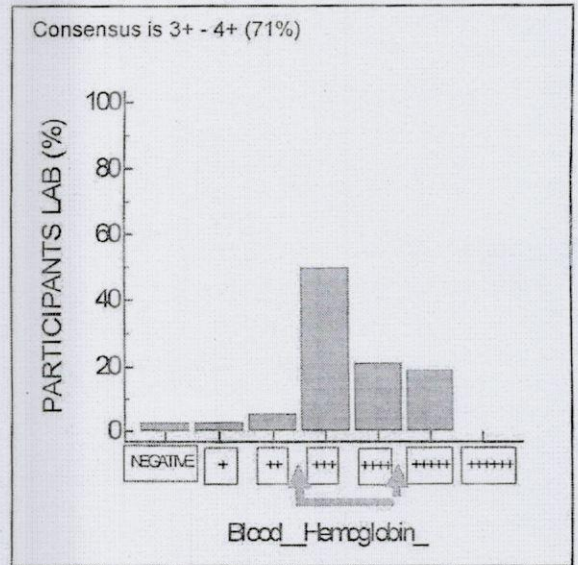





EXCELLAS CLINICS


External Quality Assurance Program-RML

SECTION : CLPTH

EQAS:RML (LAB CODE:2539)

MONTH : October-2022

ROUND NO. : 10

Date	Test Parameters	Sample Type	Date of EQAS run	Report Received on	Findings	Corrective Action Taken	Remark LD/QM
17/08/2022	Sp.Gravity pH Leukocytes Nitrite Protein Glucose Ketone Urobilinogen Bilirubin Blood(Hemoglobin)	Urine	06/10/2022	29/10/2022	All parameters are within consensus	NA	Result Satisfactory
FORM NAME : EQAS EVALUTION FORM-URINE							
FORM NO: 04							
ISSUE NO: 01							
AMN NO :00							
				ISSUE DATE: 01/06/2022		ISSUE BY : QM	
				AMMENDED DATE :00		APPROVED BY: LD	
 <small>EXCELLAS CLINICS</small>							

FM/EQAS-EVAL-URINE/QM/TP/04



# RML - Quality Assurance Program (RML - QAP)



## Urine Routine Analysis

### ALL METHOD REPORT

Lab Code: 2539


Cycle - 11/2022  
Round No -10

Date: 20/10/2022

Parameters	Units	No.of. Participants	Consensus		Consensus Result	Your Value	Remark
			Number	%			
Specific Gravity	-	253	200	79%	1.010-1.020	1.020	Within Consensus
pH	-	260	211	81%	7.0-8.0	7.0	Within Consensus
Leukocytes	/µl	251	187	75%	2+3+	.	-
Nitrite	-	249	249	86%	Positive	.	-
Protein	mg/dl	258	189	73%	2+3+	2+	Within Consensus
Glucose	mg/dl	256	224	88%	2+4+	4+	Within Consensus
Ketones	-	258	224	87%	1+3+	2+	Within Consensus
Urobilinogen	mg/dl	256	180	70%	2+3+	3+	Within Consensus
Bilirubin	mg/dl	255	239	94%	2+3+	2+	Within Consensus
Blood (Hemoglobin)	/µl	256	227	89%	3+5+	4+	Within Consensus


Legends	≥ 60% Consensus	(*) Outside Consensus	(@) No Consensus	(.) Not Reported	(#) Late Result Submission
---------	-----------------	-----------------------	------------------	------------------	----------------------------

Chief Coordinator


  
Dr. Sanjay Mehrotra

Programme Director

  
Dr. Bandana Mehrotra

Checked By: 

Page 1 of 4

Prepared By: SS 

Doc. No.: ASS/FR/10/R01/DL:05.01.2022



Address: B-171, Nirala Nagar, Lucknow - 226 020, Ph: 4034100-130 (30 Lines), 4077180, 2788444 Fax: (0522)2788555

Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

Continuous Efforts And Execution Leads To Quality Excellence











## URINE ROUTINE ANALYSIS

### GRAPHICAL REPORT

Cycle - 11/2022  
Round-10

Date:20/10/2022

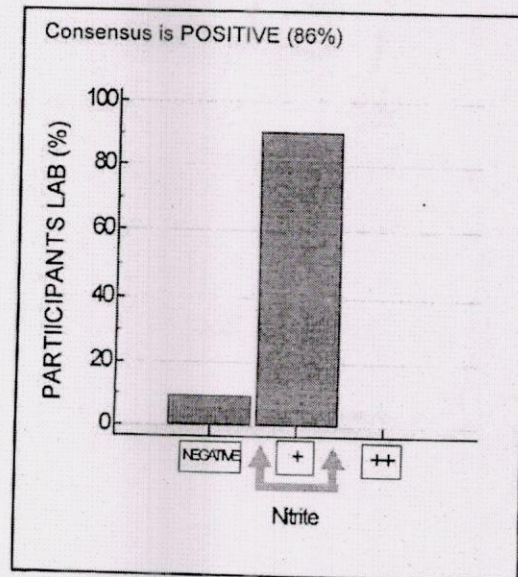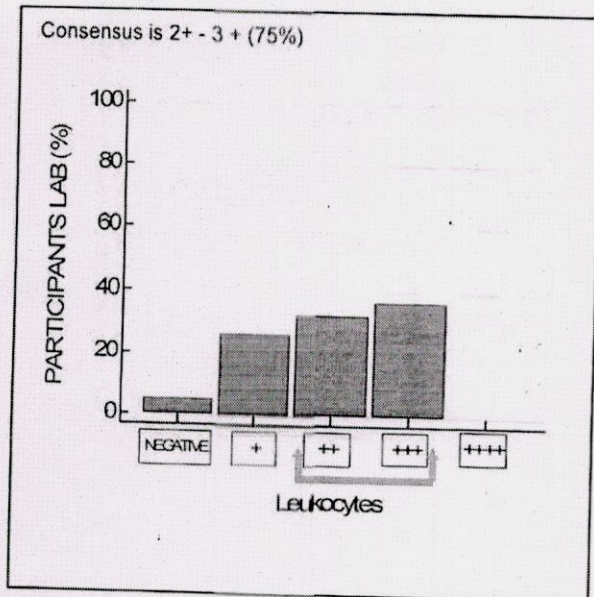







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-10

Date:20/10/2022







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-10

Date:20/10/2022





EXCELLAS CLINICS

External Quality Assurance Program-RML

SECTION : CLPTH

EQAS:RML (LAB CODE:2539)

MONTH : Sept-2022

ROUND NO.: 09

Date	Test Parameters	Sample Type	Date of EQAS run	Report Received on	Findings	Corrective Action Taken	Remark LD/QM
17/08/2022	Sp.Gravity pH Leukocytes Nitrite Protein Glucose Ketone Urobilinogen Bilirubin Blood(Hemoglobin)	Urine	05/08/2022	24/09/2022	All parameters are within consensus	NA	Result Satisfactory

FORM NO: 04      FORM NAME : EQAS EVALUTION FORM-URINE      FM/EQAS-EVAL-URINE/QM/TP/04

ISSUE NO: 01      ISSUE DATE: 01/06/2022      ISSUE BY : QM

AMN NO :00      AMMENDED DATE :00      APPROVED BY: LD

*[Signature]*  
EXCELLAS CLINICS



# RML – Quality Assurance Program (RML – QAP)



## Urine Routine Analysis

### ALL METHOD REPORT

Lab Code: 2539

Cycle - 11/2022  
Round No - 9

Date: 24/09/2022

Parameters	Units	No.of. Participants	Consensus		Consensus Result	Your Value	Remark
			Number	%			
Specific Gravity	-	260	225	87%	1.010-1.020	1.010	Within Consensus
pH	-	260	217	83%	6.0-7.0	*5.0	Outside Consensus
Leukocytes	/µl	254	249	98%	Negative	.	.
Nitrite	-	252	245	97%	Negative	.	.
Protein	mg/dl	260	257	99%	Negative	Negative	Within Consensus
Glucose	mg/dl	261	260	100%	Negative	Negative	Within Consensus
Ketones	-	261	260	100%	Negative	Negative	Within Consensus
Urobilinogen	mg/dl	257	255	99%	Negative	Negative	Within Consensus
Bilirubin	mg/dl	259	254	98%	Negative	Negative	Within Consensus
Blood (Hemoglobin)	/µl	256	245	96%	Negative	Negative	Within Consensus

Legends	≥ 60% Consensus	(*) Outside Consensus	(@) No Consensus	(.) Not Reported	(#) Late Result Submission
---------	-----------------	-----------------------	------------------	------------------	----------------------------

Chief Coordinator

Dr. Sanjay Mehrotra

Checked By:

Prepared By: SS

Programme Director

Dr. Bandana Mehrotra

Page 1 of 4

Doc. No: ASS/PR/10/R 01/DT: 05.01.2022

RML  
Research Foundation

Address: B-171, Nirala Nagar, Lucknow - 226 020. Ph. : 4034100-130 (30 Lines), 4077180, 2788444 Fax : (0522)2788555

Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

Continuous Efforts And Execution Leads To Quality Excellence







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-9

Date:24/09/2022

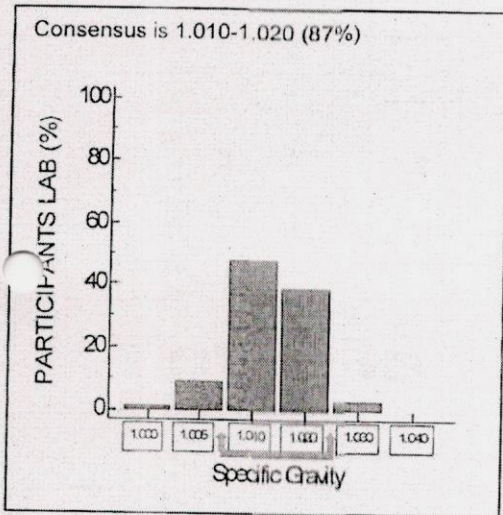







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-9

Date:24/09/2022







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-9

Date:24/09/2022





RML-RAP-2022  
Round - 09.  
Date:- 07/09/2022  
Urine Routine Analysis.

Urobilinogen - Negative  
Protein - Negative  
pH - 5.0  
Blood - Negative  
Specific Gravity - 1.010  
Ketone - Negative  
Bilirubin - Negative  
Glucose - Negative

Urim  
Dip  
Stick



*Gay*

DONE BY

*Pradip*

QUALITY MANAGER

*Nice*

LAB DIRECTOR



EXCELLAS CLINICS

External Quality Assurance Program-RML

SECTION : CLPTH

EQAS:RML (LAB CODE:2539)

MONTH : August-2022

ROUND NO.: 08

Date	Test Parameters	Sample Type	Date of EQAS run	Report Received on	Findings	Corrective Action Taken	Remark LD/QM
17/08/2022	Sp.Gravity pH Leukocytes Nitrite Protein Glucose Ketone Urobilinogen Bilirubin Blood(Hemoglobin)	Urine	05/08/2022	11/09/2022	All parameters are within consensus	NA	Result Satisfactory
FORM NAME : EQAS EVALUTION FORM-URINE							
FORM NO: 04							
ISSUE NO: 01							
AMN NO :00							
				ISSUE DATE: 01/06/2022		ISSUE BY : QM	
				AMMENDED DATE :00		APPROVED BY: LD	

FM/EQAS-EVAL-URINE/QM/TP/04

LAB DIRECTOR



# RML – Quality Assurance Program (RML – QAP)



## Urine Routine Analysis

### ALL METHOD REPORT

Lab Code: 2539

Cycle - 11/2022  
Round No - 8

Date: 07/09/2022

Parameters	Units	No.of. Participants	Consensus		Consensus Result	Your Value	Remark
			Number	%			
Specific Gravity	-	255	218	85%	1.010-1.020	1.020	Within Consensus
pH	-	256	220	86%	6.0-7.0	6.0	Within Consensus
Leukocytes	/µl	242	167	69%	2+-3+	.	-
Nitrite	-	245	208	85%	Positive	.	-
Protein	mg/dl	252	192	76%	2+-3+	*1+	Outside Consensus
Glucose	mg/dl	255	185	72%	3+-4+	3+	Within Consensus
Ketones	-	254	217	85%	1+-3+	1+	Within Consensus
Urobilinogen	mg/dl	252	210	83%	1+-3+	2+	Within Consensus
Bilirubin	mg/dl	254	239	94%	2+-3+	2+	Within Consensus
Blood (Hemoglobin)	/µl	252	219	87%	3+-5+	3+	Within Consensus

Legends	≥ 60% Consensus	(*) Outside Consensus	(@) No Consensus	(.) Not Reported	(#) Late Result Submission
---------	-----------------	-----------------------	------------------	------------------	----------------------------

Chief Coordinator

Dr. Sanjay Mehrotra

Checked By:

Prepared By: PS

**Remark:-** All parameter are within consensus except protein. For corrective action Refer EQAS evaluation report soon.


Programme Director

Dr. Bandana Mehrotra

Page 1 of 4

**LAB DIRECTOR**

Doc. No.: ASK/FR/10/R01/DL:05.01.2022



Address: B-171, Nirala Nagar, Lucknow - 226 020. Ph: 4034100-130 (30 Lines) 4077180, 2788-44 Fax: (0522)2788555

Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

Continuous Efforts And Execution Leads To Quality Excellence



# RML – Quality Assurance Program (RML – QAP)







## URINE ROUTINE ANALYSIS

### GRAPHICAL REPORT

Cycle - 11/2022  
Round-8

Date:07/09/2022









URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-8

Date:07/09/2022







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-8

Date:07/09/2022



EQNS: RML LAB CODE - 2539

Urine Routine Analysis

ROUND - 08

Sample testing Date: 05/08/2022

Specific Gravity - 1.020

PH - 6.0

Protein - 1+

Glucose - 3+

Ketone - 1+

Urobilinogen - 2+

Bilirubin - 2+

Blood - 3+



DONE BY

Ashish.

QUALITY MANAGER

Souam Poudit

*Souam Poudit*



<p align="center"><b>EXCELLAS CLINICS</b></p> <p align="center">External Quality Assurance Program-RML</p> <p align="center">SECTION : CLPTH</p> <p align="center">EQAS:RML (LAB CODE:2539)</p>		<p align="center">EXCELLAS CLINICS</p> <p align="center">External Quality Assurance Program-RML</p> <p align="center">SECTION : CLPTH</p> <p align="center">EQAS:RML (LAB CODE:2539)</p>					
<p align="center">ROUND NO. : 07</p> <p align="center">MONTH : July-2022</p>							
Date	Test Parameters	Sample Type	Date of EQAS run	Report Received on	Findings	Corrective Action Taken	Remark LD/QM
17/08/2022	Sp.Gravity pH Leukocytes Nitrite Protein Glucose Ketone Urobilinogen Bilirubin Blood(Hemoglobin)	Urine	09/07/2022	15/08/2022	All parameters are within consensus	NA	Result Satisfactory
FORM NO: 04		FORM NAME : EQAS EVALUTION FORM-URINE		FM/EQAS-EVAL-URINE/QM/TP/04			
ISSUE NO: 01		ISSUE DATE: 01/06/2022		ISSUE BY : QM			
AMN NO :00		AMMENDED DATE :00		APPROVED BY: ID			

**LAB DIRECTOR**





# RML – Quality Assurance Program (RML – QAP)



## Urine Routine Analysis

### ALL METHOD REPORT

Lab Code: 2539

Cycle - 11/2022  
Round No -7

Date: 01/08/2022

Parameters	Units	No.of Participants	Consensus		Consensus Result	Your Value	Remark
			Number	%			
Specific Gravity	-	257	239	93%	1.010-1.020	1.010	Within Consensus
pH	-	258	227	88%	6.0	*5.0	Outside Consensus
Leukocytes	/µl	251	250	99%	Negative	-	-
Nitrite	-	251	248	99%	Negative	-	-
Protein	mg/dl	257	256	100%	Negative	Negative	Within Consensus
Glucose	mg/dl	258	256	99%	Negative	Negative	Within Consensus
Ketones	-	257	256	100%	Negative	Negative	Within Consensus
Urobilinogen	mg/dl	255	255	100%	Negative	Negative	Within Consensus
Bilirubin	mg/dl	257	254	99%	Negative	Negative	Within Consensus
Blood (Hemoglobin)	/µl	255	254	100%	Negative	Negative	Within Consensus

Legends	≥ 60% Consensus	(*) Outside Consensus	(@) No Consensus	( ) Not Reported	(#) Late Result Submission
---------	-----------------	-----------------------	------------------	------------------	----------------------------

Chief Coordinator

Dr. Sanjay Mehrotra

Checked By:

Prepared By: PS


Programme Director

Dr. Bandana Mehrotra

Page 1 of 4

## LAB DIRECTOR

Doc. No.: ASS/FR/10/R/01/Dt.: 05.01.2022



Address: B-171, Nirala Nagar, Lucknow - 226 020. Ph.: 4034100-130 (30 Lines), 4077180, 2768444 Fax: (0522)2788555

Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

Continuous Efforts And Execution Leads To Quality Excellence







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-7

Date:01/08/2022









URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-7

Date:01/08/2022







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 11/2022  
Round-7

Date:01/08/2022



RML-QAP-2022.  
Cycle-11 Round-07  
Las Date-9/07/2022  
Urine Routine Analysis.



Specific gravity- 1.010  
PH - 5.0  
Protein- Negative  
Glucose- Negative  
ketones- Negative  
urobilinogen - Negative  
Bilirubin- Negative  
Blood- Negative

DONE BY -



QUALITY MANAGER -

9001  
2015  
IFIED

DIAGNOSTICS | IMAGING | VACCINATION | CONSULTATIONS | CORPORATE HEALTH CHECK-UPS