



Urine Routine Analysis

ALL METHOD REPORT

Lab Code: 2864

Cycle - 12/2023
Round No -03

Date: 31/03/2023

Parameters	Units	No.of. Participants	Consensus		Consensus Result	Your Value	Remark
			Number	%			
Specific Gravity	-	312	273	88%	1.010-1.020	*1.030	Outside Consensus
pH	-	313	261	83%	6.0	5.5	Within Consensus
Leukocytes	/µl	305	297	97%	Negative	Negative	Within Consensus
Nitrite	-	304	292	96%	Negative	Negative	Within Consensus
Protein	mg/dl	311	294	95%	Negative	Negative	Within Consensus
Glucose	mg/dl	313	302	96%	Negative	Negative	Within Consensus
Ketones	-	312	309	99%	Negative	Negative	Within Consensus
Urobilinogen	mg/dl	309	301	97%	Negative	Negative	Within Consensus
Bilirubin	mg/dl	309	300	97%	Negative	Negative	Within Consensus
Blood (Hemoglobin)	/µl	309	297	96%	Negative	Negative	Within Consensus

Legends	≥ 60% Consensus	(*) Outside Consensus	(@) No Consensus	(.) Not Reported	(#)Late Result Submission
---------	-----------------	-----------------------	------------------	------------------	---------------------------

Chief Coordinator

Dr.Sanjay Mehrotra

Checked By:

Prepared By: S

Programme Director

Dr.Bandana Mehrotra

Page 1 of 4





URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 12/2023

Round-3

Date:31/03/2023

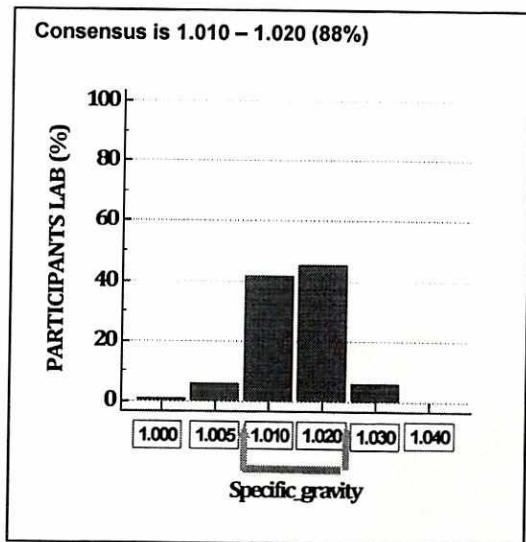





URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 12/2023

Round-3

Date:31/03/2023

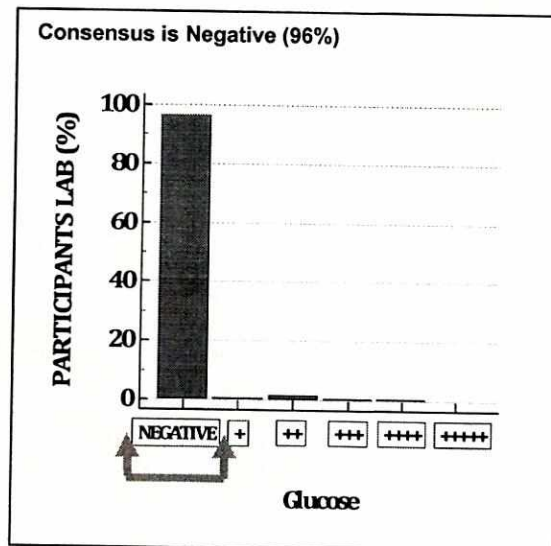



URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 12/2023
Round-3

Date:31/03/2023

