

## Urine Routine Analysis

### ALL METHOD REPORT

Cycle - 12/2023

Date: 31/03/2023

Lab Code: 2619

Round No -03

Parameters	Units	No.of. Participants	Consensus		Consensus Result	Your Value	Remark
			Number	%			
Specific Gravity	-	312	273	88%	1.010-1.020	*1.005	Outside Consensus
pH	-	313	261	83%	6.0	6.0	Within Consensus
Leukocytes	/µl	305	297	97%	Negative	Negative	Within Consensus
Nitrite	-	304	292	96%	Negative	Negative	Within Consensus
Protein	mg/dl	311	294	95%	Negative	Negative	Within Consensus
Glucose	mg/dl	313	302	96%	Negative	Negative	Within Consensus
Ketones	-	312	309	99%	Negative	Negative	Within Consensus
Urobilinogen	mg/dl	309	301	97%	Negative	Negative	Within Consensus
Bilirubin	mg/dl	309	300	97%	Negative	Negative	Within Consensus
Blood (Hemoglobin)	/µl	309	297	96%	Negative	Negative	Within Consensus


Legends	≥ 60% Consensus	(*) Outside Consensus	(@) No Consensus	(.) Not Reported	(#)Late Result Submission
---------	-----------------	-----------------------	------------------	------------------	---------------------------

Chief Coordinator



Dr.Sanjay Mehrotra

Checked By



Prepared By: S

Programme Director



Dr.Bandana Mehrotra

Page 1 of 4





## URINE ROUTINE ANALYSIS

### GRAPHICAL REPORT

Cycle - 12/2023

Round-3

Date:31/03/2023


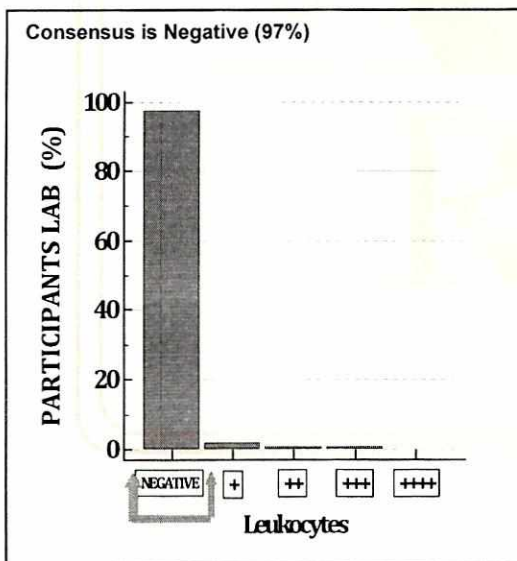




## URINE ROUTINE ANALYSIS

### GRAPHICAL REPORT

Cycle - 12/2023  
Round-3

Date:31/03/2023





## URINE ROUTINE ANALYSIS

### GRAPHICAL REPORT

Cycle - 12/2023  
Round-3

Date:31/03/2023

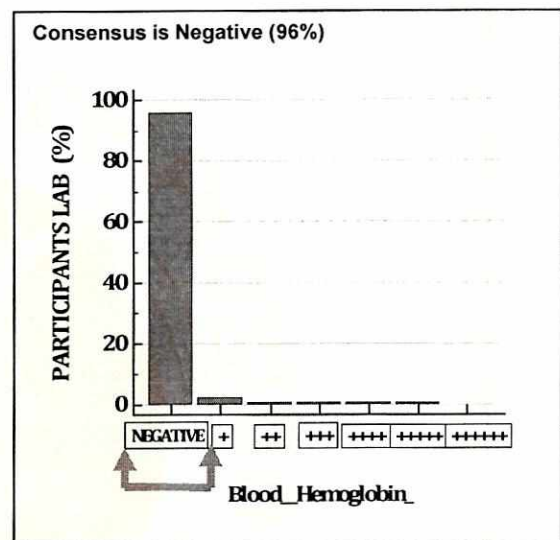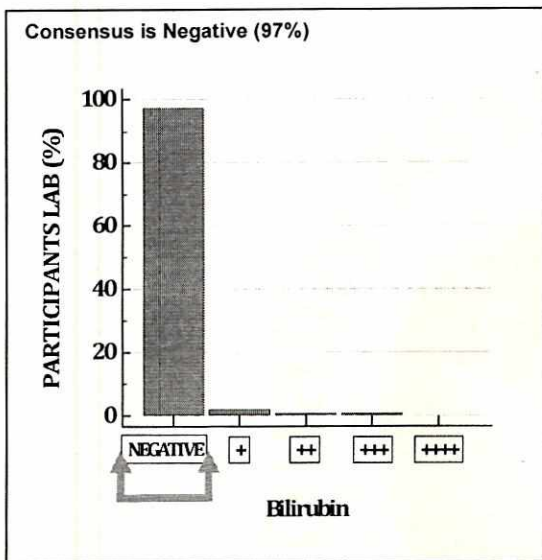

DEKAPHAN LAURA  
Seq.No: 0068  
ID: SPLIT TEST-1  
2023.04.01 09:09 AM

.....  
BLD NEG  
BIL NEG  
UBG NORM  
KET NEG  
GLU NEG  
PRO NEG  
pH 6  
NIT NEG  
LEU NEG  
SG 1.000

-----  
<Admin>

*सुप्रभा*  
*1/4/23*

DEKAPHAN LAURA  
Seq.No: 0069  
ID: SPLIT TEST-2  
2023.04.01 09:11 AM

.....  
BLD NEG  
BIL NEG  
UBG NORM  
KET NEG  
GLU NEG  
PRO NEG  
pH 6  
NIT NEG  
LEU NEG  
SG 1.000

-----  
<Admin>

*सुप्रभा*  
*1/4/23*

**IQC / EQAS Outlier Log**

TM/FR/16/R00/Dt: 01.08.2022

Department Clinical Pathology

Date/Time	Parameter	Rule violated	Corrective action	Tech Sign	Reviewed by
11/4/22	RML APP Cycle-12 Round-3	Outside consensus	Use same strip - OK Use material - OK PT material - OK Installation maintain- ance - OK	<i>[Signature]</i>	<i>[Signature]</i>
	Specific Gravity.		Clerical Error - NA Inker technician comparison done Result acceptable		

