

# CALIBRATION CERTIFICATE

**K B DIAGNOSTICS CENTER**

**Vanthavasi**

**604 408**

Dear Sir/Madam,

As desired by you please find enclosed herewith the calibration rreport

Instrument Model ; EM200

Serial number ; B200450

Range of the instrument : optical density Linear from 0-3.5 A

**Calibration done Date : 18<sup>TH</sup> APR 2023**

**Calibration due Date : 17<sup>th</sup> APR 2024**

Pressure	Ideal	Actual
	1 bar	0.98bar
Lamp voltage	12 V	12.31 V
Temperature	37 ° C	37 ° C
Photometer calibration check		ok
Cuvette blank check		ok
Wavelength	Gain	
340	860	
405	601	
505	524	
546	505	
578	468	
600	503	
660	480	

## CALIBRATION CERTIFICATE

700	438
-----	-----

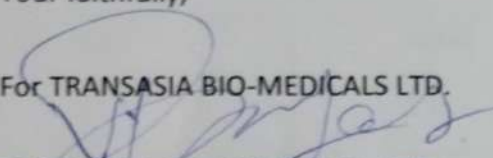
The instrument does photometer check before each batch of tests is run. It will give an error message if

The photometer test fails and it will not run any samples.

Thanking you and assuring of our prompt attention at all times.

Your faithfully,

For TRANSASIA BIO-MEDICALS LTD.

  
TRANSASIA BIO MEDICAL LTD.

New No. 19, Dr. Ranga Road,  
Jupiter Complex, 3rd Floor,  
Mylapore, Chennai - 600 004