



Urine Routine Analysis

ALL METHOD REPORT

Lab Code: 2864

Cycle - 12/2023
Round No -03

Date: 31/03/2023

Parameters	Units	No.of. Participants	Consensus		Consensus Result	Your Value	Remark
			Number	%			
Specific Gravity	-	312	273	88%	1.010-1.020	*1.030	Outside Consensus
pH	-	313	261	83%	6.0	5.5	Within Consensus
Leukocytes	/µl	305	297	97%	Negative	Negative	Within Consensus
Nitrite	-	304	292	96%	Negative	Negative	Within Consensus
Protein	mg/dl	311	294	95%	Negative	Negative	Within Consensus
Glucose	mg/dl	313	302	96%	Negative	Negative	Within Consensus
Ketones	-	312	309	99%	Negative	Negative	Within Consensus
Urobilinogen	mg/dl	309	301	97%	Negative	Negative	Within Consensus
Bilirubin	mg/dl	309	300	97%	Negative	Negative	Within Consensus
Blood (Hemoglobin)	/µl	309	297	96%	Negative	Negative	Within Consensus

Legends	≥ 60% Consensus	(*) Outside Consensus	(@) No Consensus	(.) Not Reported	(#)Late Result Submission
---------	-----------------	-----------------------	------------------	------------------	---------------------------

Chief Coordinator

Dr.Sanjay Mehrotra

Checked By:

Prepared By: S

Programme Director

Dr.Bandana Mehrotra

Page 1 of 4





URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 12/2023

Round-3

Date:31/03/2023







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 12/2023
Round-3

Date:31/03/2023

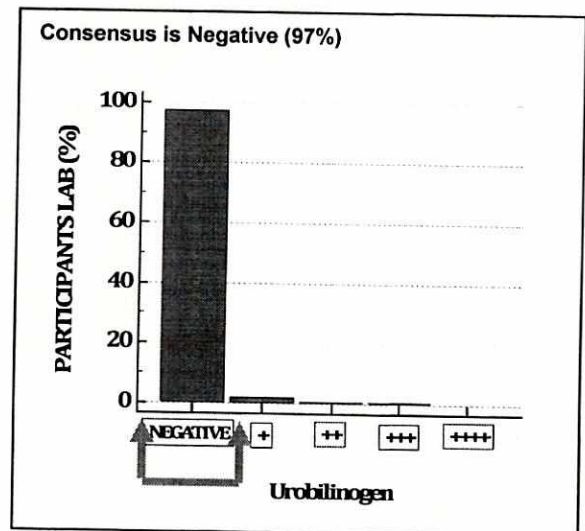





URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 12/2023
Round-3

Date:31/03/2023

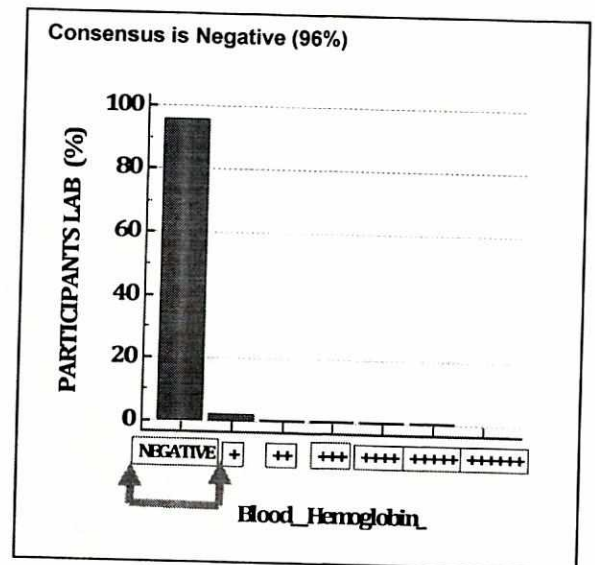



RADVISION DIAGNOSTICS & LABS

ACCURACY BRINGS CREDIBILITY

Sub - Lab ID - MELT - 00777

Date: 16-06-2023


Dear Sir/Madam,

We request you to exclude alkaline phosphate from biochemistry scope, RBC from Hematology scope and specific gravity from clinical pathology scope and issue the certificate.


Kindly do the needful.


Regards

For PRIMISH MEDICAL CARE SERVICES PVT. LTD.


Director

For PRIMISH MEDICAL CARE SERVICES PVT. LTD.


Director


Radvision Diagnostics & Labs
Accuracy Brings Credibility
No. 196, Ground Floor,
Nandidurga Road,
BANGALORE - 560046.


Radvision Diagnostics & Labs
Accuracy Brings Credibility
No. 196, Ground Floor,
Nandidurga Road,
BANGALORE - 560046.

A Unit of Primish Medical Care Services Pvt. Ltd.

196, Ground Floor, Near Airtel Office, Nandidurga Road, Jayamahal Extension, Bengaluru - 560 046.

☎ 080-41703610 | 7676565714 | ✉ info@radvisiondiagnostics.com | 🌐 www.radvisiondiagnostics.com

Ultrasound • Digital X-ray • OPG • 2D Echo • TMT • PFT • Pathology Lab • Health Packages • Consultation