

VIEW LAB MONTHLY SUMMARY

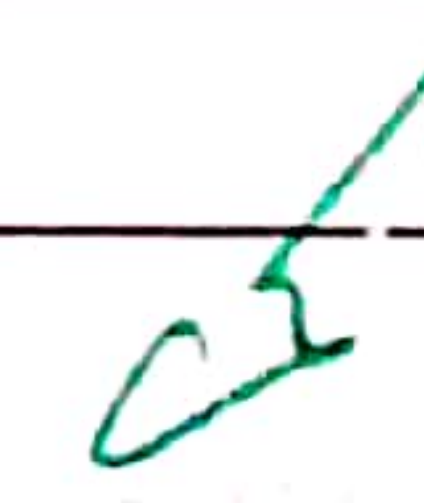
Lab Name	Govt. PHC, Subbalapuram.T.	Details About Robust Analysis	
Lab No	12699	Detail About Monthly Summary	
Month	August	Detail about SDI	
Year	2023		
Constituent Group	Chemistry III		
Click on the analyte to view Graphical Data		All Analyser Result	Print
Date of Result Entered : 21/08/2023			
Date of Report Published : 01/09/2023			

Sl.No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	Participants		Your Value	SDI	U
						CV	SD			
1	GLUCOSE III	GOD-POD III	Robonik (Semi automatic / Fully Automatic)	1841	175.58	5.13	9.00	176.43 mg/dL	0.09	0.42
2	UREA III	Others (Urease Berthelot / Ned Dye) III	Any Analyser (Automation / Semi Automation)	59	28.92	13.99	4.05	31.57 mg/dL	0.66	1.05
3	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik (Semi automatic / Fully Automatic)	1852	1.76	6.77	0.12	1.9 mg/dL	1.18	0.01
4	URIC ACID III	Enzymatic / Uricase Colorimetric III	Robonik (Semi automatic / Fully Automatic)	40	5.43	10.18	0.55	7.2 mg/dL	3.20	0.17
5	CHOLESTROL III	CHOD-PAP III	Robonik (Semi automatic / Fully Automatic)	1764	113.80	4.07	4.64	100 mg/dL	-2.98	0.22

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ± 1.01 to ± 2.00	Good.
Within ± 2.01 to ± 2.99	Accept with caution. Warning Signal.
Beyond ± 3.0	Unacceptable performance. Action Signal.

Links

Modify Address	Modify Methods	Submit Lab Results	View Lab Monthly Summary
Yearly Summary	Change Password	Home	Sign-out


 MEDICAL OFFICER
 Govt. Primary Health Centre
 Subbalapuram
 Theni Dist.