

Details About Robust Analysis  
 Detail About Monthly Summary  
 Detail about SDI

Lab Name: Govt. UPHC, Vadiveesavaram  
 Lab No: 10715  
 Month: March  
 Year: 2023  
 Constituent: Chemistry III

[All Analyser Result](#) [Print](#)

Click on the analyte to view Graphical Data  
 Date of Result Entered : 18/03/2023

Date of Report Published : 04/04/2023

Analyte	Method / Principle Name	Analyzer Name	No of Participants	Participants			Year Value	SDI	U
				DV	CV	SD			
GLUCOSE III	GOD-POD III	Robonik ( Semi automatic / Fully Automatic )	1878	91.48	7.46	6.82	87 mg/dL	-0.66	0.31
CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik ( Semi automatic / Fully Automatic )	1851	1.33	9.08	0.12	1.39 mg/dL	0.50	0.01
CHOLESTROL III	CHOD-PAP III	Robonik ( Semi automatic / Fully Automatic )	1761	110.93	5.23	5.80	111 mg/dL	0.01	0.28

SDI Range		Interpretation
within -1.00 to +1.00		Excellent.
within ±1.01 to ±2.00		Good.
within ±2.01 to ±2.99		Accept with caution. Warning Signal.
beyond ±3.0		Unacceptable performance. Action Signal.

ks  
 Modify Address  
 Submit Lab Results  
 View Lab Monthly Summary  
 Change Password  
 Home  
 Sign-out

*Medical Officer*  
 VADIVEESAVARAM  
 URBAN PRIMARY HEALTH CENTRE

LAB MONTHLY SUMMARY

Lab Name Govt. UPHC, Vadiveeswaram  
 Lab No 10715  
 Month April  
 Year 2023  
 Constituent Chemistry III  
 Group

Details About Robust Analysis  
 Detail About Monthly Summary  
 Detail about SDI

Click on the analyte to view Graphical Data

[All Analyser Result](#) [Print](#)

Date of Result Entered : 18/04/2023

Date of Report Published : 06/05/2023

No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	Participants		Your Value	SDI	U
						CV	SD			
1	GLUCOSE III	GOD-POD III	Robonik ( Semi automatic / Fully Automatic )	1832	119.45	6.04	7.21	103 mg/dL	-2.28	0.34
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik ( Semi automatic / Fully Automatic )	1820	2.16	8.09	0.18	2.39 mg/dL	1.31	0.01
3	CHOLESTROL III	CHOD-PAP III	Robonik ( Semi automatic / Fully Automatic )	1750	111.61	5.19	5.79	108 mg/dL	-0.62	0.28

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ±1.01 to ±2.00	Good.
Within ±2.01 to ±2.99	Accept with caution. Warning Signal.
beyond ±3.0	Unacceptable performance. Action Signal.

links			
Modify Address	Modify Methods	Submit Lab Results	View Lab Monthly Summary
Early Summary	Change Password	Home	Sign-out

*(Signature)*  
**Medical Officer**  
 URBAN PRIMARY HEALTH CENTRE  
 VADIVEESWARAM

CMC EXTERNAL QUALITY ASSURANCE SCHEME  
MONTHLY SUMMARY REPORT - MAY 2023

10715  
18/05/2023  
05/06/2023

Lab Name: Govt. UPHC, Vadiveesvaram  
Constituent Group: Chemistry III  
PT Item: Lyophilized human serum based

Lab No  
Date of Result Entered :  
Date of Report Published :

Sl.No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	Participants		Your Value	SDI	U
						CV	SD			
1	GLUCOSE III	GOD-POD III	Robonik ( Semi automatic / Fully Automatic	1834	180.88	5.19	9.39	183 mg/dL	0.23	0.44
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik ( Semi automatic / Fully Automatic	1854	1.76	7.48	0.13	2.02 mg/dL	1.97	0.01
3	CHOLESTROL III	CHOD-PAP III	Robonik ( Semi automatic / Fully Automatic	1798	114.60	5.08	5.83	126 mg/dL	1.96	0.27


SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ±1.01 to ±2.00	Good.
Within ±2.01 to ±2.99	Accept with caution. Warning Signal.
Beyond ±3.0	Unacceptable performance. Action Signal.

LAB ADDRESS :  
Govt. UPHC, Vadiveesvaram  
MEDICAL OFFICER, NAGERCOIL  
Vadiveesvaram  
TAMILNADU629001

*Pamela Chittudoss*  
Dr. Pamela Christudoss  
CMC EQAS Coordinator  
Christian Medical College, Vellore

Coordinator Contact Details:  
Email: [clinqc@cmcvellore.ac.in](mailto:clinqc@cmcvellore.ac.in)  
Contact Number: 0416-2283102

Homogeneity and Stability of the sample is passed.  
Data in CMC EQAS reports is confidential  
CMC EQAS does not sub contract any components  
\*\*\*\*\* End of Report \*\*\*\*\*

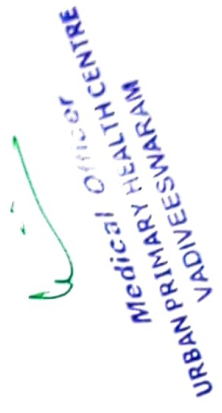



DEPARTMENT OF CLINICAL BIOCHEMISTRY  
CMC EXTERNAL QUALITY ASSURANCE SCHEME  
MONTHLY SUMMARY REPORT - JUNE 2023



PC-1024

10715

20/06/2023

04/07/2023

Govt. UPHC, Vadivesvaram

Chemistry III

Lyophilized human serum based

Lab Name

Constituent Group

PT item

Sl.No	Analyte	Method	Principle Name	Analyzer Name	No of Participants	DV	Participants				
							CV	SD	U		
1	GLUCOSE III	GOD-POD III		Robonik ( Semi automatic / Fully Automatic )	1823	286.63	5.17	14.82	270 mg/dL	-1.12	0.69
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III		Robonik ( Semi automatic / Fully Automatic )	1848	2.57	6.64	0.17	2.6 mg/dL	0.18	0.01
3	CHOLESTROL III	CHOD-PAP III		Robonik ( Semi automatic / Fully Automatic )	1804	113.73	4.46	5.07	128 mg/dL	2.81	0.24

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ±1.01 to ±2.00	Good.
Within ±2.01 to ±2.99	Accept with caution. Warning Signal.
Beyond ±3.0	Unacceptable performance. Action Signal.

LAB ADDRESS :


Govt. UPHC, Vadivesvaram  
MEDICAL OFFICER, NAGERCOIL  
Vadivesvaram  
TAMILNADU629001

*Pamela Christudoss*

Dr. Pamela Christudoss  
CMC EQAS Coordinator  
Christian Medical College, Vellore

Coordinator Contact Details:  
Email: [clinqc@cmcvellore.ac.in](mailto:clinqc@cmcvellore.ac.in)  
Contact Number: 0416-2283102

Homogeneity and Stability of the sample is passed.  
Data in CMC EQAS reports is confidential  
CMC EQAS does not sub contract any components  
\*\*\*\*\* End of Report \*\*\*\*\*

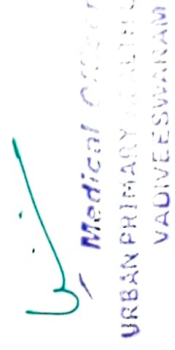

Medical Officer  
URBAN PRIMARY HEALTH CENTRE  
VADIVESVARAM



Lab Name: Govt. UPHC, Vadiveeswaram Lab No: 10715

Constituent Group: Chemistry III Date of Result Entered: 19/07/2023

PT Item: Lyophilized human serum based Date of Report Published: 07/08/2023

Sl No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	Participants CV	SD	Your Value	SDI	U
1	GLUCOSE III	GOD-POD III	Robonik ( Semi automatic / Fully Automatic	1876	109.35	5.55	6.07	106 mg/dL	-0.55	0.28
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik ( Semi automatic / Fully Automatic	1850	5.83	6.00	0.35	6 mg/dL	0.49	0.02
3	CHOLESTROL III	CHOD-PAP III	Robonik ( Semi automatic / Fully Automatic	1776	113.00	4.12	4.66	112 mg/dL	-0.21	0.22
<b>SDI Range Interpretation</b>										
Within -1.00 to +1.00				Excellent.						
Within ±1.01 to ±2.00				Good.						
Within ±2.01 to ±2.99				Accept with caution. Warning Signal.						
Beyond ±3.0				Unacceptable performance. Action Signal.						

**LAB ADDRESS :**  
 Govt. UPHC, Vadiveeswaram  
 MEDICAL OFFICER, NAGERCOIL  
 Vadiveeswaram  
 TAMILNADU629001

**Coordinator Contact Details:**  
 Email: [clinqc@cmcvellore.ac.in](mailto:clinqc@cmcvellore.ac.in)  
 Contact Number: 0416-2283102

*Paula Christodoss*  
 Dr. Pamela Christodoss  
 CMC EQAS Coordinator  
 Christian Medical College, Vellore

Homogeneity and Stability of the sample is passed.  
 Data in CMC EQAS reports is confidential  
 CMC EQAS does not sub contract any components  
 \*\*\*\*\* End of Report \*\*\*\*\*

**Medical Officer**  
 URBAN PRIMARY HEALTH CENTRE  
 VADIVEESWARARAM



# CHRISTIAN MEDICAL COLLEGE

DEPARTMENT OF CLINICAL BIOCHEMISTRY  
CMC EXTERNAL QUALITY ASSURANCE SCHEME  
MONTHLY SUMMARY REPORT - AUGUST 2023



PC-1024

Lab Name Govt. UPHC, Vadiveesvaram  
Constituent Group Chemistry III  
PT Item Lyophilized human serum based

Lab No 10715  
Date of Result Entered : 18/08/2023  
Date of Report Published : 01/09/2023

Sl No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	Participants		Your Value	SDI	L
						CV	SD			
1	GLUCOSE III	GOD-POD III	Robonik ( Semi automatic / Fully Automatic )	1841	175.58	5.13	9.00	171 mg/dL	-0.51	0.42
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik ( Semi automatic / Fully Automatic )	1852	1.76	6.77	0.12	1.76 mg/dL	0.00	0.01
3	CHOLESTROL III	CHOD-PAP III	Robonik ( Semi automatic / Fully Automatic )	1764	113.80	4.07	4.64	112 mg/dL	-0.39	0.22

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ±1.01 to ±2.00	Good.
Within ±2.01 to ±2.99	Accept with caution. Warning Signal.
Beyond ±3.0	Unacceptable performance. Action Signal.

LAB ADDRESS :  
Govt. UPHC, Vadiveesvaram  
MEDICAL OFFICER, NAGERCOIL  
Vadiveesvaram  
MILNADU629001

Coordinator Contact Details:  
Email:clinqc@cmcvellore.ac.in

*[Signature]*  
Medical Officer  
URBAN PRIMARY HEALTH CENTRE  
VADIVEESWARAM

*[Signature]*  
Dr. Pamela Christudoss  
CMC EQAS Coordinator  
Christian Medical College, Vellore