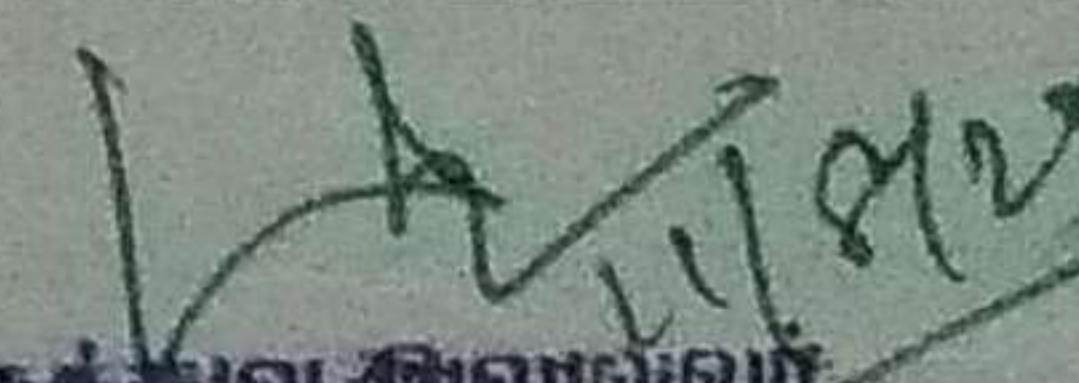


VIEW LAB MONTHLY SUMMARY

| Lab Name | Govt. PHC, Vadugapatti | Details About Robust Analysis | | | | | | | | |
|---|------------------------|--|--|--------------------|--------|-----------------|------|--------------|-------|------|
| Lab No | 12906 | Detail About Monthly Summary | | | | | | | | |
| Month | July | Detail about SDI | | | | | | | | |
| Year | 2023 | | | | | | | | | |
| Constituent Group | Chemistry III | | | | | | | | | |
| Click on the analyte to view Graphical Data | | All Analyser Result | Print | | | | | | | |
| Date of Result Entered : 21/07/2023 | | | | | | | | | | |
| Date of Report Published : 07/08/2023 | | | | | | | | | | |
| Sl.No | Analyte | Method / Principle Name | Analyzer Name | No of Participants | DV | Participants CV | SD | Your Value | SDI | U |
| 1 | GLUCOSE III | GOD-POD III | Robonik (Semi automatic / Fully Automatic) | 1876 | 109.35 | 5.55 | 6.07 | 110.73 mg/dL | 0.23 | 0.28 |
| 2 | CREATININE III | Jaffes Kinetic - Alkaline Picrate III | Robonik (Semi automatic / Fully Automatic) | 1850 | 5.83 | 6.00 | 0.35 | 6.04 mg/dL | 0.60 | 0.02 |
| 3 | CHOLESTROL III | CHOD-PAP III | Robonik (Semi automatic / Fully Automatic) | 1776 | 113.00 | 4.12 | 4.66 | 111.88 mg/dL | -0.24 | 0.22 |
| SDI Range | | Interpretation | | | | | | | | |
| Within -1.00 to +1.00 | | Excellent. | | | | | | | | |
| Within ± 1.01 to ± 2.00 | | Good. | | | | | | | | |
| Within ± 2.01 to ± 2.99 | | Accept with caution. Warning Signal. | | | | | | | | |
| Beyond ± 3.0 | | Unacceptable performance. Action Signal. | | | | | | | | |

Links

| | | | |
|----------------|-----------------|--------------------|--------------------------|
| Modify Address | Modify Methods | Submit Lab Results | View Lab Monthly Summary |
| Yearly Summary | Change Password | Home | Sign-out |


 மருத்துவ அலுவலர்
 அரசு ஆரம்ப சுகாதார நிலையம்
 வடமேற்கு.