



# Vanavil Calibrations

Make It Simple, But Significant !

## CALIBRATION CERTIFICATE

Page no: 1 of 1

<b>Customer Name &amp; Address:</b> M/S GOVERNMENT PRIMARY HEALTH CENTRE, SERAPATTU, KALLAKURICHI - 606 401.	Certificate No:	VCPL/CC/23-24/31-004
	Date of Calibration:	27-09-2023
	Date of issue:	28-09-2023
	Date of Receipt:	27-09-2023
	Next cal Date:	26-09-2024

### Details of Device Under Calibration

Description:	MICROPIPETTE	Make:	MICROLUX
Range:	(5 to 50) $\mu$ l	Model/Type:	GB MAX I PET
Resolution:	1 $\mu$ l	Condition of DUC	GOOD
Serial Number	-	Location:	LABORATORY
ID number	GPHC/LAB/MP-02	Cal. At:	LAB
<b>Environmental Conditions</b>		<b>Calibration Method Used</b>	
Temperature	23.5 $^{\circ}$ C	Calibration Method Used	ISO 8655:2002 PART-6
Humidity	49 % Rh	Cal procedure no:	-

### Master Details

SL no:	Description	ID No / SL No	Certificate No	Make/Model	Valid Till
1	ELECTRONIC BALANCE	16031172	E-150323-1	WINTECH	15-03-2024

### RESULT OF CALIBRATION

S.NO	Duc Readings ( $\mu$ l )	Standard Reading Mean Value ( mg )	ERROR (mg)
1	5	4.91	0.09
2	25	24.78	0.22
3	50	49.89	0.11


### Remarks:

- 1.DUC is Defined as Device Under Calibration.
- 2.Calibration Frequency decided by the customer.
- 3.The above instrument is working in good condition.

Calibrated By:

*C. Akash*  
C.AKASH

(CALIBRATION ENGINEER)

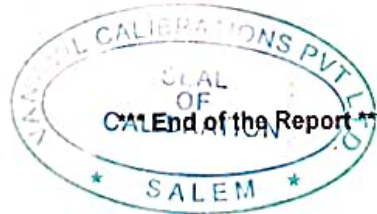

Authorised by:

*S. Lakshmanan*  
S. LAKSHMANAN MURUGAN,  
Technical Manager  
Vanavil Calibrations Pvt Ltd.

## Vanavil Calibrations Pvt. Ltd

(A Unit of Rainbow Bio Medical Engineers)

S2, Rishi Maharaj Apartment, Indra Nagar, 250 Reddiyur Main Road, Narasothipatty, Salem - 636 004.

No. 96,97,98, Anadhamaya Apartments, 2<sup>nd</sup> Floor, KVR Flats, 2<sup>nd</sup> Cross Street, Thangam Nagar, Pallikaranai, Chennai - 600 100.

Cell: 99949 13872 / 99949 23872 Ph: 0427-7965376

✉ vanavilcalibrations@gmail.com 🌐 www.rainbowbiomedicalengineers.com 🌐 www.vanavilcalibrations.com