



Vanavil Calibrations
Make It Simple, But Significant!

CALIBRATION CERTIFICATE

Page no: 1 of 1

Customer Name & Address: GOVT PRIMARY HEALTH CENTRE, PUDUPATTU - 632 508.	SRF No :	VCPL/22-23 /06-01/25-03-2023
	Date of Issue :	27/Mar/2023
	Date of Receipt :	25/Mar/2023
	Date of Calibration :	25/Mar/2023
	Cal Due Date :	24/Mar/2024
	Calibration at	IN LAB

Details of Device Under Calibration:

Description:	MICRO PIPETTE	Make :	-
Range:	0-1000 μ l	Model/Type:	MICROLUX
Resolution:	10 μ l	Accuracy :	
Serial Number:		Instrument Location:	LAB
ID number:	-	Condition of DUC:	GOOD

Temperature	24.8 °C	National/International standard:	-
Humidity	52 % Rh	Cal procedure no:	-

Master Details


SL no:	Description	Serial No	Make/Model	Certificate No	Valid Till
1	ELECTRONIC BALANCE	16031172	WINTECH / -	E150323-3-1	15/Mar/24

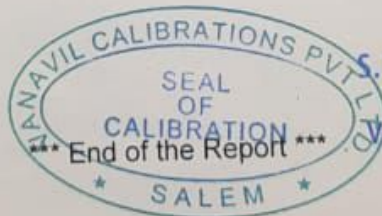
CALIBRATION RESULT

S.NO	DUC Readings (μ l)	Standard Rreadings Mean Value (mg)	ERROR (μ l)
1	10	9.93	0.070
2	500	499.88	0.120
3	1000	998.92	1.080


- 1.DUC is Defined as Device Under Calibration.
- 2.Calibration Frequency decided by the customer.
- 3.The above instrument is working in good condition.

Calibrated By:


C.AKASH
(CALIBRATION ENGINEER)



Authorised by:


S. LAKSHMANAN MURUGAN,
Technical Manager
Vanavil Calibrations Pvt Ltd.

Vanavil Calibrations Pvt. Ltd

(A Unit of Rainbow Bio Medical Engineers)

S2, Rishi Maharaj Apartment, Indira Nagar, 250 Reddiyur Main Road, Narasothipatty, Salem - 636 004

Cell: 99949 13872 / 99949 23872 Ph: 0427-7965376

Web : vanavilcalibrations.com | Email : vanavilcalibrations@gmail.com



Vanavil Calibrations
Make It Simple, But Significant!

CALIBRATION CERTIFICATE

Page no: 1 of 1

Customer Name & Address: GOVT PRIMARY HEALTH CENTRE, PUDUPATTU - 632 508.	SRF No :	VCPL/22-23 /06-01/25-03-2023
	Date of Issue :	27/Mar/2023
	Date of Receipt :	25/Mar/2023
	Date of Calibration :	25/Mar/2023
	Cal Due Date :	24/Mar/2024
	Calibration at	IN LAB

Details of Device Under Calibration:

Description:	MICRO PIPETTE	Make :	-
Range:	0-1000 μ l	Model/Type:	MICROLUX
Resolution:	10 μ l	Accuracy :	
Serial Number:		Instrument Location:	LAB
ID number:	-	Condition of DUC:	GOOD

Temperature	24.8 °C	National/International standard:	-
Humidity	52 % Rh	Cal procedure no:	-

Master Details


SL no:	Description	Serial No	Make/Model	Certificate No	Valid Till
1	ELECTRONIC BALANCE	16031172	WINTECH / -	E150323-3-1	15/Mar/24

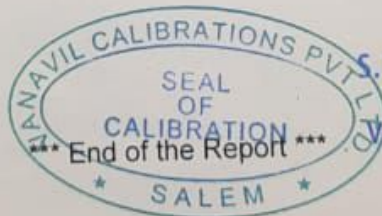
CALIBRATION RESULT

S.NO	DUC Readings (μ l)	Standard Rreadings Mean Value (mg)	ERROR (μ l)
1	10	9.93	0.070
2	500	499.88	0.120
3	1000	998.92	1.080


- 1.DUC is Defined as Device Under Calibration.
- 2.Calibration Frequency decided by the customer.
- 3.The above instrument is working in good condition.

Calibrated By:


C.AKASH
(CALIBRATION ENGINEER)



Authorised by:


S. LAKSHMANAN MURUGAN,
Technical Manager
Vanavil Calibrations Pvt Ltd.

Vanavil Calibrations Pvt. Ltd

(A Unit of Rainbow Bio Medical Engineers)

S2, Rishi Maharaj Apartment, Indira Nagar, 250 Reddiyur Main Road, Narasothipatty, Salem - 636 004

Cell: 99949 13872 / 99949 23872 Ph: 0427-7965376

Web : vanavilcalibrations.com | Email : vanavilcalibrations@gmail.com