
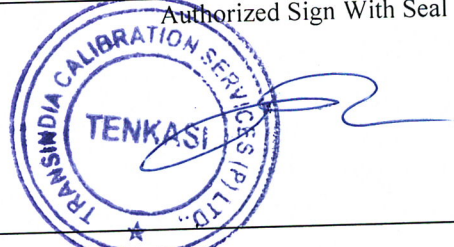


CALIBRATION / TESTING REPORT			
CUSTOMER DETAILS: GOVT.PRIMARY HEALTH CENTRE SATHARASANKOTTAI, SIVAGANGAI.		CERTIFICATE NO	TICS/2023/MM/SG/08
		EQUIPMENT NAME	MICROSCOPE
		MANUFACTURE	LABOMED
		MODEL	VISION 2000
CALIBRATION DATE	27/09/2023	SERIAL NO	211133674
CALIBRATION DUE DATE	26/09/2024	INSTALLED DEPARTMENT	LAB
LOCATION OF CALIBRATION	SITE	ASSET NUMBER	SKLAB-008
1. General maintenance required		<input type="checkbox"/> Yes	<input checked="" type="checkbox"/> No
2. Any Physical damage observed		<input type="checkbox"/> Yes	<input checked="" type="checkbox"/> No
3. Spare Replacement (if required)		<input type="checkbox"/> Yes	<input checked="" type="checkbox"/> No
TEST EQUIPMENT	MANUFACTURE	SERIAL NUMBER	CERTIFICATE NUMBER/VALIDITY
ELECTRICAL SAFTY ANALYZER	DATREND/ V Pad-mini	VPM 18040011	ACCS221441/28-07-2023
*The above mentioned instrument has been tested using standards manufactures recommended protocols, using equipment having traceability to National/International standards.			
<input checked="" type="checkbox"/> ACCEPTABLE FOR USE <input type="checkbox"/> CORRECTIVE MAINTENANCE REQUIRED <input type="checkbox"/> REMOVED FROM USE			
Calibrated By :		Authorized Sign With Seal	
			

*Electrical safety test result attached

CALIBRATION / TESTING REPORT				
CUSTOMER DETAILS : GOVT.PRIMARY HEALTH CENTRE SATHARASANKOTTAI, SIVAGANGAI.		CERTIFICATE NO		TICS/2023/MM/SG/08
		EQUIPMENT NAME		MICROSCOPE
		MANUFACTURE		LABOMED
		MODEL		VISION 2000
CALIBRATION DATE	27/09/2023	SERIAL NO		211133674
CALIBRATION DUE DATE	26/09/2024	INSTALLED DEPARTMENT		LAB

TEST REPORT –Electrical Safety

Test Standard: IEC 62353

Parameter	Units	Value	Limits	Status
Main Voltage L1-L2	V	232.5	240±10	PASS
Main Voltage L1-G(PE)	V	232.1	240±10	PASS
Main Voltage L2-G(PE)	V	0.6	<5	PASS
Load Current	A	0.204	As per unit	PASS
Protective Earth Resistance	Ω	0	<0.3	PASS
Point-to-Point Resistance	Ω	0	<0.5	PASS
Equipment Leakage	μA	0.15	Class I - < 500 Class II - < 100	PASS
Applied Part Leakage	μA	0	Type BF - < 5mA Type CF- <50μA*	PASS

* Note: Defibrillator paddles 100 μA, per IEC 60601-2-4

The above mentioned instrument has been tested using standards manufactures recommended protocols, using equipment having traceability to National/International standards.

