

TECHNICAL RESOURCES

SALES, REPAIRS, AMC & FRANCHISE SERVICES OF ANALYTICAL, PRECISION, BIO-MEDICAL, BLOOD BANKING, IVF & HISTOPATHOLOGY LABORATORY EQUIPMENT.

A MSME Registered Unit, NSIC-CRISIL Rated SE 3C
A NABL Accredited Laboratory



CC-2112

Mob. : 9819327149
Email : info@technical-resources.in
technicalresources@gmail.com
Handset : 9819103181
Webpage : www.technical-resources.in

SERVICE CENTRE : OFFICE NO. 2, M D TONES PARADISE, OPP. NEW PEDESTRAIN BRIDGE, NAVAGAON, DAHISAR (W), MUMBAI - 400 068.

Calibration Certificate

Calibration field: Mechanical-RPM Accreditation valid upto: 11.04.2024 Requisition no: Sep2023-124 Calibration done at: At Site	NABL Accreditation no: CC-2112 Certificate no: TR/2023/RPM/237 ULR no: CC211223000003208 Date of calibration: 29.09.2023 Agreed Next Calib On: 28.09.2024 Page no: 1 of 2
Customer details: Name: Vital Digital Healthcare Pvt Ltd Address: B-103, Royal Classic, New Link Road, Next to City Mall, Andheri West, Mumbai - 400053	Reference used: Master: Tachometer DT-2001B Master Ser. No.: Q33442 ID No. RM002 Traceable Certificate: M-230801-19-5 Valid upto: 16.08.2024 Calibrated at: Godrej CC-2634
Details of DUC: Equipment: Centrifuge Make: Remi Model: R8C Plus Serial No.: ZEGN-22387 ID No.: Not Specified Location: Pathology	Condition of item: Good Range RPM: Not Specified Accuracy: Not Specified Resolution (RPM): 1
Ambient Temp(*C): 25+/- 2 Humidity Rh(%): 50 +/-20	


Remark:

1. Calibration procedure used: LAB-SOP/08
2. The Reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $K=2$, providing a level of confidence of approx. 95%.
3. The observations reported represent values at the time of measurement. They do not convey any long term stability information.
4. The standards maintained are traceable to National / International Standards through accredited laboratories.
5. Sticker affixed on the unit

Note:

1. This certificate refers only to the particular instrument submitted for calibration.
2. This certificate shall not be reproduced.
3. Technical Resources shall not be responsible for any change in calibration date and performance specification on account of malfunctioning of the instrument due to damage caused to it after handing over it to the customer.
4. Any queries for the calibration certificate will be clarified only if raised within 30 days from the date of issue. The reissue of certificate after 30 days will be chargeable.

Authorised Signatory
Sr Technical Manager
N Srinivas Rao

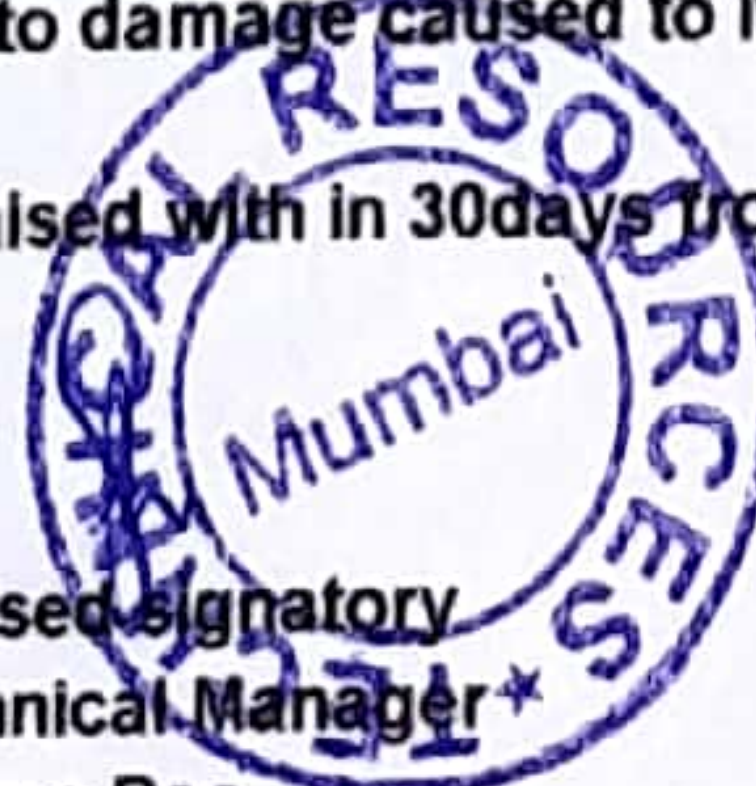

F.7.8.4

TECHNICAL RESOURCES

SALES, REPAIRS, AMC & FRANCHISE SERVICES OF ANALYTICAL, PRECISION, BIO-MEDICAL, BLOOD BANKING, IVF & HISTOPATHOLOGY LABORATORY EQUIPMENT.

A MSME Registered Unit, NSIC-CRISIL Rated SE 3C
A NABL Accredited Laboratory



CC-2112

Mob. : 9819327149
Email : info@technical-resources.in
technicalresources@gmail.com
Handset : 9819103181
Webpage : www.technical-resources.in

SERVICE CENTRE : OFFICE NO. 2, M D TONES PARADISE, OPP. NEW PEDESTRAIN BRIDGE, NAVAGAON, DAHISAR (W), MUMBAI - 400 068.

Calibration data:

Equipment:	Centrifuge	Certificate no:	TR/2023/RPM/237
Serial no:	ZEGN-22387	ULR no:	CC211223000003208
ID no.	Not Specified	Date of calibration:	29.09.2023
		Page No:	2 of 2

RUN DETAILS

Set RPM Display	Avg. Reading on UUC Display RPM	Avg. Reading On Ref. RPM	Deviation in RPM (+/-)	Expanded Uncertainty in RPM (+/-)
1500	1500	1504.6	-4.6	7.1
3000	3000	3006.1	-6.1	7.0
4000	4000	4002.2	-2.2	7.1

END OF RESULT

03.10.2023
Certificate Issue Date:

Dilip
Checked By

Authorised signatory
Sr Technical Manager
N Srinivas Rao



F.7.8.4