

## CALIBRATION CERTIFICATE

Page no: 1 of 1

<b>Customer Name &amp; Address:</b> M/S GOVERNMENT PRIMARY HEALTH CENTRE , THOLASAMPATTI - 636 503.	Certificate No:	VCPL/CC/23-24/36-002
	Date of Calibration:	05-10-2023.
	Date of issue:	06-10-2023
	Date of Receipt:	05-10-2023
	Next cal Date:	04-10-2024

### Details of Device Under Calibration

Description:	MICROPIPETTE	Make:	THERMO SCIENTIFIC
Range:	10 - 100 µl	Model/Type:	FINNPIPETTE F3
Resolution:	0.2 µl	Condition of DUC	GOOD
Serial Number	RW09117	Location:	LABORATORY
ID number	TGPHC/MP/01	Cal. At:	LAB
<b>Environmental Conditions</b>		<b>Calibration Method Used</b>	
Temperature	23.5 °C	Calibration Method Used	ISO 8655-2002 PART-6
Humidity	51 % Rh	Cal procedure no:	-

### Master Details

SL no:	Description	ID No / SL No	Certificate No	Make/Model	Valid Till
1	ELECTRONIC BALANCE	16031172	E-150323-1	WINTech	15-03-2024

### RESULT OF CALIBRATION


S.NO	Duc Readings ( µl )	Standard Reading Mean Value ( mg )	ERROR (mg)
1	10.0	10.02	-0.02
2	50.0	49.94	0.06
3	100.0	99.87	0.13

**Remarks:**

1. DUC is Defined as Device Under Calibration.
2. Calibration Frequency decided by the customer.
3. The above instrument is working in good condition.

Calibrated By

**R.GOPALAKRISHNAN**  
(CALIBRATION ENGINEER)

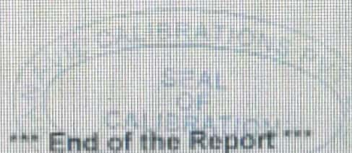

Authorised by:

*T. Sudhakar*  
**T. SUDHAKAR,**  
Technical Manager  
Vanavil Calibrations Private Limited