



Vanavil Calibrations
Make It Simple, But Significant!

CALIBRATION CERTIFICATE

Page : 1 of 1

Customer Name & Address: M/S GOVERNMENT PRIMARY HEALTH CENTRE, THOLASAMPATTI - 636 503.	Certificate No:	VCPL/CC/23-24/36-001
	Date of Calibration:	05-10-2023
	Date of Issue:	06-10-2023
	Date of Receipt:	05-10-2023
	Next cal Date:	04-10-2024

Details of Device Under Calibration

Description	CENTRIFUGE	Make:	ROTEK
Range	100 to 3500 RPM	Model/Type:	-
Resolution	10 RPM	Condition of DUC:	GOOD
Serial No / Id.No	RMCA1 / TGPHC/CEN-01	Instrument Location:	LABORATORY

Environmental Conditions

Temperature	23.4 °C	Reference Standard No	SANAS TR4501
Humidity	52 % Rh	Calibration Procedure No	-

Method Used For Calibration

Details of Reference Standard Equipment For Calibration

S.No	Description	ID No / SL No	Certificate No	Validity
1	DIGITAL TACHOMETER	DTM-01	HT/CC/221202-03/005 SYSTEMS/ HTM 560	4-Dec-23


Calibration Result

S.No	DUC Reading (RPM)	Standard Reading (RPM)	Error (RPM)	Measurement Uncertainty (RPM)
1	500	499.8	0.2	12
2	1000	1001	-1	12
3	2000	1999	1	12
4	3000	2998	2	12
5	3500	3492	8	12


Remarks:


1. DUC is Defined as Device Under Calibration.
2. Calibration Frequency decided by the customer.
3. The above instrument is working in good condition.

Calibrated By:


R. GOPALAKRISHNAN
(CALIBRATION ENGINEER)

Authorised by:


T. SUDHAKAR
Technical Manager
Vanavil Calibrations Pvt Ltd.

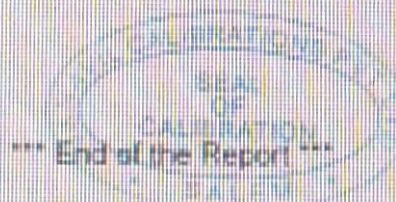

Vanavil Calibrations Pvt. Ltd

(A Unit of Rainbow Bio Medical Engineers)

52, Bala Mahaling Apartment, Indra Nagar, 250 Reddyar Main Road, Narasimhapatti, Salem - 636 004.

No. 95,97,98, Anandamaya Apartments, 2nd Floor, KVR Road, 2nd Cross Street, Thangam Nagar, Pallikarantal, Chennai - 600 100.

Call: 99949 23872 / 99949 23873 Ph: 0427-7965376

• vanavilcalibrations@gmail.com • www.rainbowbiomedicalengineers.com | www.vanavilcalibrations.com