


# L J CHART- GLUCOSE

Mean : 115 mgs/dl

CMC-IQC

Govt. Primary Health Centre - Keeripatti - phc. Sep. 2023

Range : 105 to 125 mgs/dl

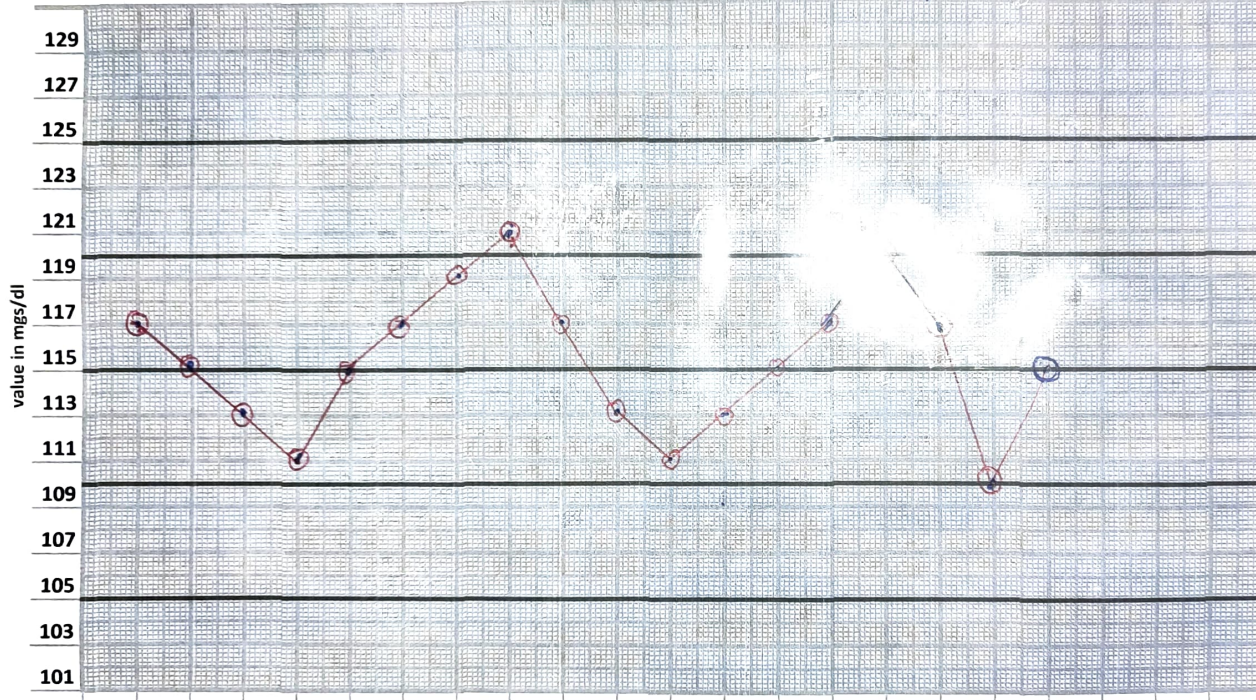

|                            |     |
|----------------------------|-----|
| Max. Value                 | 125 |
| Mean Value                 | 115 |
| 2SD (1SD x 2)              | 10  |
| 2SD for Analyte (Mean+2SD) | 125 |

|                            |     |
|----------------------------|-----|
| Max. Value                 | 125 |
| Mean Value                 | 115 |
| 1SD (Max-Mean)/2)          | 5   |
| 1SD for Analyte (Mean+1SD) | 120 |

|                               |     |
|-------------------------------|-----|
| Min. Value                    | 105 |
| Mean Value                    | 115 |
| (-1)SD (Min-Mean)/2)          | 5   |
| (-1)SD for Analyte (Mean-1SD) | 110 |

|                               |     |
|-------------------------------|-----|
| Min. Value                    | 105 |
| Mean Value                    | 115 |
| (-2)SD (1SD x 2)              | 10  |
| (-2)SD for Analyte (Mean-2SD) | 105 |

| Result | 117 | 115 | 113 | 111 | 117 | 119 | 121 | 117 | 113 | 111 | 117 | 120 | 117 | 110 |  |  |  |  |  |  |
|--------|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|-----|--|--|--|--|--|--|
| Date   | 18  | 19  | 20  | 21  | 22  | 23  | 24  | 25  | 26  | 27  | 28  | 29  | 30  |     |  |  |  |  |  |  |

Precison 12

*Indu.*  
 MEDICAL OFFICER  
 Govt. Primary Health Centre,  
 KEERIPATTY (Po),  
 Attur (Tk), Salem (Dt) - 636 107