

CALIBRATION CERTIFICATE

Page no: 1 of 1

Customer Name & Address: M/S GOVERNMENT PRIMARY HEALTH CENTRE, RISHIVANDIYAM ROAD, KATTUEDAIYAR. KALLAKURICHI - 605 751.		Certificate No:	VCPL/CC/23-24/41 -001
		Date of Calibration:	30-Sep-2023
		Date of issue:	3-Oct-2023
		Date of Receipt:	30-Sep-2023
		Next cal Date:	29-Sep-2024
Details of Device Under Calibration			
Description:	SEMI AUTO ANALYZER	Make:	ROBONIK
Range:	-	Model/Type:	PRIETEST TOUCH
Resolution:	-	Condition of DUC	GOOD
Serial Number	AT110207MRK	Location:	LABORATORY
ID number	-	Cal. At:	ONSITE
Environmental Conditions		Calibration Method Used	
Temperature	25.2 °C	National/International standard:	IEC60601-1
Humidity	49 % Rh	Cal procedure no:	-

Master Details

SL no	Description	ID No / SL No	Certificate No	Make/Model	Valid Till
1	Electrical Safety Analyzer	6014025	ACCS230581	FLUKE/ESA-612	9-Mar-24

Electrical Safety Report

S.NO	PARAMETERS	MEASURED VALUES μ A	ALLOWABLE LIMITS μ A
1	Earth Leakage	121.4	<5000 μ A For B,BF,CF
		MEASURED VALUES μ A	ALLOWABLE LIMITS μ A
2	Enclosure Leakage	186.5	<5000 μ A For B,BF,CF

Remarks:

- 1.DUC is Defined as Device Under Calibration.
- 2.Calibration Frequency decided by the customer.
- 3.The above instrument is working in good condition.


Calibrated By:


C.AKASH

(CALIBRATION ENGINEER)

Authorised by:


S. LAKSHMANAN MURUGAN,
Technical Manager
Vanavil Calibrations Pvt Ltd.

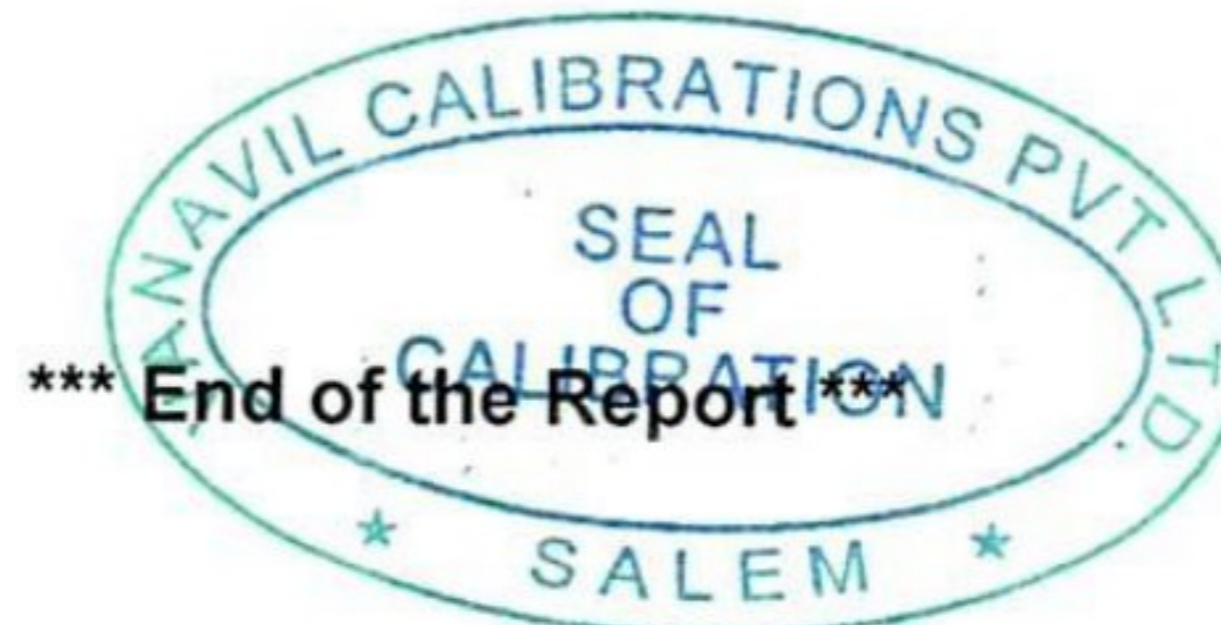

Vanavil Calibrations Pvt. Ltd

(A Unit of Rainbow Bio Medical Engineers)

S2, Rishi Maharaj Apartment, Indra Nagar, 250 Reddiyur Main Road, Narasothipatty, Salem - 636 004.

No. 96,97,98, Anadhamaya Apartments, 2nd Floor, KVR Flats, 2nd Cross Street, Thangam Nagar, Pallikaranai, Chennai - 600 100.

Cell: 99949 13872 / 99949 23872 Ph: 0427-7965376

✉ vanavilcalibrations@gmail.com 🌐 www.rainbowbiomedicalengineers.com | www.vanavilcalibrations.com