

## CALIBRATION CERTIFICATE

Page no: 1 of 1

<b>Customer Name &amp; Address:</b> M/S GOVERNMENT PRIMARY HEALTH CENTRE , RISHIVANDIYAM ROAD , KATTUEDAIYAR. KALLAKURICHI - 605 751.	Certificate No:	VCPL/CC/23-24/41 -002
	Date of Calibration:	30-Sep-2023
	Date of issue:	3-Oct-2023
	Date of Receipt:	30-Sep-2023
	Next cal Date:	29-Sep-2024

Details of Device Under Calibration			
Description:	MICROSCOPE	Make:	LABOMED
Range:	-	Model/Type:	-
Resolution:	-	Condition of DUC	GOOD
Serial Number	170699569	Location:	LABORATORY
ID number	-	Cal. At:	ONSITE
Environmental Conditions		Calibration Method Used	
Temperature	25.3 °C	National/International standard:	IEC60601-1
Humidity	50 % Rh	Cal procedure no:	-

### Master Details

SL no	Description	ID No / SL No	Certificate No	Make/Model	Valid Till
1	Electrical Safety Analyzer	6014025	ACCS230581	FLUKE/ESA-612	9-Mar-24

### Electrical Safety Report

S.NO	PARAMETERS	MEASURED VALUES $\mu$ A	ALLOWABLE LIMITS $\mu$ A
1	Earth Leakage	122.3	$<5000\mu$ A For B,BF,CF
		MEASURED VALUES $\mu$ A	ALLOWABLE LIMITS $\mu$ A
2	Enclosure Leakage	185.4	$<5000\mu$ A For B,BF,CF

**Remarks:**

- 1.DUC is Defined as Device Under Calibration.
- 2.Calibration Frequency decided by the customer.
- 3.The above instrument is working in good condition.

Calibrated By:


  
C.AKASH

(CALIBRATION ENGINEER)

Authorised by:

  
S. LAKSHMANAN MURUGAN,  
Technical Manager  
Vanavil Calibrations Pvt Ltd.

\*\*\* End of the Report \*\*\*

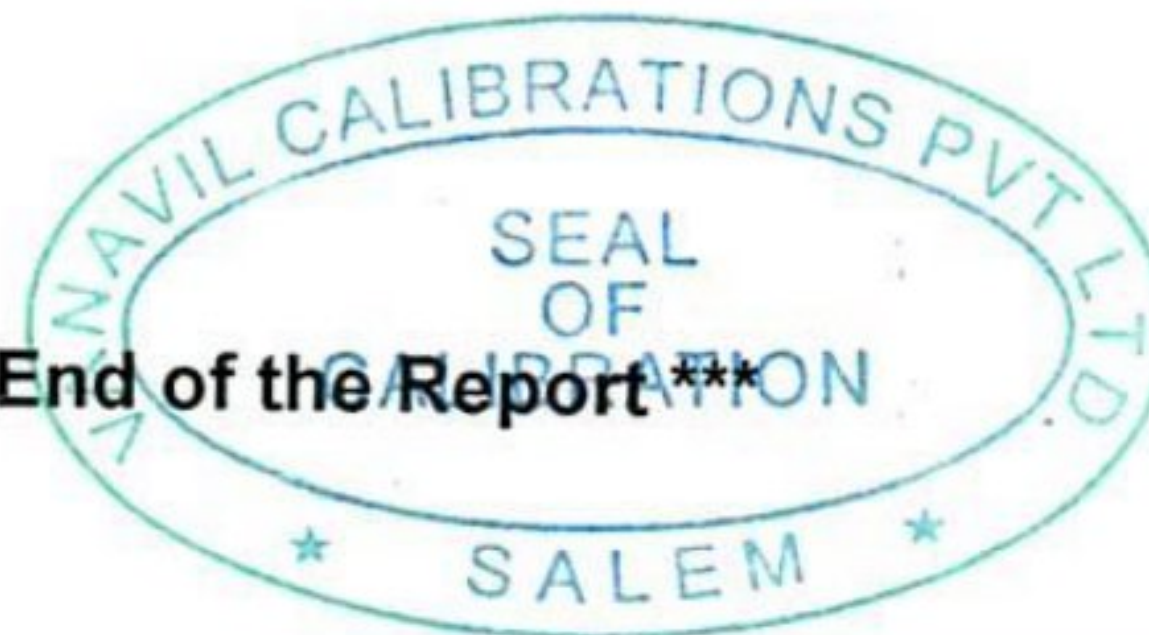

## Vanavil Calibrations Pvt. Ltd

(A Unit of Rainbow Bio Medical Engineers)

S2, Rishi Maharaj Apartment, Indra Nagar, 250 Reddiyar Main Road, Narasothipatty, Salem - 636 004.

No. 96,97,98, Anadhamaya Apartments, 2<sup>nd</sup> Floor, KVR Flats, 2<sup>nd</sup> Cross Street, Thangam Nagar, Pallikaranai, Chennai - 600 100.

Cell: 99949 13872 / 99949 23872 Ph: 0427-7965376

✉ vanavilcalibrations@gmail.com 🌐 www.rainbowbiomedicalengineers.com | www.vanavilcalibrations.com