

CALIBRATION CERTIFICATE

Page no: 1 of 1

Customer Name & Address: M/S GOVERNMENT PRIMARY HEALTH CENTRE , P RISHIVANDIYAM ROAD , KATTUEDAIYAR. KALLAKURICHI - 605 751.		Certificate No:	VCPL/CC/23-24/41 -005
		Date of Calibration:	30-Sep-2023
		Date of issue:	3-Oct-2023
		Date of Receipt:	30-Sep-2023
		Next cal Date:	29-Sep-2024
Details of Device Under Calibration			
Description:	MICROPIPETTE	Make:	MICROLUX
Range:	(5 to 50) µl	Model/Type:	-
Resolution:	1 µl	Condition of DUC	GOOD
Serial Number	-	Location:	LABORATORY
ID number	GPHC/LAB/MP-02	Cal. At:	LAB
Environmental Conditions		Calibration Method Used	
Temperature	23.5 °C	Calibration Method Used	ISO 8655:2002 PART-6
Humidity	52 % Rh	Cal procedure no:	-

Master Details

SL no:	Description	ID No / SL No	Certificate No	Make/Model	Valid Till
1	ELECTRONIC BALANCE	16031172	E-150323-1	WINTECH	15-03-2024

RESULT OF CALIBRATION

S.NO	Duc Readings (µl)	Standard Reading Mean Value (mg)	ERROR (mg)
1	5	4.94	0.06
2	25	24.89	0.11
3	50	49.83	0.17

Remarks:

- 1.DUC is Defined as Device Under Calibration.
- 2.Calibration Frequency decided by the customer.
- 3.The above instrument is working in good condition.

Calibrated By:

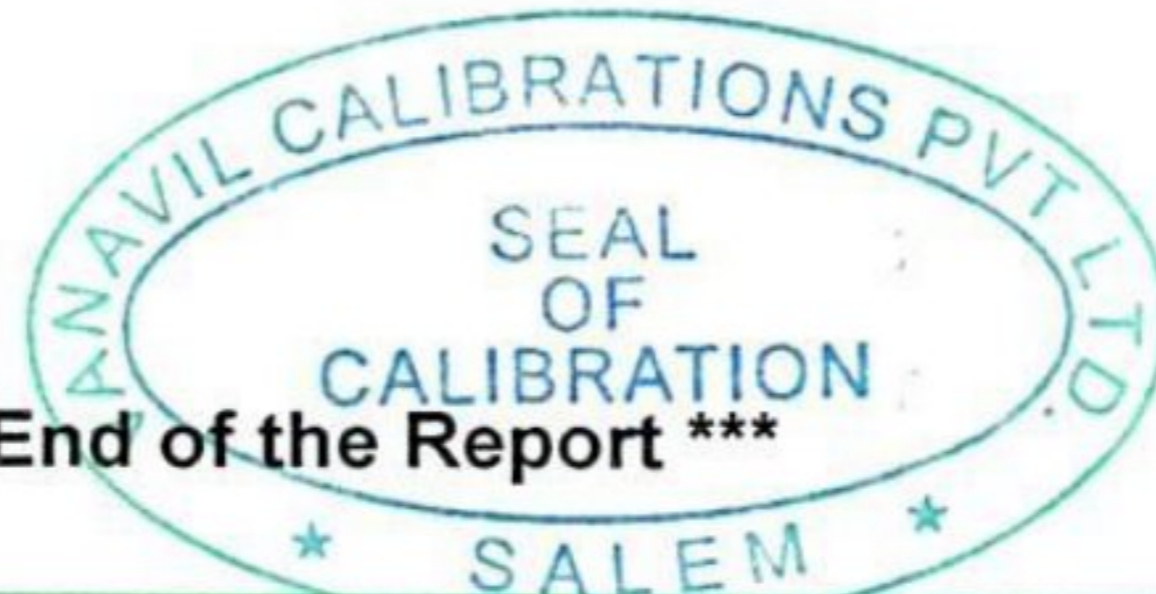

C.AKASH

(CALIBRATION ENGINEER)

Authorised by:


S. LAKSHMANAN MURUGAN,
Technical Manager
Vanavil Calibrations Pvt Ltd.

*** End of the Report ***



Vanavil Calibrations Pvt. Ltd

(A Unit of Rainbow Bio Medical Engineers)

S2, Rishi Maharaj Apartment, Indra Nagar, 250 Reddiyur Main Road, Narasothipatty, Salem - 636 004.

No. 96,97,98, Anadhamaya Apartments, 2nd Floor, KVR Flats, 2nd Cross Street, Thangam Nagar, Pallikaranai, Chennai - 600 100.

Cell: 99949 13872 / 99949 23872 Ph: 0427-7965376

✉ vanavilcalibrations@gmail.com 🌐 www.rainbowbiomedicalengineers.com | www.vanavilcalibrations.com