



Vanavil Calibrations

Make It Simple, But Significant !

CALIBRATION CERTIFICATE

Page no: 1 of 1

Customer Name & Address: M/S GOVERNMENT URBAN PRIMARY HEALTH CENTER , DEVAKOTTAI , SIVAGANGAI - 630 302.	Certificate No:	VCPL/CC/23-24/33-002
	Date of Calibration:	03-10-2023
	Date of issue:	04-10-2023
	Date of Receipt:	03-10-2023
	Next cal Date:	02-10-2024

Details of Device Under Calibration

Description:	SEMI AUTO ANALYZER	Make:	ROBONIK
Range:	-	Model/Type:	PRIETEST TOUCH
Resolution:	-	Condition of DUC	GOOD
Serial Number	AT0771214 RBK	Location:	LABORATORY
ID number	-	Cal. At:	ONSITE
Environmental Conditions		Calibration Method Used	
Temperature	25.2 °C	National/International standard:	IEC60601-1
Humidity	49 % Rh	Cal procedure no:	-

Master Details

SL no:	Description	ID No / SL No	Certificate No	Make/Model	Valid Till
1	Electrical Safety Analyzer	6014025	ACCS230581	FLUKE/ESA-612	9-Mar-24

Electrical Safety Report


S.NO	PARAMETERS	MEASURED VALUES μ A	ALLOWABLE LIMITS μ A
1	Earth Leakage	129.5	<5000 μ A For B,BF,CF
		MEASURED VALUES μA	ALLOWABLE LIMITS μA
2	Enclosure Leakage	197.5	<5000 μ A For B,BF,CF

Remarks:


- 1.DUC is Defined as Device Under Calibration.
- 2.Calibration Frequency decided by the customer.
- 3.The above instrument is working in good condition.

Calibrated By:


R.GOPALAKRISHNAN
(CALIBRATION ENGINEER)

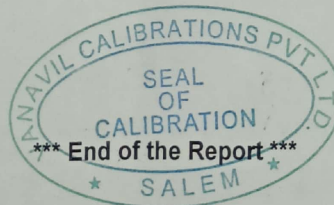

Authorised by:


M. BALAJI,
Quality Manager
Vanavil Calibrations Pvt Ltd.

Vanavil Calibrations Pvt. Ltd

(A Unit of Rainbow Bio Medical Engineers)

S2, Rishi Maharaj Apartment, Indra Nagar, 250 Reddiyur Main Road, Narasothipatty, Salem - 636 004.

No. 96,97,98, Anadhamaya Apartments, 2nd Floor, KVR Flats, 2nd Cross Street, Thangam Nagar, Pallikaranai, Chennai - 600 100.

Cell: 99949 13872 / 99949 23872 Ph: 0427-7965376

vanavilcalibrations@gmail.com  www.rainbowbiomedicalengineers.com | www.vanavilcalibrations.com



Scanned with OKEN Scanner