

CALIBRATION REPORT

Report No : HBMS/CAL/23-24	Calibration Date : 03.10.2023
	Calibration valid : 02.04.2024

1.1. CUSTOMER DETAILS:

Name and Address of the organization	M/s, URBAN GOVERNMENT PRIMARY HEALTH CENTRE, GUGAI, SALEM CORPORATION, SALEM.
--------------------------------------	---

1.2. DESCRIPTION OF DEVICE UNDER TEST (DUT):

EQUIPMENT NAME		MICRO PIPETTE
i	Manufactured by	THERMO SCIENTIFIC
ii	Model	FINE PIPETE F3
iii	Value	100µl-1000µl
iv	Serial No	RW11597

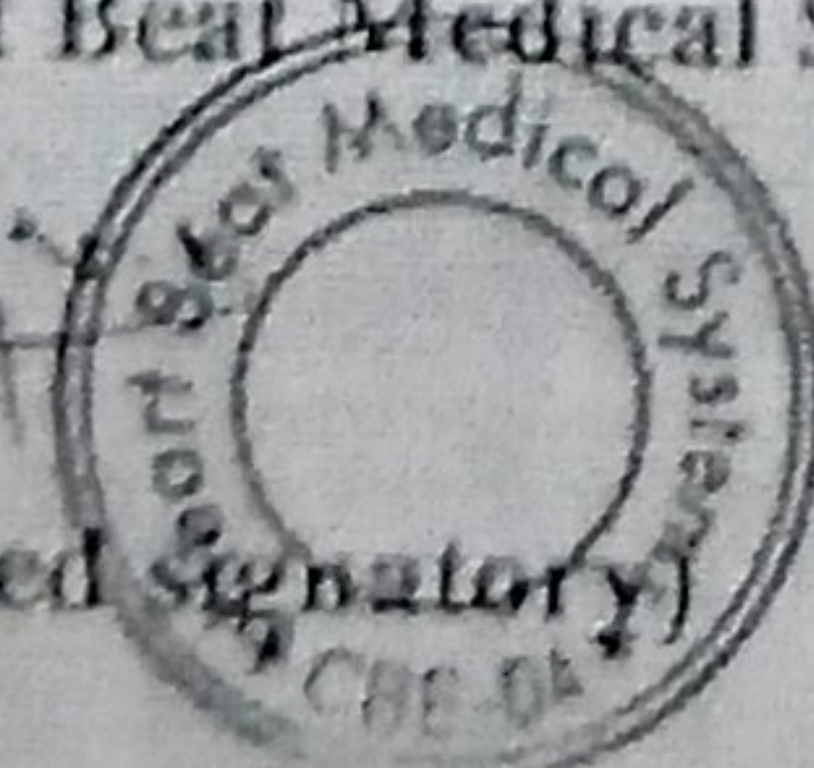
Calibration standards used :

Master instrument	Model	Serial no	Date of calibration	Calibration due on
Electrical compact scale	SF-400C	SF400-2240	07-OCT-2022	06-OCT-2023

Calibration test Report.

Number of measurement	Channel 1 (Volume)		
	100µl	500µl	1000µl
1	100.01	500.05	1000.01
2	100.01	500.01	1000.04
3	100.04	500.05	1000.07
4	100.02	500.09	1000.08
5	100.02	500.05	1000.12
6	100.05	500.07	1000.04

For Heart Beat Medical Systems,

[Signature]
 (Authorized Signatory)


CALIBRATION REPORT

Report No - HBMS/CAL/23-24	Calibration Date : 03 10 2023 Calibration valid : 02 04 2024
I.1. CUSTOMER DETAILS:	
Name and Address of the organization	M/s, URBAN GOVERNMENT PRIMARY HEALTH CENTRE , GUGAI, SALEM CORPORATION, SALEM.
I.2. DESCRIPTION OF DEVICE UNDER TEST (DUT):	
EQUIPMENT NAME	MICRO PIPETTE
i Manufactured by	THERMO SCIENTIFIC
ii Model	FINE PIPETE F3
iii Value	10 µl -100 µl
iv Serial No	RW09074

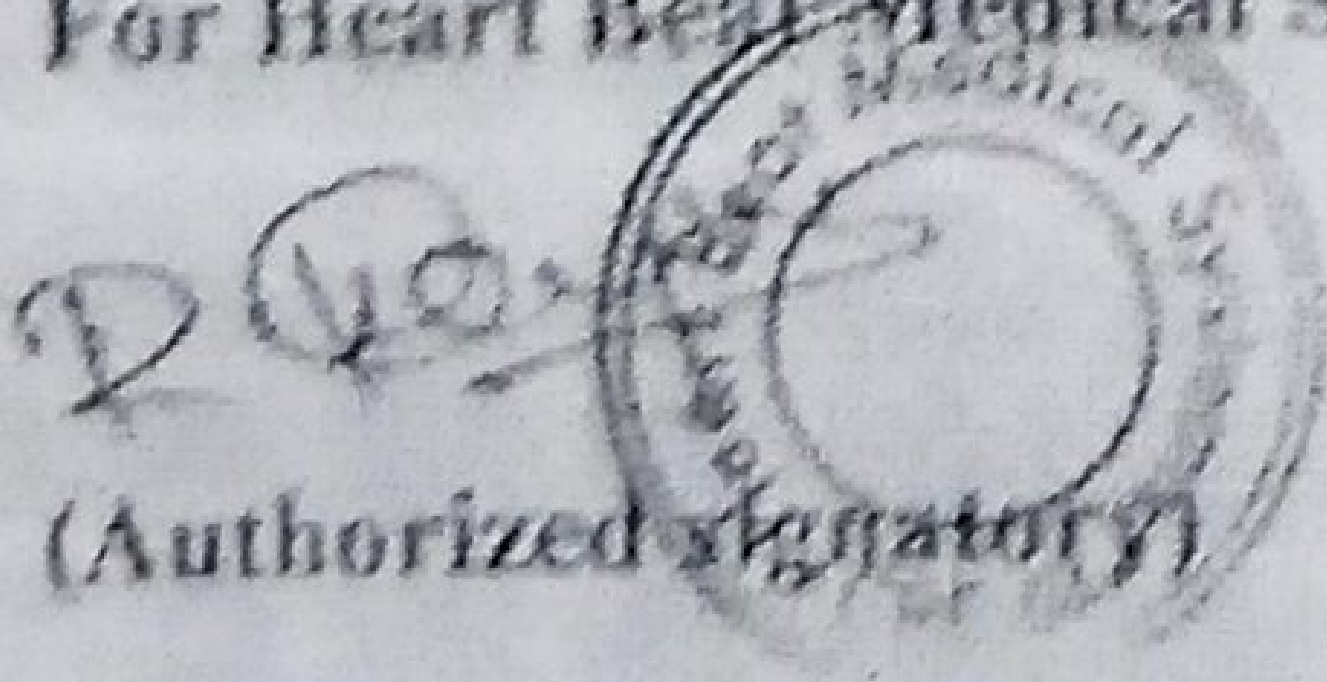
Calibration standards used :

Master instrument	Model	Serial no	Date of calibration	Calibration due on
Electrical compact scale	SF-400C	SF400-2240	07-OCT-2022	06-OCT-2023

Calibration test Report.

Number of measurement	Channel 1 (Volume)		
	10µl	50µl	100µl
1	10.02	50.03	100.03
2	10.02	50.04	100.02
3	10.00	50.02	100.01
4	10.02	50.02	100.05
5	10.00	50.02	100.04
6	10.02	50.02	100.02

For Heart Beat Medical Systems,


(Authorized signatory)