

CALIBRATION CERTIFICATE

Customer Name & Address: M/S GOVERNMENT PRIMARY HEALTH CENTRE , KANNANGUDI , SIVAGANGAI - 630 303.	Certificate No:	VCPL/CC/23-24/32-003
	Date of Calibration:	03-10-2023
	Date of issue:	04-10-2023
	Date of Receipt:	03-10-2023
	Next cal Date:	02-10-2024

Details of Device Under Calibration

Description	CENTRIFUGE	Make:	ELECTRIC CENTRIFUGE
Range	4000 RPM	Model/Type:	DALAL
Resolution	10 RPM	Condition of DUC:	GOOD
Serial No / Id.No	55824-53	Instrument Location:	LABORATORY

Enviromental Conditions

Method Used For Calibration

Temperature	23.4 °C	Reference Standard No	SANAS TR4501
Humidity	52 % Rh	Calibration Procedure No	-

Details of Reference Standard Equipment For Calibration

S.No	Description	ID No / SL No	Certificate No	Validity
1	DIGITAL TACHOMETER	DTM-01	HT/CC/221202-03/005 SYSTEMS/ HTM 560	4-Dec-23


Calibration Result

S.No	DUC Reading (RPM)	Standard Reading (RPM)	Error (RPM)	Measurement Uncertainty (RPM)
1	500	499.8	0.2	12
2	1000	1001	-1	12
3	2000	1999	1	12
4	3000	2998	2	12
5	4000	3996	4	12

Remarks:

- 1.DUC is Defined as Device Under Calibration.
- 2.Calibration Frequency decided by the customer.
- 3.The above instrument is working in good condition.


Calibrated By:


C.AKASH

(CALIBRATION ENGINEER)

Authorised by:


S. LAKSHMANAN MURUGAN,
Technical Manager
Vanavil Calibrations Pvt Ltd.

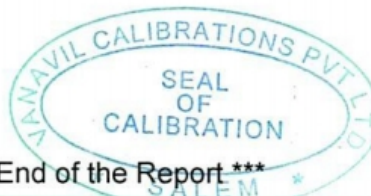

*** End of the Report ***