

22.Sep.2023 01:27 -0.098272 443.89134

23.Aug.2023 01:18 -0.099881 474.22076

Flags/Action

ALB2

Cf.a.s.

71219801


564995

71219801

564995

Result - Calibration ALB2 (Quantitative) - Detail

Cassette: ALB2 Lot No.: 71219801
Calibrator: Cf.a.s. Lot No.: 564995

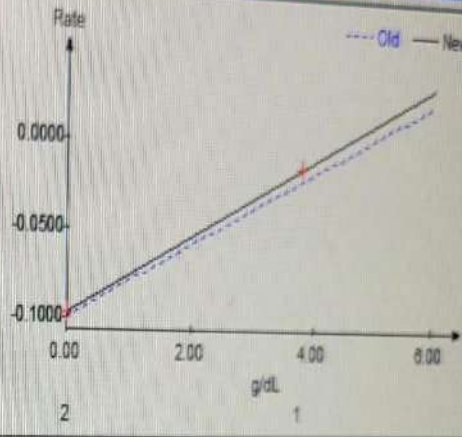

R0 F
-0.098272 443.89134

Std-1	Assign.	Calc.	Rate
RM:	3.8 g/dL	3.8	-0.0131 dA
<input checked="" type="checkbox"/> R1:		3.8	-0.0131 dA
<input checked="" type="checkbox"/> R2:		3.8	-0.0132 dA

Comment

9/22/2023 01:27

admin



Delete

Help

Print

Rate Info...



Accept

Print

Close

Aspartate Aminotrans. liquid

Next Cal. Due: None

Date Calibrated

R0

F

Flags/Action

ASTL

Cf.a.s.

21 Sep 2023 20:46

-0.000626

5826.3771

71009801

564995

23 Aug 2023 01:20

-0.000591

6032.3631

71671801

564995


Result - Calibration ASTL (Quantitative) - Detail

Cassette: ASTL

LotNo: 71009801

Calibrator: Cf.a.s.

LotNo: 564995

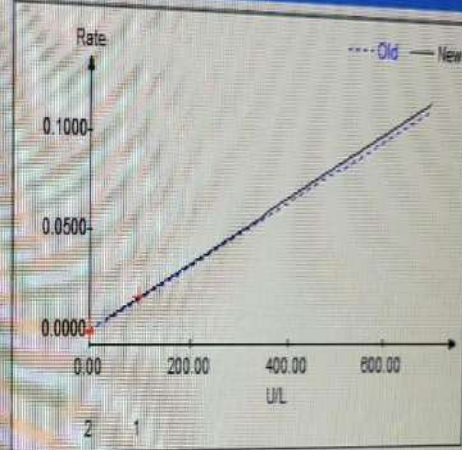

R0: -0.000626
F: 5826.3771

Std-1	Assign	Calc	Rate
	PM: 98.4 U/L	98.4	0.01626 dA
<input checked="" type="checkbox"/>	R1:	98.2	0.01622 dA
<input checked="" type="checkbox"/>	R2:	98.6	0.01631 dA

Comment

9/21/2023 20:46

admin

Navigation buttons: ↑, ↓, Delete, Accept, Help, Print, Paste Info, Close

Next Cal. Due: None

Date Calibrated	R0	F	Flags/Action	BILD2	C.f.a.s.
04 Oct 2023 03:42	0.0000306	1434.1421		69521001	564995
02 Oct 2023 03:03	-0.000036	1419.4905		69521001	564995
01 Oct 2023 03:45	0.0000502	1409.0700		69521001	564995

Result - Calibration BILD2 (Quantitative) - Detail


Cassette: BILD2 Lot No.: 69521001
Calibrator: C.f.a.s. Lot No.: 564995

Empty text area for notes or comments.

R0	F
0.0000306	1434.1421

Comment:

10/4/2023 03:42 admin

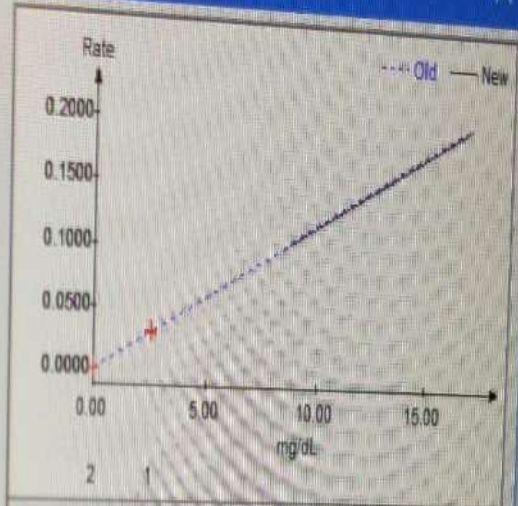

Std-1	Assign	Calc	Plate
RM:	2.57 mg/dL	2.57	0.03071 dA
<input checked="" type="checkbox"/> R1:		2.59	0.03085 dA
<input checked="" type="checkbox"/> R2:		2.56	0.03056 dA

	Delete	Help	Print	Reprint
	Accept	Rerun	Close	

Dilution Total Gen 3

Next Cal Due: None

Date Calibrated

R0

F

Flags/Action

BILT3

C.f.a.s.

04 Oct 2023 03:43

0.0010118

4021.1959

66986401

564995

21 Sep 2023 21:16

0.0009606

4004.5443

66986401

564995

Result - Calibration BILT3 (Quantitative) - Detail

Cassette

BILT3


Lot No: 66986401

Calibrator

C.f.a.s.

Lot No: 564995

Rate

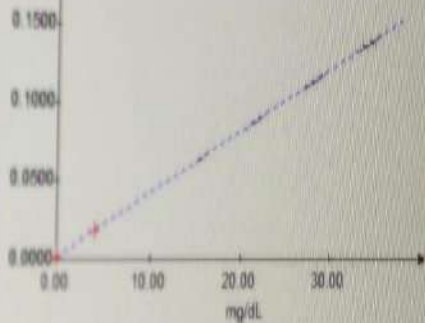

R0

F

0.0010118

4021.1959

Comment

Std-1

Assign

Calc

Rate

RM

41 mg/dL

41

0.01839 dA

R1

41

0.01836 dA

R2

41

0.01843 dA

10/4/2023 03:43

admin

Print

Rate Info

Delete

Help

Close

Accept

Renew

Date Calibrated	R0	F	Flags/Action	CHOL2	Cfas
02 Oct 2023 03:04	-0.000637	23.457420		69958701	564995
21 Sep 2023 21:17	-0.000162	22.651662		69958701	564995
23 Aug 2023 01:53	-0.000245	24.099990		69958701	564995


Result - Calibration CHOL2 (Quantitative) - Detail

Cessette: CHOL2 LotNo: 69958701
 Calibrator: Cfas LotNo: 564995

R0: -0.000637
 F: 23.457420


Comment:

10/02/2023 03:04 admin

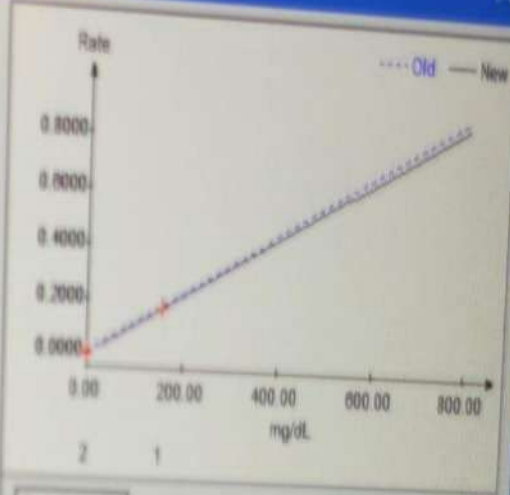

Std-1	Assign.	Calc.	Rate
RM	155 mg/dL	155	0.17074 dA
<input checked="" type="checkbox"/>	R1	155	0.17031 dA
<input checked="" type="checkbox"/>	R2	156	0.17117 dA

	Delete	Help	Print	Rate Info
	Accept	Cancel	Close	



Sample

Calibration

Quality Control

y Test

Cholesterol Gen 2

Next Cal. Due:

None

Date Calibrated

R0

F

Flags/Action

CHOL2

Clas.

02.Oct.2023 03:04

-0.000637

23.457420

69958701

564995

21.Sep.2023 21:17

-0.000162

22.651682

69958701

564995

23.Aug.2023 01:53

-0.000245

24.099980

69958701

564995


Result - Calibration CHOL2 (Quantitative) - Detail

Cassette: CHOL2

Lot No.: 69958701

Calibrator: Clas.

Lot No.: 564995

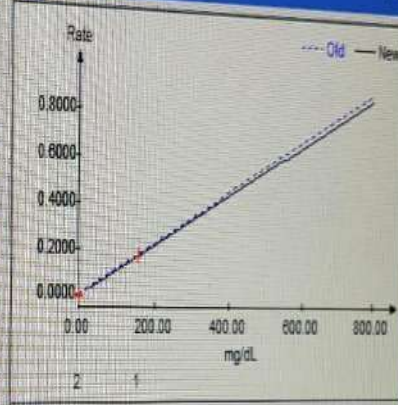

R0

F

-0.000637

23.457420

Std-1 Assign

Calc.

Rate

RM 155 mg/dL

155

0.17074 dA

R1

155

0.17031 dA

R2

156

0.17117 dA

Comment

10/2/2023 03:04

admin

Delete

Help

Print

Rate Info



Assign

Print

Close




HDL-C plus Gen.4 Next Cal. Due: None

Date Calibrated	R0	F	Flags / Action	HDLC4	CFASL
28.Sep.2023 11:06	0.0001892	12.703394		65818301	474723
05.Jun.2023 03:07	0.0002476	13.214900		63877601	474723

Result - Calibration HDLC4 (Quantitative) - Detail [X]

Cassette: HDLC4 Lot No.: 65818301
Calibrator: CFASL Lot No.: 474723

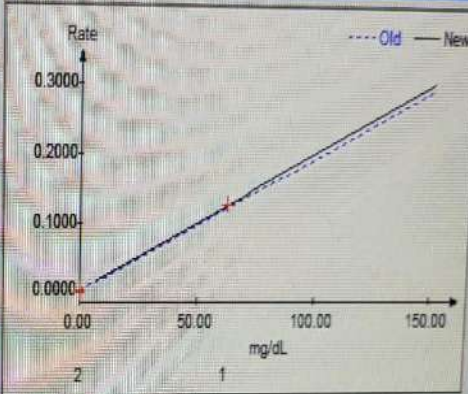

R0 F
0.0001892 12.703394

Comment: []


Std-1	Assign.	Calc.	Rate
	PM: 62 mg/dL	62	0.12693 dA
<input checked="" type="checkbox"/>	R1:	63	0.12782 dA
<input checked="" type="checkbox"/>	R2:	62	0.12604 dA

9/28/2023 11:06 admin

Navigation buttons: [Up Arrow] Delete [Help] [Print] [Rate Info] [Down Arrow] Accept [Return] [Close]

Result - Calibration LDLC3 (Quantitative) - Detail

Cassette: LDLC3 LotNo: 51974201
 Calibrator: CFASL LotNo: 474723

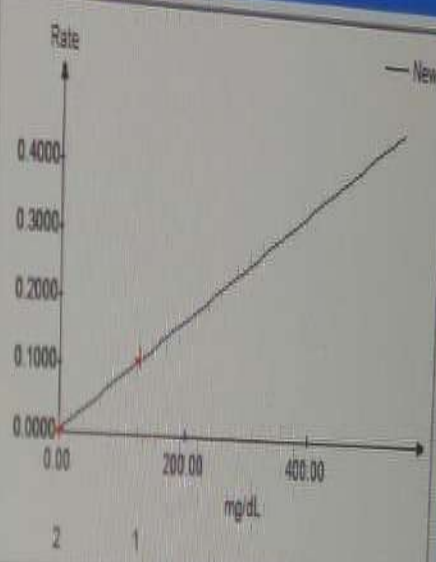

[Empty text area]

R0 F
 0.0007868 30.164927

Comment [Empty text box]

10/2/2021 13:15 admin

Std-1	Assign.	Calc.	Rate
RM	127 mg/dL	127	0.10985 dA
<input checked="" type="checkbox"/>	R1	127	0.11002 dA
<input checked="" type="checkbox"/>	R2	127	0.10968 dA

↑	Delete	Help	Print	Rate Info...
↓	Accept	Return	Close	



Date Calibrated	Next Cal. Due	None	Flags / Action	CRP4	CFASP
21.Sep.2023 12:57				71491801	530429
22.Jun.2023 07:15				70668101	530429

Result - Calibration CRP4 (Quantitative) - Detail

Cassette: CRP4 Lot No.: 71491801
 Calibrator: CFASP Lot No.: 530429

Std-1	Assign	Calc	Rate
RM	325.0 mg/L	325.0	0.50331 dA
<input checked="" type="checkbox"/> R1		314.6	0.49258 dA
<input checked="" type="checkbox"/> R2		335.4	0.50905 dA

Comment:

9/21/2023 12:57 admin