



CHRISTIAN MEDICAL COLLEGE

DEPARTMENT OF CLINICAL BIOCHEMISTRY
CMC EXTERNAL QUALITY ASSURANCE SCHEME
MONTHLY SUMMARY REPORT - APRIL 2023



PC-1024

Lab Name	Govt. Block PHC, Vellalore	Lab No	7091
Constituent Group	Chemistry III	Date of Result Entered :	19/04/2023
PT item	Lyophilized human serum based	Date of Report Published :	06/05/2023

Sl. No.	Test Name	Method	Instrument	Run No.	Result	Target	Delta	Delta 2	Delta 3	Delta 4
1	GLUCOSE III	GOD-POD III	Robonik (Semi automatic / Fully Automatic)	1832	119.45	6.04	7.21	117 mg/dL	-0.34	0.34
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik (Semi automatic / Fully Automatic)	1820	2.16	8.09	0.18	2.3 mg/dL	0.80	0.01
3	CHOLESTROL III	CHOD-PAP III	Robonik (Semi automatic / Fully Automatic)	1750	111.61	5.19	5.79	102 mg/dL	-1.66	0.28

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ± 1.01 to ± 2.00	Good.
Within ± 2.01 to ± 2.99	Accept with caution. Warning Signal.
Beyond ± 3.0	Unacceptable performance. Action Signal.


LAB ADDRESS :

Govt. Block PHC, Vellalore
The Block Medical Officer VELLALORE, Madurai District
Vellalore
TAMILNADU625109

Coordinator Contact Details:
Email: clinqc@cmcvellore.ac.in
Contact Number: 0416-2283102

Pamela Christudoss
Dr. Pamela Christudoss
CMC EQAS Coordinator
Christian Medical College, Vellore

Homogeneity and Stability of the sample is passed.
Data in CMC EQAS reports is confidential
CMC EQAS does not sub contract any components
***** End of Report *****

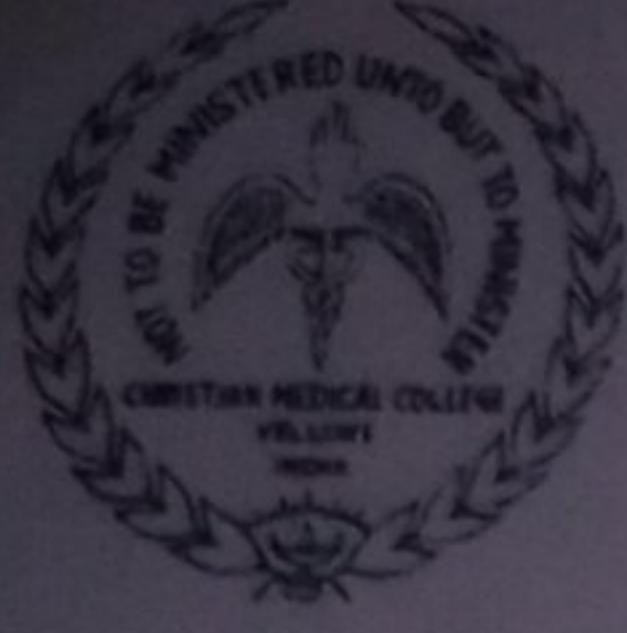

CHRISTIAN MEDICAL COLLEGE

DEPARTMENT OF CLINICAL BIOCHEMISTRY

CMC EXTERNAL QUALITY ASSURANCE SCHEME

MONTHLY SUMMARY REPORT - MAY 2023



PC-1024

Lab Name	Govt. Block PHC, Vellalore	Lab No	7091
Constituent Group	Chemistry III	Date of Result Entered :	20/05/2023
PT item	Lyophilized human serum based	Date of Report Published :	05/06/2023

Sl. No.	Analyte	Method/Principle	Analyzer/Model	Run No.	Mean	SD	CV	Target	SDI	Delta
1	GLUCOSE III	GOD-POD III	Robonik (Semi automatic / Fully Automatic)	1834	180.88	5.19	9.39	190 mg/dL	0.97	0.44
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik (Semi automatic / Fully Automatic)	1854	1.76	7.48	0.13	1.9 mg/dL	1.06	0.01
3	CHOLESTROL III	CHOD-PAP III	Robonik (Semi automatic / Fully Automatic)	1798	114.60	5.08	5.83	112 mg/dL	-0.45	0.27

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ± 1.01 to ± 2.00	Good.
Within ± 2.01 to ± 2.99	Accept with caution. Warning Signal.
Beyond ± 3.0	Unacceptable performance. Action Signal.

LAB ADDRESS :

Govt. Block PHC, Vellalore
The Block Medical Officer VELLALORE, Madurai District
Vellalore
TAMILNADU625109

Coordinator Contact Details:
Email:clinqc@cmcvellore.ac.in
Contact Number: 0416-2283102

Pamela Christudoss
Dr. Pamela Christudoss
CMC EQAS Coordinator
Christian Medical College, Vellore

Homogeneity and Stability of the sample is passed.

Data in CMC EQAS reports is confidential

CMC EQAS does not sub contract any components

***** End of Report *****