



ISO 9001 : 2015  
RQ91/3144

# S.M. ENTERPRISES

(Calibration and Testing of Electrical, Electronic & Precision Instruments)

27<sup>th</sup>  
Years of Service

Office/Cal. Lab : Plot No. 12, "Ganesh Niwas", Sanjeevaiah Nagar, Co-operative Society, Besides Tadbund Hanuman Temple, Sikh Village, Secunderabad - 500 009, T.S, INDIA ☎: (040) 27840697, 48541008  
Cell: 9848020798, 9948291008, 9948292008, 9848293008, 9948294008 Email: msudheer\_98@yahoo.com, msudheer\_98@smentp.org, SME\_003@YAHOO.IN, url : www.smentp.org

## CALIBRATION CERTIFICATE

### CALIBRATION ON

15/05/2023

### CALIBRATION DUE

14/05/2024

1. Calibration Report Ref. No. & Date :	SME/NP/GMC/TIM/016/2023;Dt:15/05/2023
2. Requested by : (Name and address of the organization)	<b>To, Prof &amp; HOD( Department Of Microbiology).</b> Government Medical College,Ananthapur.
3. Instrument Name:	Digital Timer
4. Instrument Make/Model:	ACETEQ / DT-1045
5. Instrument ID. No:	GMC/TIM/016
6. Range :	0 to 99 min
7. Accuracy :	+/- 1 % FSD
8. Environmental Condition	Temp/RH : 28 +/- 2 Deg C; R.H: 65 +/- 5%
9. Test parameter & condition :	Time V/S Time (Comparision Method)
10. Standard Instruments used for Calibration:	Time Interval Meter
11. Traceability Certificate Ref. No.	C-220622-5-1 ,Date: 29/06/2022 , Due Dt: 29/06/2023


### TEST RESULTS

Sl No	Standard Reading Of Time	Observed Reading Of Time	Error Value(+/-)
	Hr:min:sec:ms	min:sec	Hr:min:sec:ms
1	00:01:00:15	01:00	00:00:00:15
2	00:10:00:57	10:00	00:00:00:57
3	00:30:00:43	30:00	00:00:00:43
4	01:50:00:41	90:00	00:00:00:41

PLEASE NOTE: THE INSTRUMENTS ERROR FOUND TO BE WITHIN THE SPECIFIED ACCURACY LIMIT ANDTHIS CERTIFICATE VALID FOR PERIOD OF ONE YEAR FROM THE DATE OF ISSUE.

CALIBRATED BY  
S . M. Enterprises

ENGINEER INCHARGE

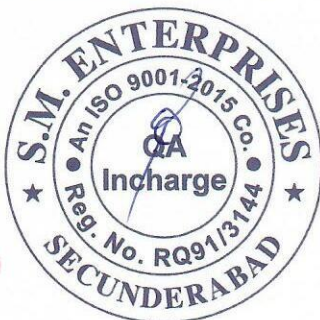

GSTIN : 36AFVPS4924F1ZW Service Tax No. : AFVPS4924FST001 PAN No. : AFVPS4924F

NABL APPROVED LAB (CC-2471) / Approved Laboratory of ISO 9001-2015

TEST EQUIPT. / STANDARDS USED ARE TRACEABLE TO NATIONAL STANDARDS