



Vanavil Calibrations

Make It Simple, But Significant !

CALIBRATION CERTIFICATE

Page : 1 of 1

Customer Name & Address: M/S GOVERNMENT PRIMARY HEALTH CENTRE , SURULODU-629 164.	Certificate No:	VCPL/CC/23-24/26-001
	Date of Calibration:	29-09-2023
	Date of issue:	30-09-2023
	Date of Receipt:	29-09-2023
	Next cal Date:	28-09-2024

Details of Device Under Calibration

Description	CENTRIFUGE	Make:	REMI
Range	3500 RPM	Model/Type:	C-854/4
Resolution	10 RPM	Condition of DUC:	GOOD
Serial No / Id.No	LELC-12845	Instrument Location:	LABORATORY

Environmental Conditions

Temperature	25.4 °C	Reference Standard No	SANAS TR4501
Humidity	53 % Rh	Calibration Procedure No	-

Method Used For Calibration

Details of Reference Standard Equipment For Calibration

S.No	Description	ID No / SL No	Certificate No	Validity
1	DIGITAL TACHOMETER	DTM-01	HT/CC/221202-03/005 SYSTEMS/ HTM 560	4-Dec-23


Calibration Result


S.No	DUC Reading (RPM)	Standard Reading (RPM)	Error (RPM)	Measurement Uncertainty (RPM)
1	500	500.2	-0.2	12
2	1000	999.7	0.3	12
3	1800	1803	-3	12
4	3000	2996	4	12
5	3500	3496	4	12

Remarks:

- 1.DUC is Defined as Device Under Calibration.
- 2.Calibration Frequency decided by the customer.
- 3.The above instrument is working in good condition.


Calibrated By:


R.GOPALAKRISHNAN
(CALIBRATION ENGINEER)

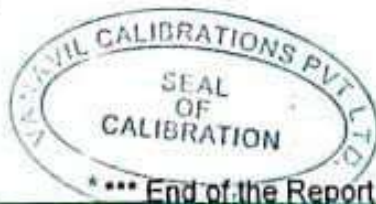

*** End of the Report ***

Authorised by:


S.LAKSHMANAN MURUGAN,
Technical Manager
Vanavil Calibrations Pvt Ltd.

Vanavil Calibrations Pvt. Ltd

(A Unit of Rainbow Blo Medical Engineers)

S2, Rishi Maharaj Apartment, Indra Nagar, 250 Reddiyur Main Road, Narasothipatty, Salem - 636 004.

No. 96,97,98, Anadhamaya Apartments, 2nd Floor, KVR Flats, 2nd Cross Street, Thangam Nagar, Pallikaranai, Chennai - 600 100.

Cell: 99949 13872 / 99949 23872 Ph: 0427-7965376

www.vanavilcalibrations.com | www.rainbowblomedicalengineers.com | www.vanavilcalibrations.com