



Vanavil Calibrations

Make It Simple, But Significant !

CALIBRATION CERTIFICATE

Page : 1 of 1

Customer Name & Address:	Certificate No:	VCPL/CC/23-24/45-001
M/S GOVERNMENT UPGRADED PRIMARY HEALTH CENTRE, THADIKKARANKONAM-629 851.	Date of Calibration:	12-10-2023
	Date of issue:	13-10-2023
	Date of Receipt:	12-10-2023
	Next cal Date:	11-10-2024

Details of Device Under Calibration

Description	CENTRIFUGE	Make:	REMI
Range	4000 RPM	Model/Type:	-
Resolution	10 RPM	Condition of DUC:	GOOD
Serial No	-	Instrument Location:	LABORATORY
ID number	GPHC/LAB/CEN/01	Cal. At:	ONSITE

Environmental Conditions

Temperature	23.4 °C	Reference Standard No	SANAS TR4501
Humidity	52 % Rh	Calibration Procedure No	-

Method Used For Calibration

Details of Reference Standard Equipment For Calibration

S.No	Description	ID No / SL No	Certificate No	Validity
1	DIGITAL TACHOMETER	DTM-01	HT/CC/221202-03/005 SYSTEMS/ HTM 560	4-Dec-23

Calibration Result


S.No	DUC Reading (RPM)	Standard Reading (RPM)	Error (RPM)	Measurement Uncertainty (RPM)
1	500	500.6	-0.6	12
2	1000	1001	-1	12
3	2000	2001	-1	12
4	3000	2997	3	12
5	3500	3496	4	12

Remarks:

- 1.DUC is Defined as Device Under Calibration.
- 2.Calibration Frequency decided by the customer.
- 3.The above instrument is working in good condition.

Calibrated By:

R,GOPALAKRISHNAN
(CALIBRATION ENGINEER)

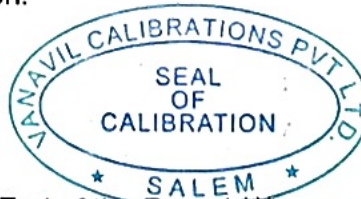

*** End of the Report ***

Authorised by:

M. KANNAN,
Technical Manager
Vanavil Calibrations Pvt Ltd.

Vanavil Calibrations Pvt. Ltd

(A Unit of Rainbow Bio Medical Engineers)

S2, Rishi Maharaj Apartment, Indra Nagar, 250 Reddiyur Main Road, Narasothipatty, Salem - 636 004.

No. 96,97,98, Anadhamaya Apartments, 2nd Floor, KVR Flats, 2nd Cross Street, Thangam Nagar, Pallikaranai, Chennai - 600 100.

Cell: 99949 13872 / 99949 23872 Ph: 0427-7965376

✉ vanavilcalibrations@gmail.com 🌐 www.rainbowbiomedicalengineers.com | www.vanavilcalibrations.com