



RML- Quality Assurance Program (RML-QAP)



Urine Routine Analysis

ALL METHOD REPORT

Lab Code: 2894

Cycle - 12/2023
Round No -09

Date: 05/10/2023

Parameters	Units	No.of. Participants	Consensus		Consensus Result	Your Value	Remark
			Number	%			
Specific Gravity	-	352	316	90%	1.010-1.020	1.020	Within Consensus
pH	-	352	315	90%	6.0	6.0	Within Consensus
Leukocytes	/µl	345	337	98%	Negative	Negative	Within Consensus
Nitrite	-	342	337	99%	Negative	Negative	Within Consensus
Protein	mg/dl	351	345	98%	Negative	Negative	Within Consensus
Glucose	mg/dl	351	349	99%	Negative	Negative	Within Consensus
Ketones	-	351	348	99%	Negative	Negative	Within Consensus
Urobilinogen	mg/dl	349	344	99%	Negative	Negative	Within Consensus
Bilirubin	mg/dl	349	345	99%	Negative	Negative	Within Consensus
Blood (Hemoglobin)	/µl	349	341	98%	Negative	Negative	Within Consensus

Legends	≥ 60% Consensus	(*) Outside Consensus	(@) No Consensus	(.) Not Reported	(#)Late Result Submission
---------	-----------------	-----------------------	------------------	------------------	---------------------------

Chief Coordinator

Dr.Sanjay Mehrotra

Checked By

Prepared By: SM

Programme Director

Dr.Bandana Mehrotra

Page 1 of 4

Doc. No.: ASS/FR/10/R 01/Dt.: 05.01.2022



Address: B-171, Nirala Nagar, Lucknow-226020. Ph.: 4034100-130 (30 Lines), 4077180, 2788444 Fax : (0522)2788555
Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

Continuous Efforts And Execution Leads To Quality Excellence







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 12/2023

Round-9

Date:05/10/2023

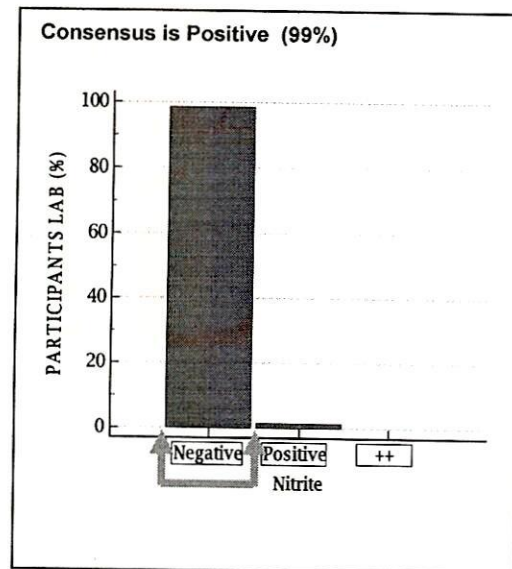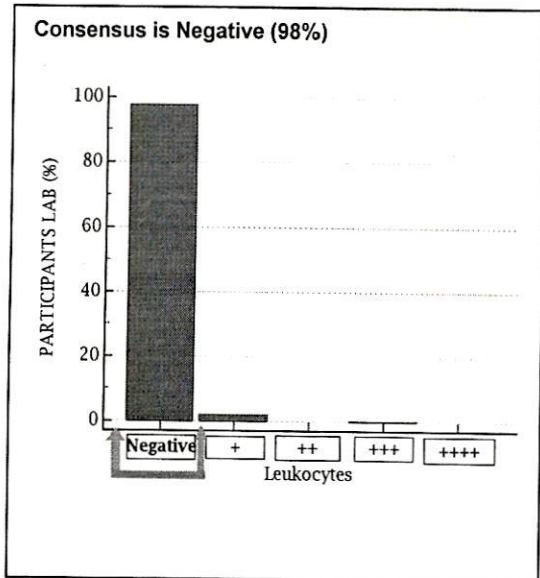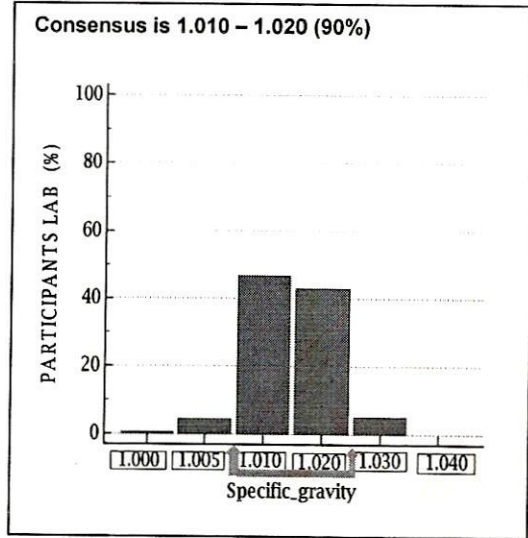







URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 12/2023

Round-9

Date:05/10/2023

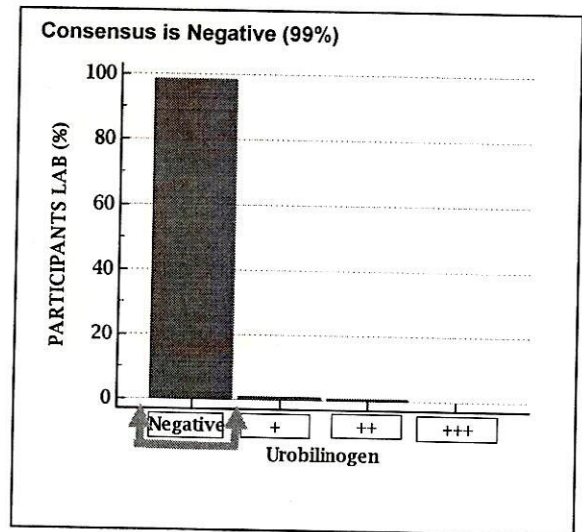





URINE ROUTINE ANALYSIS

GRAPHICAL REPORT

Cycle - 12/2023
Round-9

Date:05/10/2023

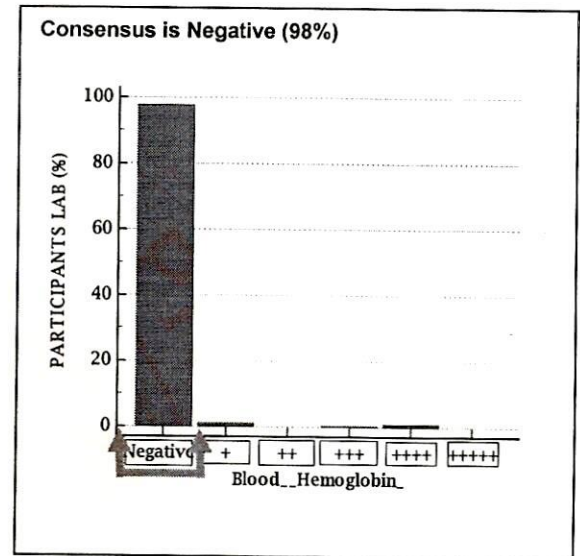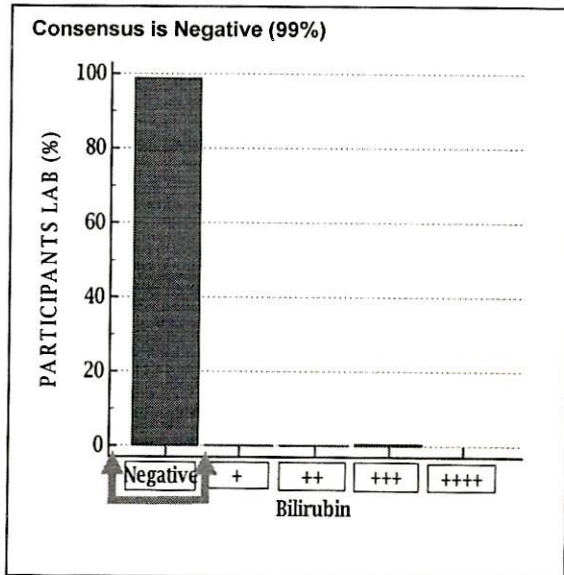



PC 1001

RML- Quality Assurance Program (RML-QAP)



BIO-CHEMISTRY-02

ALL METHOD REPORT

Lab Code: 2894

Cycle - 12/2023

Round No - 09

Date: 05/10/2023

Parameters	Units	No. of Participants	Robust Mean	Robust Standard deviation (SD)	Uncertainty of Assign Values	Range (± 2 SD)	Your Value	Z Score
Albumin	g/dL	120	2.9	0.2	0.03	2.5-3.3	2.7	-0.9
Alkaline Phosphatase	U/L	119	328.3	52.7	6.04	222.9-433.6	287	-0.8
Bilirubin (Total)	mg/dL	121	5.1	0.5	0.06	4.1-6.1	6.1	2.0
Calcium (Total)	mg/dL	113	12.4	0.5	0.06	11.3-13.5	12.0	-0.8
Cholesterol (Total)	mg/dL	120	266.6	12.4	1.41	241.9-291.3	260	-0.5
Creatinine	mg/dL	120	4.1	0.3	0.04	3.5-4.8	3.8	-0.9
Glucose	mg/dL	121	266.3	10.8	1.22	244.8-287.9	240	-2.4
HDL	mg/dL	115	84.7	13.6	1.59	57.5-111.9	64.3	-1.5
Potassium	mEq/L	98	5.8	0.3	0.04	5.2-6.3	5.5	-0.9
Protein (Total)	g/dl	119	4.5	0.2	0.02	4.1-4.8	4.3	-1.0
Sodium	mEq/L	98	156.2	4.4	0.55	147.5-164.9	147	-2.1
SGPT/ALT	U/L	121	132.0	9.7	1.10	112.5-151.5	121	-1.1
SGOT/AST	U/L	120	135.7	7.8	0.89	120.1-151.2	120	-2.0
Triglyceride	mg/dL	118	251.8	11.1	1.28	229.7-274.0	235.0	-1.5
Urea	mg/dL	121	113.0	5.6	0.64	101.8-124.0	101.0	-2.1
Uric Acid	mg/dl	118	9.4	0.7	0.08	8.1-10.8	4.4	-7.1
Chloride	mEq/L	93	115.9	4.1	0.53	107.7-124.1	107	-2.2
Phosphorus	mg/dL	85	6.8	0.3	0.04	6.3-7.3	6.7	-0.3
Magnesium	mg/dl	23	4.4	0.2	0.06	4.1-4.7	.	-
Iron	µg/dL	74	215.0	13.6	1.98	187.8-242.2	214	-0.1
Amylase	U/L	63	283.2	22.8	3.59	237.6-328.7	293	0.4
CK	U/L	23	472.2	96.3	25.10	279.5-664.9	382	-0.9

Interpretation of Z Score :

Z Score Value(+/-)	$[Z] \leq 2.0$	$2.0 < [Z] < 3.0$	$[Z] \geq 3.0$
Interpretation	Satisfactory Performance No signal	Questionable Warning Signal	Unsatisfactory Performance action Signal

Legends	(*) Excluded From Group Mean	{.} Not Reported	(#)Late Result Submission	(\$)Reported in other Unit
---------	------------------------------	------------------	---------------------------	----------------------------

Chief Coordinator

Dr.Sanjay Mehrotra

Programme Director

Dr.Bandana Mehrotra

Checked By:

Prepared by:

Page 1 of 7

Doc. No.: ASS / FR / 03A / R 01 / Dt.: 05.01.2022



Address: B-171, Nirala Nagar, Lucknow-226020. Ph.: 4034100-130 (30 Lines), 4077180, 2788444 Fax : (0522)2788555
Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

Continuous Efforts And Execution Leads To Quality Excellence



PC 1001

RML- Quality Assurance Program (RML-QAP)



BIO-CHEMISTRY-02

METHOD WISE REPORT

Cycle - 12/2023

Round No - 09

Lab Code: 2894

Date: 05/10/2023

Note: Your Lab is not the part of this method group.

Parameters	Units	Method Group	No.of. Participants	Robust Mean	Robust Standard deviation (SD)	Uncertainty of Assign Values	Range (± 2 SD)	Your Value	Z Score
Albumin	g/dL	Bromocresal Green (BCG)	85	3.0	0.2	0.03	2.6-3.3	-	-
Alkaline Phosphatase	U/L	PNPP	85	325.5	48.1	6.52	229.3-421.8	-	-
Bilirubin Total	mg/dL	Diazonium Ion	75	5.1	0.5	0.07	4.1-6.1	-	-
Calcium(Total)	mg/dL	Arsenazo iii	64	12.3	0.4	0.06	11.5-13.2	-	-
Cholesterol (Total)	mg/dL	Cholesterol Oxidase,esterase, peroxidase	91	266.5	12.7	1.66	241.2-291.8	-	-
Creatinine	mg/dL	Alkaline picrate	73	4.1	0.3	0.04	3.4-4.8	-	-
Glucose	mg/dL	Glucose oxidase,hydrogen peroxide(Trinder)	63	270.3	11.3	1.78	247.8-292.9	-	-
HDL	mg/dL	Direct measure	49	90.9	9.4	1.68	72.1-109.7	-	-
Potassium	mEq/L	ISE Direct	43	5.6	0.3	0.06	5.0-6.2	-	-
Protein (Total)	g/dl	Biuret, reagent blank, end point	59	4.5	0.2	0.03	4.1-4.8	-	-
Sodium	mEq/L	ISE Direct	43	154.1	4.7	0.90	144.8-163.5	-	-
SGPT/ALT	U/L	UV without P5P	64	130.5	10.1	1.58	110.2-150.8	-	-
SGOT/AST	U/L	UV without P5P	62	133.2	9.9	1.57	113.3-153.1	-	-
Triglyceride	mg/dL	Enzymatic method	59	254.1	16.7	2.72	220.8-287.4	-	-
Urea	mg/dL	Urease	78	113.3	5.5	0.78	102.3-124.3	-	-
Uric Acid	mg/dl	Uricase	57	9.3	0.5	0.08	8.2-10.4	-	-
Chloride	mEq/L	ISE Indirect	43	115.5	3.5	0.67	108.4-122.5	-	-
Phosphorus	mg/dL	Phosphomolybdate method	64	6.7	0.2	0.03	6.2-7.2	-	-
Magnesium	mg/dl	Uricase Colorimetic	10	4.2	0.3	0.12	3.5-4.8	-	-
Iron	µg/dL	Ferene	32	209.7	12.6	2.78	184.4-234.9	-	-
Amylase	U/L	Uricase Colorimetic	32	284.8	27.3	6.03	230.1-339.4	-	-
CK	U/L	NAC Activated	13	461.1	82.7	28.67	295.7-626.5	-	-

Interpretation of Z Score :

Z Score Value(+/-)	$[Z] \leq 2.0$	$2.0 < [Z] < 3.0$	$[Z] \geq 3.0$
Interpretation	Satisfactory Performance No signal	Questionable Warning Signal	Unsatisfactory Performance action Signal

Legends	(*) Excluded From Group Mean	{,} Not Reported	(#)Late Result Submission	(\$)Reported in other Unit
---------	------------------------------	------------------	---------------------------	----------------------------

Chief Coordinator

Dr.Sanjay Mehrotra

Checked By:

Prepared by: R

Doc. No.: ASS / FR / 03A / R 01 / Dt.: 05.01.2022

Programme Director

Dr.Bandana Mehrotra

Page 2 of 7



Address: B-171, Nirala Nagar, Lucknow-226020. Ph.: 4034100-130 (30 Lines), 4077180, 2788444 Fax : (0522)2788555
 Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

Continuous Efforts And Execution Leads To Quality Excellence



RML- Quality Assurance Program (RML-QAP)



BIO-CHEMISTRY-02

METHOD WISE REPORT PART-02

Cycle - 12/2023

Round No - 09

Date: 05/10/2023

Lab Code: 2894

Note: Your Lab is not the part of this method group

Parameters	Units	Method Group	No.of. Parti- cipants	Robust Mean	Robust Standard deviation (SD)	Uncertainty of Assign Values	Range (± 2 SD)	Your Value	Z Score
Glucose	mg/dL	Hexokinase	28	265.1	5.4	1.28	254.4-275.9	-	-
Potassium	mEq/L	ISE Indirect	28	6.0	0.1	0.02	5.7-6.3	-	-
Protein (Total)	g/dl	Biuret, No Serum Blank End Point	29	4.5	0.2	0.05	4.2-4.9	-	-
Sodium	mEq/L	ISE Indirect	27	158.4	3.8	0.91	150.9-166.0	-	-
SGPT/ALT	U/L	UV with P5P	25	135.8	9.5	2.38	116.7-154.8	-	-
SGOT/AST	U/L	UV with P5P	25	156.8	16.9	4.23	122.9-190.7	-	-
Triglyceride	mg/dL	Enzymatic, End Point	31	250.6	6.6	1.48	237.4-263.8	-	-
Uric Acid	mg/dl	Enzymatic	31	9.7	0.8	0.18	8.1-11.3	-	-
Chloride	mEq/L	ISE Direct	25	116.0	3.2	0.80	109.6-122.3	-	-
Iron	μ g/dL	Forzine-NO Deproteinization	26	218.9	8.1	1.99	202.8-235.1	-	-

Interpretation of Z Score :

Z Score Value(+/-)	$[Z] \leq 2.0$	$2.0 < [Z] < 3.0$	$[Z] \geq 3.0$
Interpretation	Satisfactory Performance No signal	Questionable Warning Signal	Unsatisfactory Performance action Signal

Legends	(*) Excluded From Group Mean	{ } Not Reported	(#)Late Result Submission	(\$)Reported in other Unit
---------	------------------------------	------------------	---------------------------	-------------------------------

Chief Coordinator

Dr.Sanjay Mehrotra

Checked By:

Prepared by: R

Programme Director

Dr.Bandana Mehrotra

Page 1 of 1

Doc. No.: ASS / FR / 03A / R 01 / Dt.: 05.01.2022



Address: B-171, Nirala Nagar, Lucknow-226020. Ph.: 4034100-130 (30 Lines), 4077180, 2788444 Fax : (0522)2788555
Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

Continuous Efforts And Execution Leads To Quality Excellence









EXTENDED BIO-CHEMISTRY-02

GRAPHICAL REPORT

Cycle - 12/2023
Round-9

Date: 05/10/2023

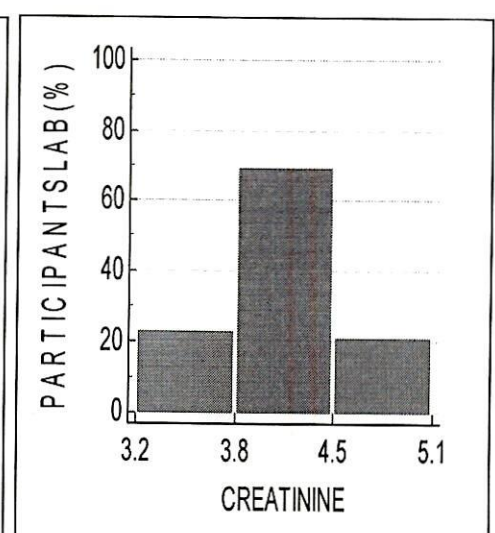

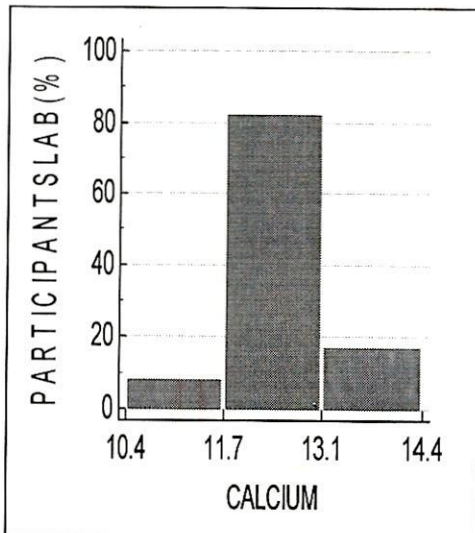
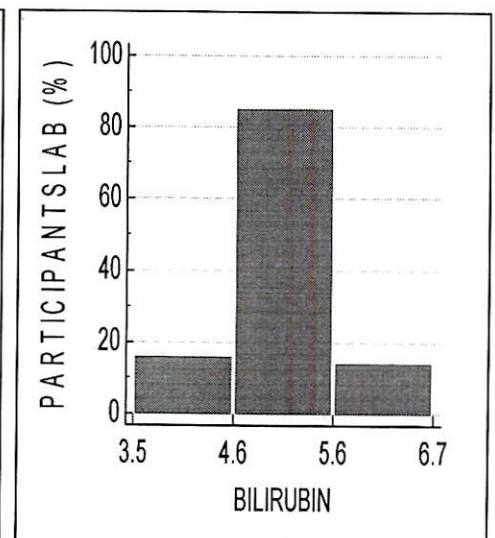
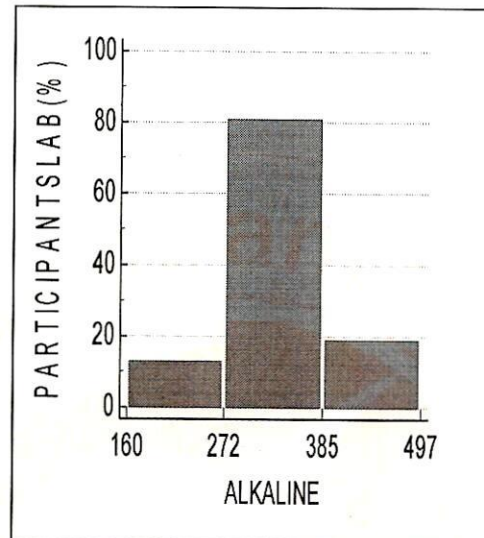



EXTENDED BIO-CHEMISTRY-02

GRAPHICAL REPORT

Cycle - 12/2023
Round-9

Date: 05/10/2023











EXTENDED BIO-CHEMISTRY-02

GRAPHICAL REPORT

Cycle - 12/2023
Round-9

Date: 05/10/2023

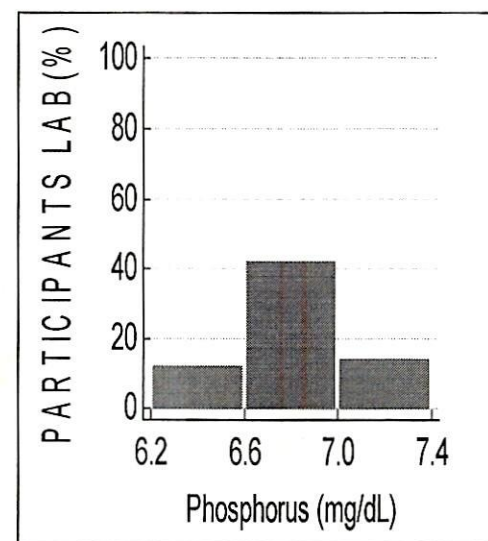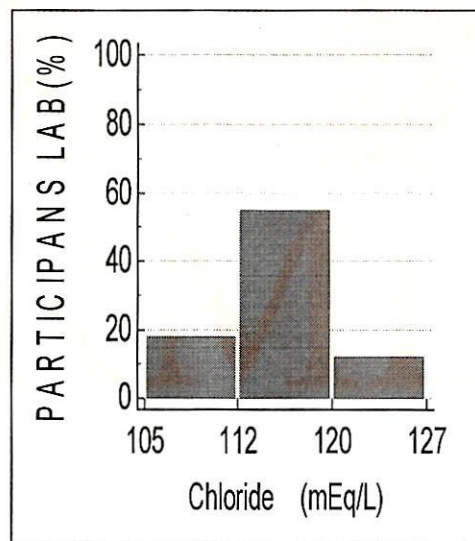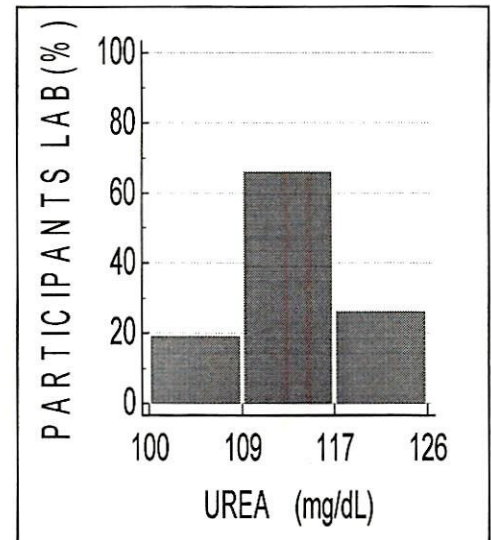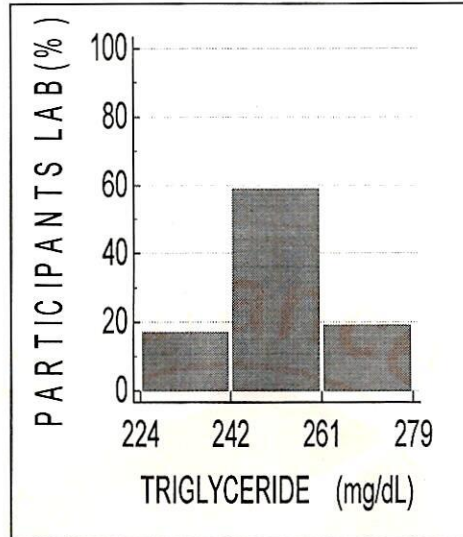







EXTENDED BIO-CHEMISTRY-02

GRAPHICAL REPORT

Cycle - 12/2023
Round-9

Date: 05/10/2023

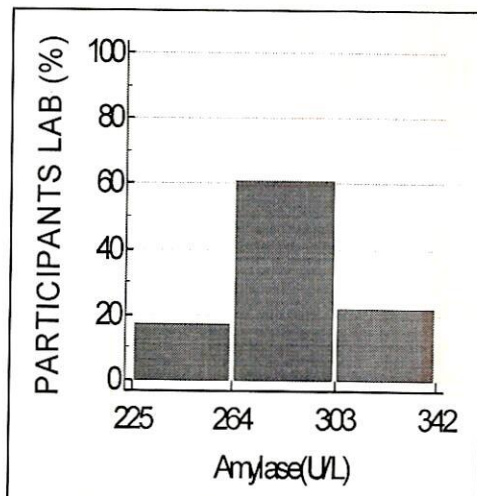



PC 1001

RML- Quality Assurance Program (RML-QAP)



Extended Biochemistry -02

ALL PARTICIPANTS COMPLETE DATA REPORT

Cycle - 12/2023

Round No - 09

Date: 05/10/2023

Note:- This report is only for information about the participants performance in the particular round .

Parameters	Total No. of Participants	No. of Responses	No of Participant Excluded from Robust Group Mean	No. of Participants Z Score b/w 0.0 - 2	No. of Participants Z Score b/w 2.1 - 2.9	No. of Participants Z Score >3
Albumin	160	120	4	111	5	4
Alkaline Phosphatase	160	119	5	111	2	6
Bilirubin Total	160	121	5	107	9	5
Calcium(Total)	160	113	7	100	6	7
Cholesterol (Total)	160	120	4	109	7	4
Creatinine	160	120	4	109	7	4
Glucose	160	121	11	99	11	11
HDL	160	115	3	92	20	3
Potassium	160	98	4	90	4	4
Protein (Total)	160	119	14	101	4	14
Sodium	160	98	5	90	3	5
SGPT/ALT	160	121	10	104	7	10
SGOT/AST	160	120	28	86	6	28
Triglyceride	160	118	16	93	9	16
Urea	160	121	8	106	7	8
Uric Acid	160	118	6	109	3	6
Chloride mEq/L	160	93	5	82	6	5
Phosphorus mg/dL	160	85	14	68	3	14
Magnesium mg/dl	160	23	14	17	1	5
Iron µg/dL	160	74	8	63	3	8
Amylase U/L	160	63	13	42	8	13
CK U/L	160	23	1	20	2	1

****End of Report****

Page 8 of 8

Doc. No.: ASS / FR / 01 / R 00 / Dt.: 01.07.2012



Address: B-171, Nirala Nagar, Lucknow-226020. Ph.: 4034100-130 (30 Lines), 4077180, 2788444 Fax : (0522)2788555
 Email: rmlresearchfoundation@gmail.com Website: www.rmlpathology.com

Continuous Efforts And Execution Leads To Quality Excellence