



CHRISTIAN MEDICAL COLLEGE VELLORE

In Service of the Nation Since 1900...

VIEW LAB MONTHLY SUMMARY

Lab Name: Govt. PHC, S.R.Pattinam Details About Robust Analysis
 Lab No: 12642 Detail About Monthly Summary
 Month: April Detail about SDI
 Year: 2023
 Constituent Group: Chemistry III

Click on the analyte to view Graphical Data

[All Analyser Result](#)

[Print](#)


Date of Result Entered : 20/04/2023

Date of Report Published : 06/05/2023

Sl.No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	Participants		Your Value	SDI	U
						CV	SD			
1	GLUCOSE III	GOD-POD III	Robonik (Semi automatic / Fully Automatic)	1832	119.45	6.04	7.21	130 mg/dL	1.46	0.34
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik (Semi automatic / Fully Automatic)	1820	2.16	8.09	0.18	2.1 mg/dL	-0.34	0.01
3	CHOLESTROL III	CHOD-PAP III	Any Analyser (Automation / Semi Automation)	143	111.22	4.31	4.79	114 mg/dL	0.58	0.80

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ±1.01 to ±2.00	Good.
Within ±2.01 to ±2.99	Accept with caution. Warning Signal.
Beyond ±3.0	Unacceptable performance. Action Signal.

D. J. J.
MEDICAL OFFICER
 Government Primary Health Centre

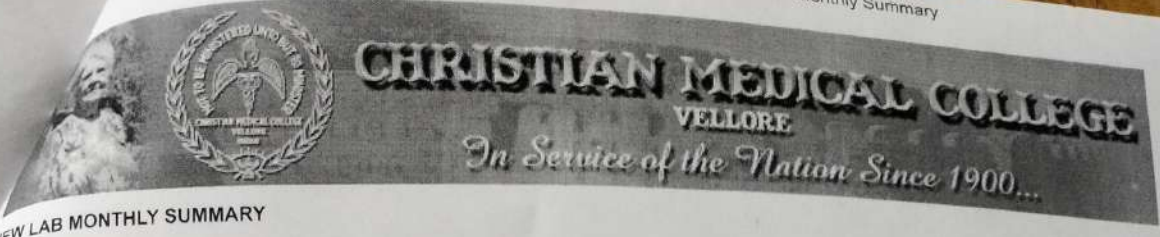

VIEW LAB MONTHLY SUMMARY

Lab Name Govt. PHC, S.R.Pattinam Details About Robust Analysis
 Lab No 12642 Detail About Monthly Summary
 Month May Detail about SDI
 Year 2023
 Constituent Group Chemistry III

Click on the analyte to view Graphical Data

[All Analyser Result](#) [Print](#)

Date of Result Entered : 18/05/2023

Date of Report Published : 05/06/2023

Sl.No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	Participants		Your Value	SDI	U
						CV	SD			
1	GLUCOSE III	GOD-POD III	Robonik (Semi automatic / Fully Automatic)	1834	180.88	5.19	9.39	167 mg/dL	-1.48	0.44
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik (Semi automatic / Fully Automatic)	1854	1.76	7.48	0.13	1.6 mg/dL	-1.21	0.01
3	CHOLESTROL III	CHOD-PAP III	Any Analyser (Automation / Semi Automation)	154	114.84	5.08	5.83	111 mg/dL	-0.66	0.94

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ±1.01 to ±2.00	Good.
Within ±2.01 to ±2.99	Accept with caution. Warning Signal.
Beyond ±3.0	Unacceptable performance. Action Signal.

Links			
Modify Address	Modify Methods	Submit Lab Results	View Lab Monthly Summary
Yearly Summary	Change Password	Home	Sign-out

Site Maintained by
Swiftware Solutions

[Signature]
MEDICAL OFFICER
 Government Primary Health Centre
 S. R. PATTINAM



VIEW LAB MONTHLY SUMMARY

Lab Name	Govt. PHC, S.R.Pattinam	Details About Robust Analysis
Lab No	12642	Detail About Monthly Summary
Month	June	Detail about SDI
Year	2023	
Constituent Group	Chemistry III	

Click on the analyte to view Graphical Data

Date of Result Entered : 19/06/2023

Date of Report Published : 04/07/2023

Sl.No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	Participants		Your Value	SDI	U
						CV	SD			
1	GLUCOSE III	GOD-POD III	Robonik (Semi automatic / Fully Automatic)	1823	286.63	5.17	14.82	294 mg/dL	0.50	0.69
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik (Semi automatic / Fully Automatic)	1848	2.57	6.64	0.17	2.2 mg/dL	-2.16	0.01
3	CHOLESTROL III	CHOD-PAP III	Any Analyser (Automation / Semi Automation)	149	114.61	4.05	4.64	110 mg/dL	-0.99	0.76

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ±1.01 to ±2.00	Good.
Within ±2.01 to ±2.99	Accept with caution. Warning Signal.
Beyond ±3.0	Unacceptable performance. Action Signal.

Links			
Modify Address	Modify Methods	Submit Lab Results	View Lab Monthly Summary
Yearly Summary	Change Password	Home	Sign-out

Site Maintained by
Swiftware Solutions

MEDICAL OFFICER
 Government Primary Health Center
S R PATTINAM



CHRISTIAN MEDICAL COLLEGE

DEPARTMENT OF CLINICAL BIOCHEMISTRY
 CMC EXTERNAL QUALITY ASSURANCE SCHEME
 MONTHLY SUMMARY REPORT - JANUARY 2023

Lab Name: Govt. PHC, S.R.Pattinam Lab No: 12642
 Constituent Group: Chemistry III Date of Result Entered: 20/01/2023
 PT Item: Lyophilized human serum based Date of Report Published: 09/02/2023

Sl.No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	Participants		Your Value	SDI	U
						CV	SD			
1	GLUCOSE III	GOD-POD III	Robonik (Semi automatic / Fully Automatic)	1890	119.87	6.38	7.65	116 mg/dL	-0.51	0.35
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik (Semi automatic / Fully Automatic)	1865	2.21	10.02	0.22	2.1 mg/dL	-0.50	0.01
3	CHOLESTROL III	CHOD-PAP III	Any Analyser (Automation / Semi Automation)	149	111.59	5.08	5.67	109 mg/dL	-0.46	0.93

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ±1.01 to ±2.00	Good.
Within ±2.01 to ±2.99	Accept with caution. Warning Signal.
Beyond ±3.0	Unacceptable performance. Action Signal.

LAB ADDRESS :
 Govt. PHC, S.R.Pattinam
 S.R.Pattinam
 TAMILNADU

Coordinator Contact Details:
 Email: clinqc@cmcvellore.ac.in
 Contact Number: 0416-2283102

Pamela Christudoss
 Dr. Pamela Christudoss
 CMC EQAS Coordinator
 Christian Medical College, Vellore

Homogeneity and Stability of the sample is passed.
 Data in CMC EQAS reports is confidential
 CMC EQAS does not sub contract any components
 ***** End of Report *****

Prof
 MEDICAL OFFICER
 Government Primary Health Centre
 S. R. PATTINAM
 MEDICAL OFFICER
 Government Primary Health Centre
 S. R. PATTINAM

VIEW LAB MONTHLY SUMMARY

Lab Name: Govt. PHC, S.R.Pattinam
 Lab No: 12642
 Month: July
 Year: 2023
 Constituent Group: Chemistry III

Click on the analyte to view Graphical Data

[Details About Robust Analysis](#)

[Detail About Monthly Summary](#)


[Detail about SDI](#)

Date of Result Entered : 19/07/2023

Date of Report Published : 07/08/2023

Sl No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	CV	SD	Your Value	SDI	U
1	GLUCOSE III	GOD-POD III	Robonik (Semi automatic / Fully Automatic)	1876	109.35	5.55	6.07	104 mg/dL	-0.88	0.28
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Robonik (Semi automatic / Fully Automatic)	1850	5.83	6.00	0.35	5.95 mg/dL	0.34	0.02
3	CHOLESTROL III	CHOD-PAP III	Any Analyser (Automation / Semi Automation)	148	112.78	4.33	4.88	111 mg/dL	-0.36	0.80

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ±1.01 to ±2.00	Good.
Within ±2.01 to ±2.99	Accept with caution. Warning Signal.
Beyond ±3.0	Unacceptable performance. Action Signal.

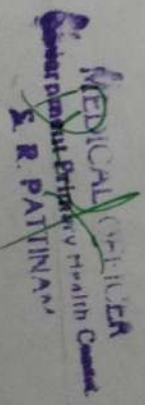

VIEW LAB MONTHLY SUMMARY

Lab Name Govt. PHC, S.R.Pattinam
 Lab No 12642
 Month August
 Year 2023
 Constituent Group Chemistry III

Click on the analyte to view Graphical Data


[Details About Robust Analysis](#)
[Detail About Monthly Summary](#)
[Detail about SDI](#)

Date of Result Entered : 19/08/2023

Date of Report Published : 01/09/2023

Sl.No	Analyte	Method / Principle Name	Analyzer Name	No of Participants	DV	Participants CV	SD	Your Value	SDI	U
1	GLUCOSE III	GOD-POD III	Roborik (Semi automatic / Fully Automatic)	1841	175.58	5.13	9.00	182 mg/dL	0.71	0.42
2	CREATININE III	Jaffes Kinetic - Alkaline Picrate III	Roborik (Semi automatic / Fully Automatic)	1852	1.76	6.77	0.12	1.69 mg/dL	-0.59	0.01
3	CHOLESTROL III	CHOD-PAP III	Any Analyser (Automation / Semi Automation)	149	113.96	4.36	4.97	118 mg/dL	0.81	0.81

SDI Range	Interpretation
Within -1.00 to +1.00	Excellent.
Within ±1.01 to ±2.00	Good.
Within ±2.01 to ±2.99	Accept with caution. Warning Signal.
Beyond ±3.0	Unacceptable performance. Action Signal.


MEDICAL OFFICER
 Government Primary Health Centre
 S. P. PATTINAM