

CALIBRATION / TESTING REPORT

CUSTOMER DETAILS : GOVERNMENT PRIMARY HEALTH CENTRE PANANKUDI, SIVAGANGAL.	CERTIFICATE NO	TICS/2023/PK/SG/01	
	EQUIPMENT NAME	MICROSCOPE	
	MANUFACTURE	OLYMBUS	
	MODEL	CH20IBIMF	
CALIBRATION DATE	20/10/2023	SERIAL NO	111G016
CALIBRATION DUE DATE	19/10/2024	INSTALLED DEPARTMENT	LAB

- 1. General maintenance required Yes No
- 2. Any Physical damage observed Yes No
- 3. Spare Replacement (if required) Yes No

TEST EQUIPMENT	MANUFACTURE	MODEL	SERIAL NUMBER
ELECTRICAL SAFTY ANALYZER	DATREND	V Pad-mini	VPM 18040011


PARAMETER	UNITS	VALUE	LIMITS	STATUS
Main Voltage L1-L2	V	227.1	230±10	PASS
Main Voltage L1-G(PE)	V	228.4	230±10	PASS
Main Voltage L2-G(PE)	V	0.62	<5	PASS
Load Current	A	0.288	As per unit	PASS
Protective Earth	Ω	0	<0.3	PASS
Point-to-Point Resistance	Ω	0	<0.5	PASS
Equipment Leakage	μA	0	Class I - < 500 Class II - < 100	PASS
Applied Part Leakage	μA	0	Type BF - < 5mA Type CF- <50μA*	PASS

Note : Test Standard: IEC 62353
 Defibrillator paddles 100 μA, per IEC 60601-2-4

*The above mentioned instrument has been tested using standards manufactures recommended protocols, using equipment having traceability to National/International standards.

ACCEPTABLE FOR USE CORRECTIVE MAINTENANCE REQUIRED REMOVED FROM USE
 Calibrated By : _____ Authorized Sign With Seal

Pr

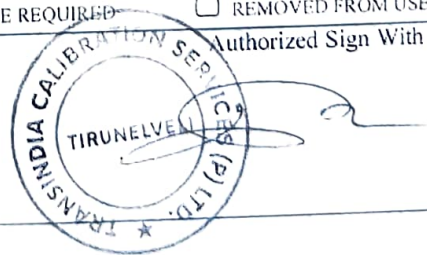

CALIBRATION / TESTING REPORT

CUSTOMER DETAILS : GOVERNMENT PRIMARY HEALTH CENTRE PANANKUDI, SIVAGANGAL		CERTIFICATE NO	TICS/2023/PK/SG/02
		EQUIPMENT NAME	CENTRIFUGE
		MANUFACTURE	REMI
		MODEL	C852
CALIBRATION DATE	20/10/2023	ASSET NO	ZALN0269
CALIBRATION DUE	19/10/2024	DEPARTMENT	LAB


- General maintenance required Yes No
- Any Physical damage observed Yes No
- Spare Replacement (if required) Yes No


TEST EQUIPMENT	MANUFACTURE	MODEL	SERIAL NUMBER
DIGITAL TACHOMETER	KUSAM MECO	KM2234 BL	S1049875
TEST REPORT			Temperature 25°C Humidity RH 55%

PARAMETERS	UNITS	SET VALUE	MEASURED VALUES	TOLERANCE	STATUS
ROTATION PER MINUTE	RPM	SPEED 2	1892	± 5	PASS
		SPEED 5	2917		

*The above mentioned instrument has been tested using standards manufactures recommended protocols, using equipment having traceability to National/International standards.

ACCEPTABLE FOR USE
 CORRECTIVE MAINTENANCE REQUIRED
 REMOVED FROM USE

Calibrated By: 

CALIBRATION / TESTING REPORT

CUSTOMER DETAILS : GOVERNMENT PRIMARY HEALTH CENTRE PANANKUDI, SIVAGANGAL.		CERTIFICATE NO	TICS/2023/PK/SG/03
		EQUIPMENT NAME	SEMI ANALYZER
		MANUFACTURE MODEL	ROBONIK PRIETEST TOUCH PLUS
CALIBRATION DATE	20/10/2023	SERIAL NO	ATP0160522RBK
CALIBRATION DUE DATE	19/10/2024	INSTALLED DEPARTMENT	LAB

- General maintenance required Yes No
- Any Physical damage observed Yes No
- Spare Replacement (if required) Yes No

TEST EQUIPMENT	MANUFACTURE	MODEL	SERIAL NUMBER
ELECTRICAL SAFTY ANALYZER	DATREND	V Pad-mini	VPM 18040011

PARAMETER	UNITS	VALUE	LIMITS	STATUS
Main Voltage L1-L2	V	226.8	230±10	PASS
Main Voltage L1-G(PF)	V	226.7	230±10	PASS
Main Voltage L2-G(PF)	V	0.69	<5	PASS
Load Current	A	0.376	As per unit	PASS
Protective Earth	Ω	0	<0.3	PASS
Point-to-Point Resistance	Ω	0	<0.5	PASS
Equipment Leakage	μA	0.15	Class I - < 500 Class II - < 100	PASS
Applied Part Leakage	μA	0	Type BF - < 5mA Type CF- <50μA*	PASS

Note : Test Standard: IEC 62353
Defibrillator paddles 100 μA, per IEC 60601-2-4

*The above mentioned instrument has been tested using standards manufactures recommended protocols, using equipment having traceability to National/International standards.

ACCEPTABLE FOR USE CORRECTIVE MAINTENANCE REQUIRED REMOVED FROM USE

Calibrated By :

Pr



Authorized Sign With Seal

CALIBRATION / TESTING REPORT

CUSTOMER DETAILS :

GOVERNMENT PRIMARY HEALTH CENTRE
PANANKUDI, SIVAGANGAI.

CALIBRATION DATE
CALIBRATION DUE DATE

20/10/2023
19/10/2024

CERTIFICATE NO
EQUIPMENT NAME
MANUFACTURE
MODEL
ASSET NO
INSTALLED DEPARTMENT

TICS/2023/PK/SG/04
MICROPIPETTE
THERMO SCIENTIFIC
FINE PIPETTE 100-1000 μ L
RW02658
LAB

1. Have more dust in machine outside Yes No
2. Any Physical damaged in machine Yes No
3. Machine inside Cleaning (if required) Yes No

TEST EQUIPMENT	ID. NO	CERTIFICATE NUMBER	VALIDITY
ELECTRONIC SEMI MICRO BALANCE	NCS/WB01	TSC/23-24/5424-1	27-JUNE-2024

TEST REPORT

PARAMETERS	UNITS	SET VALUE	MEASURED VALUES	TOLERANCE	STATUS
VOLUME	μ L	100	100.03	± 1	PASS
		1000	1000.03	± 1	PASS

*The above mentioned instrument has been tested using standards manufactures recommended protocols, using equipments having traceability to National/International standards.

ACCEPTABLE FOR USE CORRECTIVE MAINTENANCE REQUIRED REMOVED FROM USE
 Calibrated By : _____ Authorized Sign With Seal

Per





CALIBRATION / TESTING REPORT

CUSTOMER DETAILS :		CERTIFICATE NO	TICS/2023/PK/SG/05
GOVERNMENT PRIMARY HEALTH CENTRE PANANKUDI, SIVAGANGAI.		EQUIPMENT NAME	MICROPIPETTE
CALIBRATION DATE		20/10/2023	MANUFACTURE MODEL
CALIBRATION DUE DATE		19/10/2024	THERMO SCIENTIFIC FINE PIPETTE 10-100 µl.
		ASSET NO	RW01497
		INSTALLED DEPARTMENT	LAB

- 1. Have more dust in machine outside Yes No
- 2. Any Physical damaged in machine Yes No
- 3. Machine inside Cleaning (if required) Yes No

TEST EQUIPMENT	ID. NO	CERTIFICATE NUMBER	VALIDITY
ELECTRONIC SEMI MICRO BALANCE	NCS/WB01	TSC/23-24/5424-1	27-JUNE-2024

TEST REPORT

PARAMETERS	UNITS	SET VALUE	MEASURED VALUES	TOLERANCE	STATUS
VOLUME	µL	10	99.98	± 1	PASS
		100	99.98	± 1	PASS

*The above mentioned instrument has been tested using standards manufactures recommended protocols, using equipments having traceability to National/International standards.

ACCEPTABLE FOR USE
 CORRECTIVE MAINTENANCE REQUIRED
 REMOVED FROM USE
 Calibrated By: 

Authorized Sign With Seal





CALIBRATION / TESTING REPORT

CUSTOMER DETAILS : GOVERNMENT PRIMARY HEALTH CENTRE PANANKUDI, SIVAGANGAL.	CERTIFICATE NO	TICS/2023/PN/SG/06	
	EQUIPMENT NAME	PIPETTE	
	MANUFACTURE	DRAGON	
	MODEL	500 µL FIXED	
CALIBRATION DATE	20/10/2023	ASSET NO	YE193AL0317576
CALIBRATION DUE	19/10/2024	DEPARTMENT	LAB

- 1. Have more dust in machine outside Yes No
- 2. Any Physical damaged in machine Yes No
- 3. Machine inside Cleaning (if required) Yes No

TEST EQUIPMENT	ID. NO	CERTIFICATE NUMBER	VALIDITY
ELECTRONIC SEMI MICRO BALANCE	NCS/WB01	TSC/23-24/5424-1	27-JUNE-2024

TEST REPORT

Temperature 25°C
Humidity RH 55%

PARAMETERS	UNITS	SET VALUE	MEASURED VALUES	TOLERANCE	STATUS
VOLUME	µL	500	500.12	± 1	PASS

*The above mentioned instrument has been tested using standards manufactures recommended protocols, using equipments having traceability to National/International standards.

ACCEPTABLE FOR USE
 CORRECTIVE MAINTENANCE REQUIRED
 REMOVED FROM USE
 Calibrated By : _____ Authorized Sign With Seal

Rz

