



S.M. ENTERPRISES

27th
Years of Service

ISO 9001 : 2015
RQ91/3144

(Calibration and Testing of Electrical, Electronic & Precision Instruments)

Office/Cal. Lab : Plot No. 12, "Ganesh Niwas", Sanjeeviah Nagar, Co-operative Society, Besides Tadburd Hanuman Temple, Sikh Village, Secunderabad - 500 009, T.S. INDIA z: (040) 27840697, 48541008
Cell: 9848020798, 9948291008, 9948292008, 9848293008, 9948294008 Email msudheer 98@yahoo.com, msudheer 98@smentp.org, SME 003@YAHOO.IN, url : www.smentp.org

CALIBRATION CERTIFICATE

CALIBRATION ON
25/05/2023

CALIBRATION DUE
24/05/2024


1. Calibration Report Ref. No. & Date :	SME/NP/SVMC/DTHM/CAL-03/2023;Dt:25/05/2023
2. Requested by :	To, Prof & HOD (State reference Lab) Department Of Microbiology SV Medical College Tirupathi AP
3. Instrument Name	Digital Thermo Hygrometer
4. Make/Model:	HTC-2
5. Instrument ID No:	SVMC/DTHM/03
6. Range :	-10.0°C to 50.0 ° C & 10% to 99 % RH
7. Accuracy :	+/- 1° C & 5%RH
8. Environmental Conditions :	Temp/ RH: 27 +/- 2Deg C; R.H:- 60 +/- 5%
9. Test parameter & condition :	Temperature & RH V/S Temperature& RH comprasion method
10. Standard Instruments used for Calibration:	Digital Thermo Hygrometer
11. Traceablity Certificate Ref. No.	TSC/22-23/8627-1,Date:06/09/2022,Due Date:06/09/2023.

TEST RESULTS

Sl No	Standard Reading Of Temperature & RH		Observed Reading Of Under Calibration Hygrometer In Deg C & %RH		Error Value +/-	
	Temperature in °C	RH in %	Temperature in °C	RH in %	Temp in °C	RH in %
1	-10.0	10	-10.0	10	0.0	0
2	0.0	30	0.2	32	0.2	2
3	10.0	40	10.5	43	0.5	3
4	20.0	50	20.2	52	0.2	2
5	30.0	60	30.5	63	0.5	3
6	40.0	75	40.5	76	0.5	1
7	50.0	90	49.7	88	0.3	2

PLEASE NOTE: THE INSTRUMENTS ERROR NOT FOUND TO BE WITHIN THE SPECIFIED ACCURACY LIMIT
AND THIS CERTIFICATE VALID FOR PERIOD OF ONE YEAR FROM THE DATE OF ISSUE.

CALIBRATED BY
S.M. ENTERPRISES

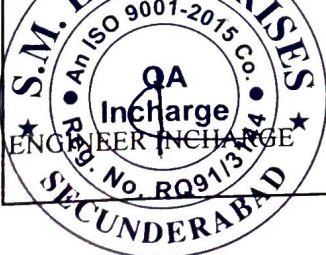

GSTIN : 36AFVPS4924F1ZW Service Tax No. : AFVPS4924FST001 PAN No. : AFVPS4924F
NABL APPROVED LAB (CC-2471) / Approved Laboratory of ISO 9001-2015
TEST EQUIPT. / STANDARDS USED ARE TRACEABLE TO NATIONAL STANDARDS