



CARE DIAGNOSTICS

Your Partner For Healthy Living

DATED: 14/12/2023

TO WHOM SO EVER IT MAY CONCERN

This is to inform you that we have started NABL Entry Level application three months before and quality manager has resigned his job. Due to that, we were not able to track the NABL application on time & we have recovered the Credentials now. Please Consider & we are ready to complete the application as soon as possible. Kindly accept & do the need.

Thanks & Regards

MANAGING PARTNER

CARE DIAGNOSTICS
4/442-D2, N.G.G.O.'s Colony,
Bagalur Road, HOSUR - 635 109.



CARE DIAGNOSTICS

Your Partner For Healthy Living

DATED: 14/12/2023

TO WHOM SO EVER IT MAY CONCERN

This is to inform you that our Biomedical Equipment calibration Testing & Sample taken from the vendor and awaiting for the reports. We will be sending you the 06/12/2023- 05/12/2024 Reports shortly. Kindly do the needful.

Thanks & Regards

MANAGING PARTNER

CARE DIAGNOSTICS
4/442-D2, N.G.G.O.'s Colony,
Bagalur Road, HOSUR - 635 109.

CARE DIAGNOSTICS# 4/442-D2, N.G.G.O 's Colony,
Bagalur Road, HOSUR - 635 109.**LIST OF EQUIPMENTS - PREVENTIVE & CALIBRATION SCHEDULE FOR THE YEAR 2023**

#	EQUIPMENT NAME	TYPE OF EQP.	ASSET NUMBER	MANUFACTURER	MODEL	SERIAL NO	CALIBRATION ON	CALIBRATION DUE
1	CELL COUNTER	MAJOR	1	MINDRAY	BC-5130	TR-1C006435	06-12-2023	05-12-2024
2	FULLY AUTOMATED ANALYSER	MAJOR	2	AMS HEALTHCARE	CKK 100	24003	06-12-2023	05-12-2024
3	HBA1C ANALYSER	MAJOR	3	SD BIOSENSOR	STD F200	FA20EB1TGO 319	06-12-2023	05-12-2024
4	HAEMOSTASIS ANALYSER	MAJOR	4	HEMOSTAR	HEMOSTAR XF 1.0	H1022S408	06-12-2023	05-12-2024
5	ELECTORLYTES ANALYSER	MAJOR	5	ARKRAY	SPOT-CHEM- EL-SE-1520	12208017	06-12-2023	05-12-2024
6	SERUM PROTIEAN ANALYSER	MAJOR	6	TULIP DIAGNOSTICS	TURBODYNE SC	P15070788	06-12-2023	05-12-2024
7	CELL COUNTER	MAJOR	8	HORIBA	MICRO 60	6050T95992	06-12-2023	05-12-2024


CARE DIAGNOSTICS# 4/442-D2, N.G.G.O.'s Colony,
Bagalur Road, HOSUR - 635 109.

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN. 33ADSPA9153Q1ZA • DL No. TN-12-20B -00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2607
		Issuing Date:	08/12/2022
		Page No:	1 of 2

Details of Device under Calibration (DUC):

DUC:	HBA1C Analyser	Id. No:	CDP/LAB/HBA1C/001
Make:	SD Biosensor	Department:	Laboratory
Model:	Standard F200	Calibrated On:	06/12/2022
Sl. No:	FA20EBITG039	Calibration Due Suggested:	05/12/2023
Type:	Semi Auto	DUC Condition on Receipt:	OK
Range & Least Count:	---		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electrical Safety Analyser	RigelSafeTest60	PSG/CIRD/BMCC/6908/2022	31/01/2023
2	Manometer	Lutron/PM9100	PC/01/22/ATL/0432-05	30/01/2023
3	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
4	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2 Room Humidity: 30-60% (At the time of Calibration)

ESA Test Results:

SL.No	Parameter	ESA Reading	Unit	Normal Range	Condition
1	Current	200	mA	500	Normal
2	Frequency	50	Hz	49 -50	Normal
3	Mains Voltage Line - Neutral	219.7	Volts	220 - 240	Normal
4	Mains Voltage Line - Earth	113.7	Volts	220 - 240	Normal
5	Mains Voltage Neutral - Earth	106.4	Volts	< 7	Normal

*Electrical Safety: Please check the attached log sheet

SL.No	Parameter	Measured	Standard	Correction	Unit
1	Lamp Voltage	11.78	12.0	-0.22	Volts
2	Detector Sensitivity	0.0	0.0	0.0	% Absorbance
3	Sipper Volume	432.5	450	-17.5	
4	Peristaltic Pump pressure	-14.42	-15.0	-0.58	

Allowable Tolerance: set by Customer

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)

aceagm@gmail.com



amshealthcareindia@gmail.com

Approved by:
(Technical Manager)

94434 74610, 93455 56148

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN: 33ADSPA9153Q17A • DL No. TN-12-20B-00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2605
		Issuing Date:	08/12/2022
		Page No:	1 of 2

Details of Device under Calibration (DUC):

DUC:	Electrolyte Analyser	Id. No:	CDP/LAB/EA/001
Make:	Arkray	Department:	Laboratory
Model:	Spot Chem-L SE-1520	Calibrated On:	06/12/2022
Sl. No:	122208017	Calibration Due Suggested:	05/12/2023
Type:	Semi Auto	DUC Condition on Receipt:	OK
Range & Least Count:	---		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electrical Safety Analyser	RigelSafeTest60	PSG/CIRD/BMCC/6908/2022	31/01/2023
2	Manometer	Lutron/PM9100	PC/01/22/ATL/0432-05	30/01/2023
3	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
4	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2 Room Humidity: 30-60% (At the time of Calibration)

ESA Test Results:

SL.No	Parameter	ESA Reading	Unit	Normal Range	Condition
1	Current	200	mA	500	Normal
2	Frequency	50	Hz	49 -50	Normal
3	Mains Voltage Line - Neutral	219.7	Volts	220 - 240	Normal
4	Mains Voltage Line - Earth	113.7	Volts	220 - 240	Normal
5	Mains Voltage Neutral - Earth	106.4	Volts	< 7	Normal

*Electrical Safety: Please check the attached log sheet

SL.No	Parameter	Measured	Standard	Correction	Unit
1	Lamp Voltage	11.78	12.0	-0.22	Volts
2	Detector Sensitivity	0.0	0.0	0.0	% Absorbance
3	Sipper Volume	432.5	450	-17.5	ml
4	Peristaltic Pump pressure	-14.42	-15.0	-0.58	cmH2O

Allowable Tolerance: set by Customer

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)



Approved by:
(Technical Manager)

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN. 33ADSPA9153Q1ZA • DL No. TN-12-20B -00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2609
		Issuing Date:	08/12/2022
		Page No:	1 of 2

Details of Device under Calibration (DUC):

DUC:	Fully Automated Analyser	Id. No:	CDP/LAB/FAA/001
Make:	Arkray	Department:	Laboratory
Model:	CKK100	Calibrated On:	06/12/2022
Sl. No:	24003	Calibration Due Suggested:	05/12/2023
Type:	Fully Auto	DUC Condition on Receipt:	OK
Range & Least Count:	---		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electrical Safety Analyser	RigelSafeTest60	PSG/CIRD/BMCC/6908/2022	31/01/2023
2	Manometer	Lutron/PM9100	PC/01/22/ATL/0432-05	30/01/2023
3	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
4	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

ESA Test Results:

SL.No	Parameter	ESA Reading	Unit	Normal Range	Condition
1	Current	200	mA	500	Normal
2	Frequency	50	Hz	49 -50	Normal
3	Mains Voltage Line - Neutral	219.7	Volts	220 - 240	Normal
4	Mains Voltage Line - Earth	113.7	Volts	220 - 240	Normal
5	Mains Voltage Neutral - Earth	106.4	Volts	< 7	Normal

*Electrical Safety: Please check the attached log sheet

SL.No	Parameter	Measured	Standard	Correction	Unit
1	Lamp Voltage	11.78	12.0	-0.22	Volts
2	Detector Sensitivity	0.0	0.0	0.0	% Absorbance
3	Sipper Volume	432.5	450	-17.5	ml
4	Peristaltic Pump pressure	-14.42	-15.0	-0.58	cmH ₂ O

Allowable Tolerance: set by Customer

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)



Approved by:
(Technical Manager)

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN. 33ADSPA9153Q1ZA • DL No. TN-12-20B -00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2602
		Issuing Date:	08/12/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Centrifuge	Id. No:	CDP/LAB/CEN/01
Make:	Remi	Department:	Laboratory
Model:	R-4c	Calibrated On:	06/12/2022
Sl. No:	CBLC-3023	Calibration Due Suggested:	05/12/2023
Type:	Manual	DUC Condition on Receipt:	OK
Range & Least Count:	0 – 3500RPM		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Digital Tachometer	Mextech / DT-2234C	PC/01/22/ATL/0432-01	30/01/2023
2	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023
3	Stop Watch	Nivia / JS 307	PC/01/22/ATL/0134-01	30/01/2023

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL.No.	DUC Reading (Positions) RPM	Standard Reading (RPM)	Correction (RPM)
1	1000	1020	+260
2	2000	2040	-121
3	2500	2580	-120
4	3500	3010	-110
5	3500	3410	-390

Allowable Tolerance: Set by Customer

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)



Approved by:
(Technical Manager)

aceagm@gmail.com

amshealthcare@gmail.com

94434 74610, 93455 56148

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN. 33ADSPA9153Q1ZA • DL No. TN-12-20B-00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2610
		Issuing Date:	08/12/2022
		Page No:	1 of 2

Details of Device under Calibration (DUC):

DUC:	Haematology Analyser-Cell Counter	Id. No:	CDP/LAB/HA/002
Make:	Mindray	Department:	Laboratory
Model:	BC-5130	Calibrated On:	06/12/2022
Sl. No:	TR-1C006435	Calibration Due Suggested:	05/12/2023
Type:	Semi Auto	DUC Condition on Receipt:	OK
Range & Least Count:	---		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electrical Safety Analyser	RigelSafeTest60	PSG/CIRD/BMCC/6908/2022	31/01/2023
2	Manometer	Lutron/PM9100	PC/01/22/ATL/0432-05	30/01/2023
3	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
4	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

ESA Test Results:

SL.No	Parameter	ESA Reading	Unit	Normal Range	Condition
1	Current	300	mA	500	Normal
2	Frequency	49.7	Hz	49 -50	Normal
3	Mains Voltage Line - Neutral	230.7	Volts	220 - 240	Normal
4	Mains Voltage Line - Earth	234.5	Volts	220 - 240	Normal
5	Mains Voltage Neutral - Earth	6.5	Volts	< 7	Normal

*Electrical Safety: Please check the attached log sheet

SL.No	Parameter	Measured	Standard	Correction	Unit
1	Lamp Voltage	11.78	12.0	-0.22	Volts
2	Detector Sensitivity	0.0	0.0	0.0	% Absorbance
3	Sipper Volume	432.5	450	-17.5	
4	Peristaltic Pump pressure	-14.42	-15.0	-0.58	cmH ₂ O

Allowable Tolerance: set by Customer

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)



Approved by:
(Technical Manager)

aceagm@gmail.com

amshealthcaremdu@gmail.com

94434 74610, 93455 56148

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN. 33ADSPA9153Q1ZA • DL No. TN-12-20B -00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2608
		Issuing Date:	08/12/2022
		Page No:	1 of 2

Details of Device under Calibration (DUC):

DUC:	Serum Protein Analyser	Id. No:	CDP/LAB/SPA/001
Make:	Tulip Diagnostics	Department:	Laboratory
Model:	Turbodyne- SC	Calibrated On:	06/12/2022
Sl. No:	P15070788	Calibration Due Suggested:	05/12/2023
Type:	Semi Auto	DUC Condition on Receipt:	OK
Range & Least Count:	---		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electrical Safety Analyser	RigelSafeTest60	PSG/CIRD/BMCC/6908/2022	31/01/2023
2	Manometer	Lutron/PM9100	PC/01/22/ATL/0432-05	30/01/2023
3	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
4	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2 Room Humidity: 30-60% (At the time of Calibration)

ESA Test Results:

SL.No	Parameter	ESA Reading	Unit	Normal Range	Condition
1	Current	200	mA	500	Normal
2	Frequency	50	Hz	49 -50	Normal
3	Mains Voltage Line - Neutral	219.7	Volts	220 - 240	Normal
4	Mains Voltage Line - Earth	113.7	Volts	220 - 240	Normal
5	Mains Voltage Neutral - Earth	106.4	Volts	< 7	Normal

*Electrical Safety: Please check the attached log sheet

SL.No	Parameter	Measured	Standard	Correction	Unit
1	Lamp Voltage	11.78	12.0	-0.22	Volts
2	Detector Sensitivity	0.0	0.0	0.0	% Absorbance
3	Sipper Volume	432.5	450	-17.5	ml
4	Peristaltic Pump pressure	-14.42	-15.0	-0.58	cmH ₂ O

Allowable Tolerance: set by Customer

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)



Approved by:
(Technical Manager)

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN: 33ADSPA9153Q17A • DI No. TN-12-20B-00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2604
		Issuing Date:	08/12/2022
		Page No:	1 of 2

Details of Device under Calibration (DUC):

DUC:	Cell Counter	Id. No:	CDP/LAB/CC/001
Make:	Horiba	Department:	Laboratory
Model:	Micros-60	Calibrated On:	06/12/2022
Sl. No:	6050T95992	Calibration Due Suggested:	05/12/2023
Type:	Semi Auto	DUC Condition on Receipt:	OK
Range & Least Count:	---		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electrical Safety Analyser	RigelSafeTest60	PSG/CIRD/BMCC/6908/2022	31/01/2023
2	Manometer	Lutron/PM9100	PC/01/22/ATL/0432-05	30/01/2023
3	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
4	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2 Room Humidity: 30-60%

(At the time of Calibration)

ESA Test Results:

SL.No	Parameter	ESA Reading	Unit	Normal Range	Condition
1	Current	200	mA	500	Normal
2	Frequency	49.8	Hz	49 -50	Normal
3	Mains Voltage Line - Neutral	230.7	Volts	220 - 240	Normal
4	Mains Voltage Line - Earth	235.3	Volts	220 - 240	Normal
5	Mains Voltage Neutral - Earth	8.2	Volts	< 7	Normal

*Electrical Safety: Please check the attached log sheet

SL.No	Parameter	Measured	Standard	Correction	Unit
1	Lamp Voltage	11.78	12.0	-0.22	Volts
2	Detector Sensitivity	0.0	0.0	0.0	% Absorbance
3	Sipper Volume	432.5	450	-17.5	ml
4	Peristaltic Pump pressure	-14.42	-15.0	-0.58	cmH ₂ O

Allowable Tolerance: set by Customer

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)

aceagm@gmail.com



amshealthcareindia@gmail.com

Approved by:
(Technical Manager)

94434 74610, 93455 56148

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN. 33ADSPA9153Q1ZA • DL No. TN-12-20B -00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2606
		Issuing Date:	08/12/2022
		Page No:	1 of 2

Details of Device under Calibration (DUC):

DUC:	Haemostasis Analyser- Coagulometer	Id. No:	CDP/LAB/HA/001
Make:	Hemostar	Department:	Laboratory
Model:	X.F-1.0	Calibrated On:	06/12/2022
Sl. No:	H1022S40B	Calibration Due Suggested:	05/12/2023
Type:	Semi Auto	DUC Condition on Receipt:	OK
Range & Least Count:	---		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electrical Safety Analyser	RigelSafeTest60	PSG/CIRD/BMCC/6908/2022	31/01/2023
2	Manometer	Lutron/PM9100	PC/01/22/ATL/0432-05	30/01/2023
3	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
4	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2 Room Humidity: 30-60% (At the time of Calibration)

ESA Test Results:

SL.No	Parameter	ESA Reading	Unit	Normal Range	Condition
1	Current	100	mA	500	Normal
2	Frequency	50	Hz	49 -50	Normal
3	Mains Voltage Line - Neutral	220.6	Volts	220 - 240	Normal
4	Mains Voltage Line - Earth	110.3	Volts	220 - 240	Normal
5	Mains Voltage Neutral - Earth	113.2	Volts	< 7	Normal

*Electrical Safety: Please check the attached log sheet

SL.No	Parameter	Measured	Standard	Correction	Unit
1	Lamp Voltage	11.78	12.0	-0.22	Volts
2	Detector Sensitivity	0.0	0.0	0.0	% Absorbance
3	Sipper Volume	432.5	450	-17.5	ml
4	Peristaltic Pump pressure	-14.42	-15.0	-0.58	cmH ₂ O

Allowable Tolerance: set by Customer

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)

aceagm@gmail.com



amshealthcaremd@gmail.com


Approved by:
(Technical Manager)

94434 74610, 93455 56148

CARE DIAGNOSTICS
4/442-D2, N.G.G.O.'s Colony,
Bagalur Road, HOSUR - 635 109.

LIST OF EQUIPMENTS - PREVENTIVE & CALIBRATION SCHEDULE FOR THE YEAR 2023

#	EQUIPMENT NAME	TYPE OF EQP.	ASSET NUMBER	MANUFACTURER	MODEL	SERIAL NO	CALIBRATION ON	CALIBRATION DUE
1	PIPETTE 1	MINOR	9	AMS HEALTHCARE	REGULAR 1 ML	CDP-LAB-VMP-001	06-12-2023	05-12-2024
2	PIPETTE 2	MINOR	10	AMS HEALTHCARE	REGULAR 1 ML	CDP-LAB-VMP-002	06-12-2022	05-12-2024
3	PIPETTE 3	MINOR	11	AMS HEALTHCARE	REGULAR 50 MICRO	CDP-LAB-FMP-001	06-12-2022	05-12-2024
4	PIPETTE 4	MINOR	12	AMS HEALTHCARE	REGULAR 50 MICRO	CDP-LAB-FMP-002	06-12-2022	05-12-2024
5	REFRIDGERATOR	MINOR	7	GODREJ	150L	885663	06-12-2022	05-12-2024
6	MICROSCOPE	MINOR	13	OLYMBUS OPTE	MLX-B-PLUS	16C0863	10-12-2023	10-12-2024


CARE DIAGNOSTICS
4/442-D2, N.G.G.O.'s Colony,
Bagalur Road, HOSUR - 635 109.

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN: 33ADSPA9153Q1ZA • DL No: TN-12-20B-00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2603
		Issuing Date:	08/12/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Microscope	Id. No:	CDP/LAB/MS/001
Make:	Magnus	Department:	Laboratory
Model:	MLX-B Plus	Calibrated On:	06/12/2022
Sl. No:	16C0863	Calibration Due	05/12/2023
Type:	Binocular Opto Sys.	Suggested:	
Range & Least Count:	---	DUC Condition on Receipt:	OK

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electrical Safety Analyser	RigelSafeTest60	PSG/CIRD/BMCC/6908/2022	31/01/2023
2	Digital Lux Meter	HTC/LX - 103	PC/01/22/ATL/0265-02	30/01/2023
3	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

ESA Test Results:

SL.No	Parameter	ESA Reading	Unit	Normal Range	Condition
1	Current	238	mA	300	Normal
2	Frequency	50.0	Hz	49 -50	Normal
3	Mains Voltage Line - Neutral	231.5	Volts	220 - 240	Normal
4	Mains Voltage Line - Earth	238.4	Volts	220 - 240	Normal
5	Mains Voltage Neutral - Earth	8.8	Volts	< 7	Normal

*Electrical Safety: Please check the attached log sheet

Test Results: Light Intensity LUX:

SL.No.	Knob Position	DUC Reading (LUX)	Distance (mm)
1	Low	200	30
2	Medium	9900	30
3	High	19200	30

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:

(Calibration Engineer)



Approved by:

(Technical Manager)

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN: 33ADSPA9153Q1ZA • DL No. TN-12-20B -00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2611
		Issuing Date:	08/12/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	CDP/LAB/VMP/001
Make:	Dragon Lab	Department:	Laboratory
Model:	Variable	Calibrated On:	06/12/2022
Sl. No:	YE5A426195	Calibration Due	05/12/2023
Type:	Variable	Suggested:	
Range & Least Count:	05 to 50µl	DUC Condition on Receipt:	OK

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
2	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	05	05.0	05.0	0.0
2	10	10.0	10.0	0.0
3	20	20.0	20.0	0.0
4	50	50.0	50.0	0.0

Allowable Tolerance: Set by User

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)



Approved by:
(Technical Manager)

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN: 33ADSPA9153Q1ZA • DL No. TN-12-20B -00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2613
		Issuing Date:	08/12/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micropipette	Id. No:	CDP/LAB/FMP/002
Make:	Dragon Lab	Department:	Laboratory
Model:	Fixed	Calibrated On:	06/12/2022
Sl. No:	YE5A578A67	Calibration Due Suggested:	05/12/2023
Type:	Fixed	DUC Condition on Receipt:	OK
Range & Least Count:	1000µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
2	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results Volume µl:


SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	1000.0	1010.0	1010.0	+10.0
2	1000.0	1010.0	1010.0	+10.0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)



Approved by:
(Technical Manager)

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN: 33ADSPA9153Q1ZA • DL No. TN-12-20B-00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/HOSP/289/2612
		Issuing Date:	08/12/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micro Pipette	Id. No:	CDP/LAB/VMP/002
Make:	Turbodyne-SE	Department:	Laboratory
Model:	Variable	Calibrated On:	06/12/2022
Sl. No:	PA537402	Calibration Due Suggested:	05/12/2023
Type:	Variable	DUC Condition on Receipt:	OK
Range & Least Count:	100 to 1000µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
2	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	100	140.0	140.0	+40.0
2	200	220.0	220.0	+20.0
3	500	550.0	550.0	+50.0
4	800	850.0	850.0	+50.0
5	1000	1050.0	1050.0	+50.0

Allowable Tolerance: Set by User

Note:

1. Calibration Points were selected as per customer request.
2. Each reading were taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)



Approved by:
(Technical Manager)

aceagm@gmail.com

amshealthcaremdu@gmail.com

94434 74610, 93455 56148

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN: 33ADSPA9153Q1ZA • DL No. TN-12-20B-00398, TN-12-21B-00398

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2614
		Issuing Date:	08/12/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Micropipette	Id. No:	CDP/LAB/FMP/001
Make:	Dragon Lab	Department:	Laboratory
Model:	Fixed	Calibrated On:	06/12/2022
Sl. No:	YE4A21576	Calibration Due Suggested:	05/12/2023
Type:	Fixed	DUC Condition on Receipt:	OK
Range & Least Count:	50µl		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	Electronic Weighing Scale	EWC/SF400C	PC/01/22/ATL/0432-02	30/01/2023
2	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results Volume µl:

SL. No.	DUC Reading (µl)	Standard Reading (µl)		Correction (µl)
		Trial 1	Trial 2	
1	50.0	51.0	51.0	+1.0
2	50.0	51.0	51.0	+1.0

Allowable Tolerance: User Defined



Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10 readings.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)



Approved by:
(Technical Manager)

Ace Medical Solutions (India) Pvt. Ltd.

An ISO 9001-2015 Certified Company

No. 770/1, Jothi Complex 2nd Floor, Alagar Kovil Main Road, Surveyor Colony,
Madurai - 625 007, Tamilnadu, India Mobile : +91 94434 74610



GSTIN 33ADSPA9153017A • DI No. TN 12 20B 00198, TN 12 21B 00198

CALIBRATION CERTIFICATE

Customer Name & Address:	M/S. Care Diagnostics & Poly Clinic, #4/442-D2, N.G.G.O. Colony, Bagalur Road, Hosur-635109	Certificate No:	AMS/LAB/289/2615
		Issuing Date:	08/12/2022
		Page No:	1 of 1

Details of Device under Calibration (DUC):

DUC:	Refrigerator - Reagent	Id. No:	CDP/LAB/REFR/01
Make:	Godrej	Department:	Laboratory
Model:	---	Calibrated On:	06/12/2022
Sl. No:	---	Calibration Due Suggested:	05/12/2023
Type:	Reagent	DUC Condition on Receipt:	OK
Range & Least Count:	-10 to 8°C/ LC 1°C		

Traceability Details:

Sl.No.	Test Equipment	Make	Certificate Number	Valid Up to
1	RTD Thermometer	Center / RTD 375	PC/01/22/ATL/0171-01	30/01/2023
2	Thermo Hygrometer	Beetech/088	PC/01/22/ATL/0265-01	30/01/2023

Room Temperature: 25°C±2

Room Humidity: 30-60%

(At the time of Calibration)

Test Results:

SL.No.	Place	DUC Reading (°C)	Standard Reading (°C)	Correction (°C)
1	Freezer	FRZ 1	-1.18	0
2		FRZ 2	-0.96	0
3	Chiller	CHI 1	1.13	0
4		CHI 2	1.08	0
5	Chamber I	CHA 1	3.47	0
6		CHA 2	3.51	0
7	Chamber II	CHA 1	4.33	0
8		CHA 2	4.28	0
9	Chamber III	CHA 1	5.13	0
10		CHA 2	5.24	0

Allowable Tolerance: User Defined

Note:

1. Calibration Points were selected as per customer request.
2. Each reading was taken by Repeatability Test (i.e.) each reading in a row is a mean of 10.
3. Results Reported are valid at the time of and under the stated conditions of measurements.

Calibrated By:
(Calibration Engineer)

aceagm@gmail.com



amshealthcaremdu@gmail.com


Approved by:
(Technical Manager)

94434 74610, 93455 56148

CARE DIAGNOSTICS & POLYCLINIC QC Chart

CKK100_Clinical_Chemistry_Analyser

Item:GLU N:11 MEAN:89.723 SD:10.009 CV:0.112




CARE DIAGNOSTICS & POLYCLINIC

GLU QC Lot:672 From:2023-10-17

Range:88.40-119.60


NO	Date	Sam. no	mg/dl
1	2023-10-17	1	111.40
2	2023-10-30	1	102.86
3	2023-11-07	1	82.50
4	2023-11-07	2	83.81
5	2023-11-07	3	89.12
6	2023-11-19	1	79.86
7	2023-11-19	2	89.44
8	2023-11-29	1	77.09
9	2023-11-29	2	88.01
10	2023-11-29	4	89.69
11	2023-11-29	21	93.17


CARE DIAGNOSTICS
41492 B2, N.C. G. S. Colony,
Bagalur Road, HOSUR - 635 109.

CARE DIAGNOSTICS & POLYCLINIC QC Chart

CKK100_Clinical_Chemistry_Analyser

Item:ALBU N:4 MEAN:3.140 SD:0.325 CV:0.104



CARE DIAGNOSTICS & POLYCLINIC

ALBU QC Lot:672 From:2023-10-17


Range:2.87-4.11

NO	Date	Sam. no	g/dl
1	2023-10-17	1	2.86
2	2023-10-17	2	3.05
3	2023-10-30	1	3.61
4	2023-11-07	1	3.04

CARE DIAGNOSTICS & POLYCLINIC QC Chart

CKK100_Clinical_Chemistry_Analyser

Item:TPROT N:6 MEAN:3.982 SD:0.370 CV:0.093

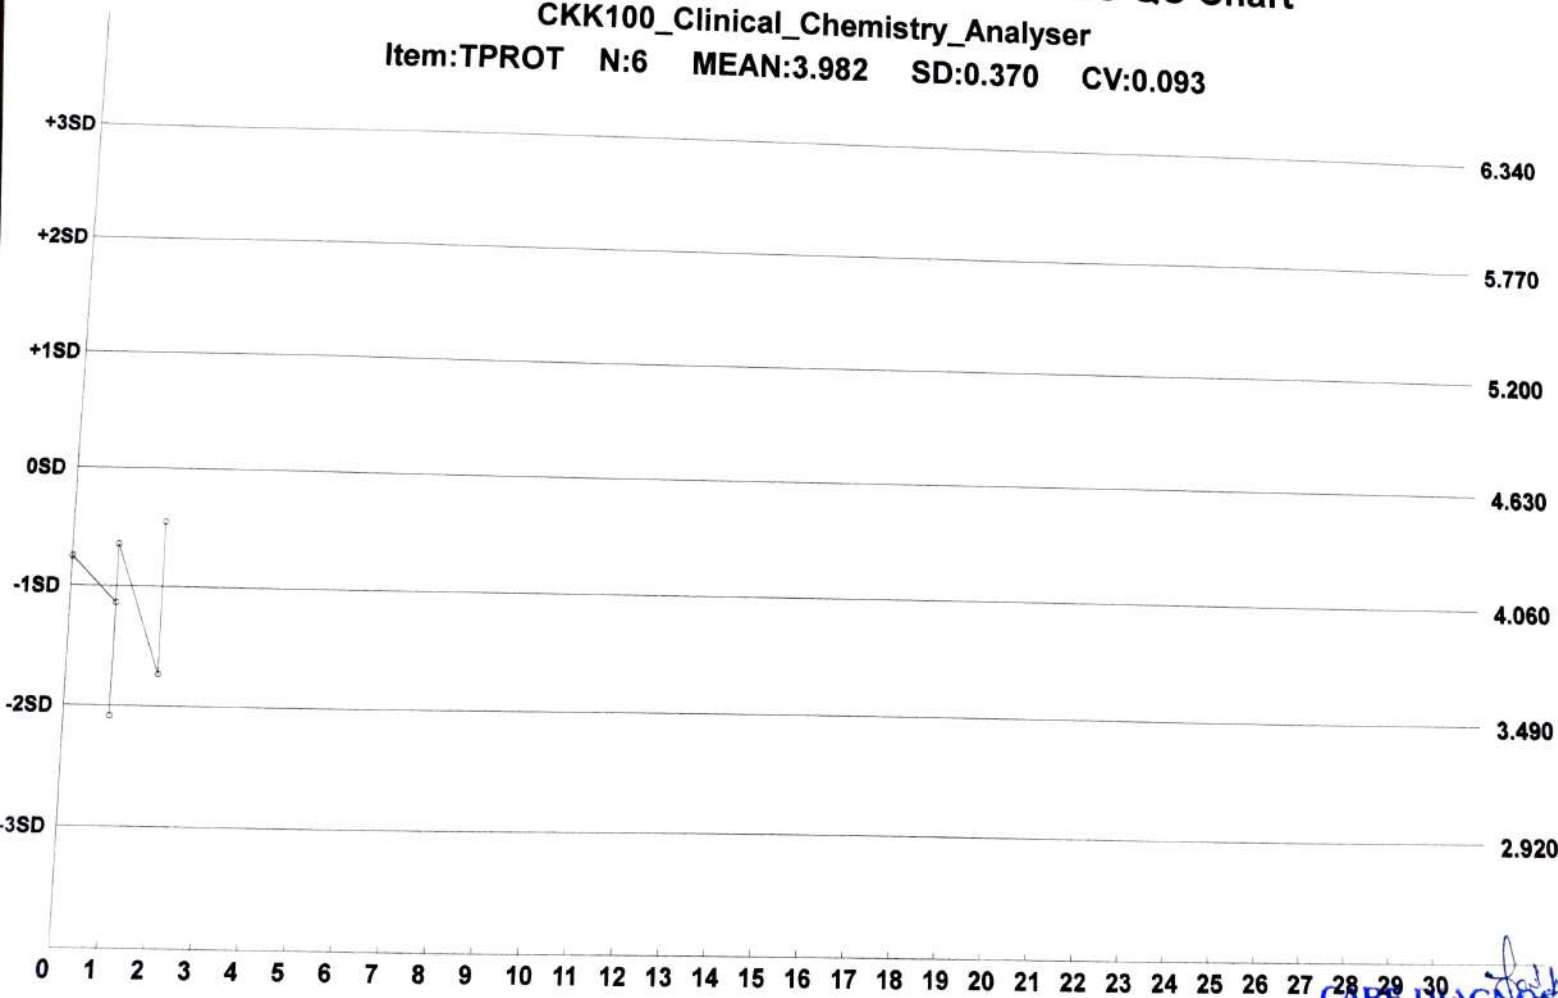

CARE DIAGNOSTICS & POLYCLINIC

TPROT QC Lot:672 From:2023-10-17

Range:4.06-5.20


NO	Date	Sam. no	g/dl
1	2023-10-17	1	4.20
2	2023-10-30	1	3.98
3	2023-10-30	2	3.44
4	2023-10-30	3	4.26
5	2023-11-07	1	3.64
6	2023-11-07	2	4.37


CARE DIAGNOSTICS
4/442-D2, N.S. G.O.'s Colony
Bagalur Road, HOSUR - 635 11

CARE DIAGNOSTICS & POLYCLINIC QC Chart

CKK100_Clinical_Chemistry_Analyser

Item:SGOT N:6 MEAN:26.980 SD:13.479 CV:0.500



CARE DIAGNOSTICS & POLYCLINIC

SGOT QC Lot:672 From:2023-10-17


Range:35.90-51.70

NO	Date	Sam. no	U/L
1	2023-10-17	1	35.47
2	2023-10-17	2	21.54
3	2023-10-30	1	40.09
4	2023-11-07	1	12.89
5	2023-11-07	2	11.21
6	2023-11-07	3	40.68

CARE DIAGNOSTICS & POLYCLINIC QC Chart

CKK100_Clinical_Chemistry_Analyser

Item:SGPT N:8 MEAN:36.125 SD:3.987 CV:0.110




CARE DIAGNOSTICS & POLYCLINIC

SGPT QC Lot:672 From:2023-10-17

Range:38.00-54.80


NO	Date	Sam. no	U/L
1	2023-10-17	1	34.23
2	2023-10-17	2	39.79
3	2023-10-30	1	40.50
4	2023-11-07	1	30.88
5	2023-11-07	2	30.62
6	2023-11-07	3	36.37
7	2023-11-08	1	36.34
8	2023-11-08	18	40.27


CARE DIAGNOSTICS
41/12-02, N.G. D. S. Colony,
Bagalur Road, HOSUR - 635 109.

CARE DIAGNOSTICS & POLYCLINIC QC Chart

CKK100_Clinical_Chemistry_Analyser

Item:UREA(UV) N:8 MEAN:43.201 SD:9.023 CV:0.209



CARE DIAGNOSTICS & POLYCLINIC

UREA(UV) QC Lot:672 From:2023-10-17

Range:29.50-39.90


NO	Date	Sam. no	mg/dl
1	2023-10-17	1	35.15
2	2023-10-30	1	53.61
3	2023-10-30	2	53.60
4	2023-10-30	3	51.70
5	2023-11-04	1	29.74
6	2023-11-07	1	43.28
7	2023-11-07	2	40.71
8	2023-11-07	3	37.82


CARE DIAGNOSTICS
4142-D2, N.G.G.O's Colony,
Bagalur Road, HOSUR - 635 109

CARE DIAGNOSTICS & POLYCLINIC QC Chart

CKK100_Clinical_Chemistry_Analyser

Item:CREAT N:7 MEAN:1.484 SD:0.162 CV:0.109



CARE DIAGNOSTICS & POLYCLINIC

CREAT QC Lot:672 From:2023-10-17

Range:1.02-1.46


NO	Date	Sam. no	mg/dl
1	2023-10-17	1	1.77
2	2023-10-17	2	1.41
3	2023-10-30	1	1.37
4	2023-11-07	1	1.62
5	2023-11-07	2	1.29
6	2023-11-19	1	1.44
7	2023-11-29	2	1.49


CARE DIAGNOSTICS
4/442-D2, N.G. 1st Colony,
Bagalur Road, HOSUR - 635 109.

CARE DIAGNOSTICS & POLYCLINIC QC Chart

CKK100_Clinical_Chemistry_Analyser

Item:TGL N:11 MEAN:70.735 SD:8.175 CV:0.116



CARE DIAGNOSTICS & POLYCLINIC

TGL QC Lot:672 From:2023-10-17


Range:69.00-94.80

NO	Date	Sam. no	mg/dl
1	2023-10-17	1	74.48
2	2023-10-30	1	87.98
3	2023-11-07	1	71.30
4	2023-11-19	1	66.76
5	2023-11-19	2	65.12
6	2023-11-19	4	64.80
7	2023-11-19	17	72.79
8	2023-11-29	1	59.87
9	2023-11-29	2	66.92
10	2023-11-29	5	66.44
11	2023-11-29	21	81.63

CARE DIAGNOSTICS & POLYCLINIC QC Chart

CKK100_Clinical_Chemistry_Analyser

Item:CHOL N:5 MEAN:73.250 SD:1.846 CV:0.025



CARE DIAGNOSTICS & POLYCLINIC

CHOL QC Lot:672 From:2023-10-17

Range:65.40-88.20


NO	Date	Sam. no	mg/dl
1	2023-10-17	1	73.85
2	2023-10-30	1	75.31
3	2023-11-07	1	71.95
4	2023-11-19	1	74.36
5	2023-11-29	1	70.78


CARE DIAGNOSTICS
4/442-D2, N.G. G. D. S Colony,
Bagalur Road, HOSUR - 635 109.

CARE DIAGNOSTICS & POLYCLINIC QC Chart

CKK100_Clinical_Chemistry_Analyser

Item:DTBIL N:3 MEAN:0.847 SD:0.035 CV:0.041




CARE DIAGNOSTICS & POLYCLINIC

DTBIL QC Lot:672 From:2023-10-17

Range:0.67-0.97

NO	Date	Sam. no	mg/dl
1	2023-10-17	1	0.85
2	2023-10-30	1	0.88
3	2023-11-07	1	0.81


CARE DIAGNOSTICS
#1142-D2 N.G.O. Colony,
Bagalur Road, HOBBAR - 555 109.