



CC-2146

# Indian Calibration Services

An Exclusive House for Validation & Calibration of Analytical Instruments  
304 & 313, Laxmi Deep, District Centre, Near Nirman Vihar Metro Station, Laxmi Nagar, Delhi-110092

Phone / Fax : (011) 22453259, 22434362, 9599482307

E-mail : indiancalibrationservices@gmail.com Website : www.multitechs.com



## CALIBRATION CERTIFICATE

Page 1 of 2

### CALIBRATION CERTIFICATE OF WATER BATH

Calibration Certificate No.	23100017582	Issued On:	29/08/2023
ULR No.	CC214623100017582F	Calibration Date:	26/08/2023
Job Identification No.	ICS/C/T/08/17582	Next Calibration Date:	25/08/2024
Ref. No:	SRF, Dated - 23/08/2023		

<b>CALIBRATED FOR:</b>	M/s Polo Labs Pvt Ltd., C/o IVY Hospital, Khanna (Punjab)
------------------------	---


EQUIPMENT DESCRIPTION			
Name	Water Bath	Visual Inspection	Ok
Make/Model	Seven Star	I.D. No.	POLO/KH/WB/01
Serial No.		Least Count	1°C
Range	0 to 110°C (Set At 37°C)	Calibration Site	On-Site
Location	Lab		

ENVIRONMENTAL CONDITIONS			
Temperature	25.0 °C ± 5.0 °C	Humidity	50 ± 15 % RH

STANDARD REFERENCE DETAILS				
Traceable to National / International Standard				
Name of the Standard	Make	Certificate No.	Calibration Agency/Traceability	Date of Calibration
Dig. Multichannel Data Logger	Microcubus	23100000030	Indian Calibration Services, Delhi	05/01/2023
				Valid up to 05/01/2024

<b>USED EQUIPMENT DETAILS</b>	N/A
<b>PRINCIPLE/METHODOLOGY OF CALIBRATION:</b>	As per Calibration Procedure No.: ICS-CAL/SOP-TH04, ITS-90 (Comparison Method)


<b>RESULTS: Thermal Calibration (Temperature)</b>										
All readings are in "°C"										
Set Value in °C	Measured Average Value in (°C) (Avg.)									Uncertainty(with 95% C.L. at k=2) (°C)
	S-1	S-2	S-3	S-4	S-5	S-6	S-7	S-8	S-9	
37	37.6	37.5	37.3	37.2	37.1	37.7	37.2	37.0	37.2	± 1.1
<b>Max Stability:-</b>	0.4									
<b>Max Uniformity:-</b>	0.5									

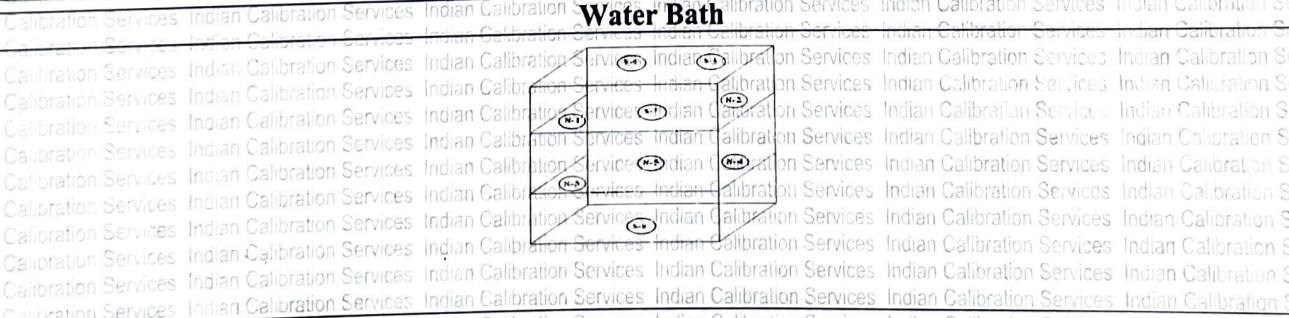

Remarks: - Calibration results are enclosed.

- Note :**
- This report is not to be reproduced wholly or in part and cannot be used as an evidence in the Court of Law and should not be used in any advertising media without our special permission in writing.
  - The result listed refer only to the tested samples and applicable parameters. Endorsement of products is neither inferred nor implied.
  - Total liability of our Organisation is limited to the invoiced amount.
  - Samples will be destroyed after one month from the date of issue of Calibration Certificate unless otherwise specified.
  - In case any reconfirmation of contents of this Calibration Certificate is required. Please contact our office.
  - The calibration certificate/Test Report is valid only for the condition of the UUC at the time under stated condition of calibration.

For and on behalf of  
**Indian Calibration Services**

Checked by  RAJESH KUMAR  
Authorized Signatory  
Operation Head