

PARTICIPANT FINAL ASSESSMENT REPORT (SUMMARY)

PT SCHEME: BIOCHEMISTRY

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6

Report Date : 22/11/2023

Sample : SEP 2023

All Methods

	Parameters	Labs (n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
1	HDL-CHOL	29	26.47	mg/dL	54.05	10.45	2.785	2.64	Questionable
2	UREA	36	46.00	mg/dL	56.61	7.87	1.739	1.35	Satisfactory
3	GLUCOSE	36	24.99	mg/dL	18.49	5.41	1.177	1.20	Satisfactory
4	BILIRUBIN	35	7.68	mg/dL	17.82	6.56	1.577	1.55	Satisfactory
5	TOTAL PROTEIN	35	2.20	g/dL	2.08	0.57	0.121	0.20	Good
6	ALBUMIN	35	1.75	g/dL	1.92	0.28	0.059	0.62	Good
7	CHOLESTEROL	34	130.81	mg/dL	134.47	8.28	2.029	0.44	Good
8	TRIGLYCERIDES	30	108.00	mg/dL	122.19	23.04	6.005	0.62	Good
9	CREATININE	36	7.00	mg/dL	7.82	0.93	0.202	0.89	Good
10	AST	36	11.00	U/L	15.32	5.86	1.337	0.74	Good
11	ALT	36	8.00	U/L	10.45	4.60	1.050	0.53	Good
12	URIC ACID	34	8.42	mg/dL	8.12	1.74	0.372	0.17	Good
13	ALKALINE PHOSPHATASE	35	83.79	U/L	81.62	10.78	2.593	0.20	Good
14	DIRECT BILIRUBIN	33	6.15	mg/dL	6.80	3.86	0.928	0.17	Good
15	CALCIUM	27	8.50	mg/dL	9.71	1.92	0.462	0.63	Good
16	SODIUM	31	Not Recvd.	mmol/L	130.81	7.48	1.680		N/A
17	POTASSIUM	31	Not Recvd.	mmol/L	4.65	0.40	0.090		N/A
18	CHLORIDE	30	Not Recvd.	mmol/L	100.81	6.96	1.644		N/A

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 1 of 22



PARTICIPANT FINAL ASSESSMENT REPORT (SUMMARY)

PT SCHEME: BIOCHEMISTRY

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6

Report Date : 22/11/2023

Sample : SEP 2023

Peer group

	Parameters	Labs (n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
19	CHOLESTEROL (CHOD-POD)	10	130.81	mg/dL	138.10	3.50		2.08	Questionable
20	BILIRUBIN (Others)	6	7.68	mg/dL	15.75	3.67		2.20	Questionable
21	HDL-CHOL (Others)	5	26.47	mg/dL	56.20	14.25		2.09	Questionable
22	ALKALINE PHOSPHATASE (Others)	7	83.79	U/L	66.00	6.46		2.75	Questionable
23	UREA (U V Kinetic GLDH)	7	46.00	mg/dL	54.00	5.62		1.42	Satisfactory
24	GLUCOSE (GOD-POD)	12	24.99	mg/dL	20.25	4.86		0.97	Good
25	CREATININE (Jaffe-Kinetic)	4	7.00	mg/dL	7.36	0.65		0.56	Good
26	TOTAL PROTEIN (Biuret)	27	2.20	g/dL	1.93	0.50	0.121	0.54	Good
27	ALBUMIN (BCG)	27	1.75	g/dL	1.95	0.28	0.068	0.70	Good
28	CALCIUM (Arsenazo)	8	8.50	mg/dL	9.15	2.67		0.24	Good
29	DIRECT BILIRUBIN (Others)	5	6.15	mg/dL	5.03	2.99		0.38	Good
30	GGTP (IFCC)	13	59.81	U/L	57.42	* 12.67	4.151	0.19	Good
31	URIC ACID (Others)	4	8.42	mg/dL	6.89	2.12		0.72	Good
32	ALT (UV-Kinetic)	3	8.00	U/L	16.20	11.60		0.71	Good
33	AST (UV-Kinetic)	3	11.00	U/L					N/A

Authorised Signatory

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor




Dr. Sujay Prasad
Technical Manager and Program coordinator

This report is for use only by the intended participant.

Dr Venkatesh

Page 2 of 22



PARTICIPANT FINAL ASSESSMENT REPORT (SUMMARY)

PT SCHEME: BIOCHEMISTRY

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6

Report Date : 22/11/2023

Sample : SEP 2023

Peer group

	Parameters	Labs (n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
34	TRIGLYCERIDES (Others)	1	108.00	mg/dL					N/A

Interpretation of z scores is as follows:

- | Z score | ≤ 1.0 – Good
- | Z score | between 1.0 to 2.0 - Satisfactory
- | Z score | between 2.0 to 3.0 - Questionable
- | Z score | ≥ 3.0 - Unsatisfactory

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

Page 3 of 22

This report is for use only by the intended participant.

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

ALBUMIN


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	35	1.75	g/dL	1.92	0.28	0.059	0.62	Good

ZScore

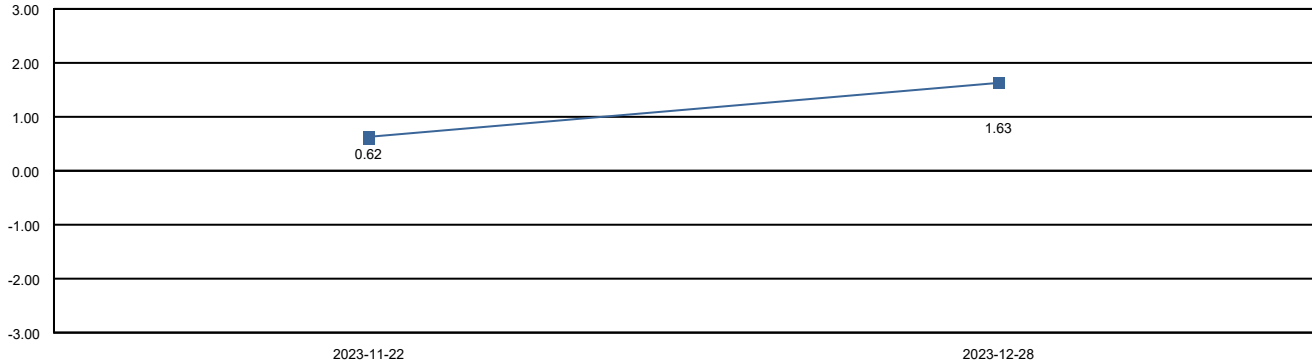

Peer group (BCG)	27	1.75	g/dL	1.95	0.28	0.068	0.70	Good
------------------	----	------	------	------	------	-------	------	------

ZScore

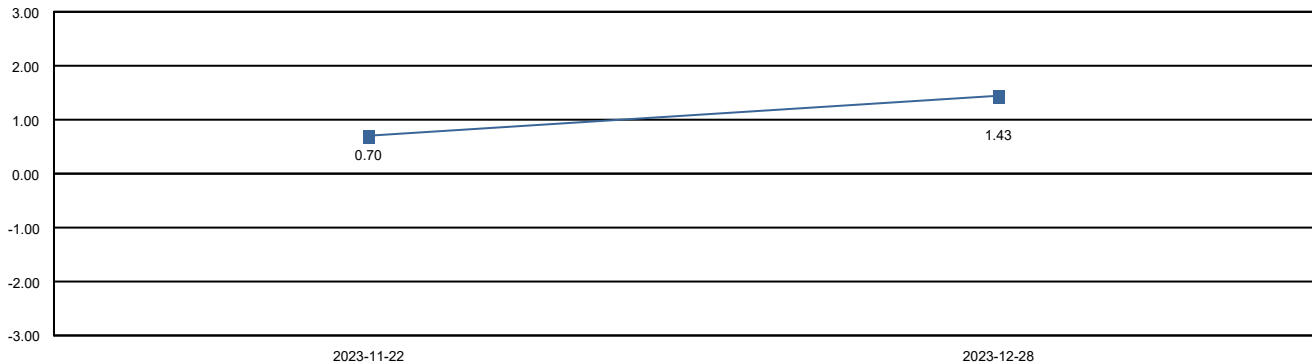

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 4 of 22

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

ALKALINE PHOSPHATASE


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (Others)	7	83.79	U/L	66.00	6.46		2.75	Questionable

ZScore

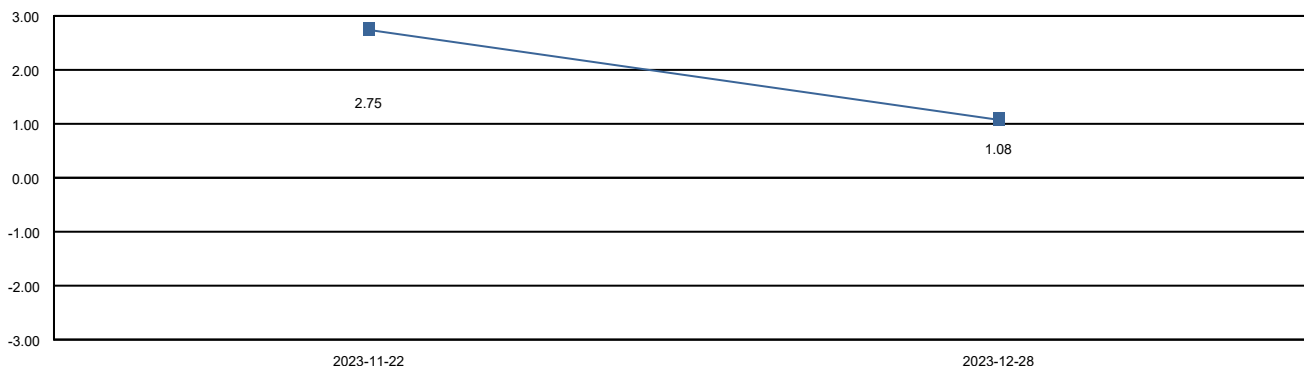


All Methods	35	83.79	U/L	81.62	10.78	2.593	0.20	Good
-------------	----	-------	-----	-------	-------	-------	------	------

ZScore

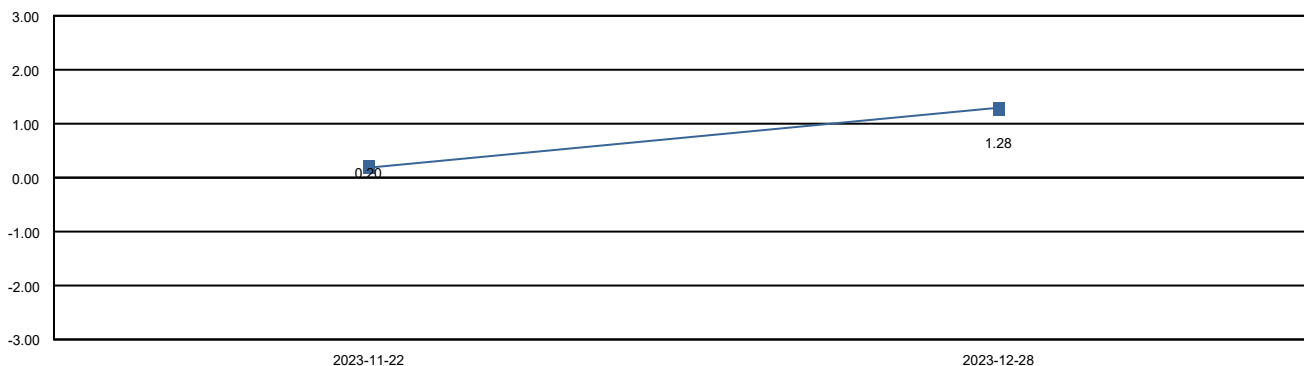

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 5 of 22

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

ALT

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	36	8.00	U/L	10.45	4.60	1.050	0.53	Good

ZScore

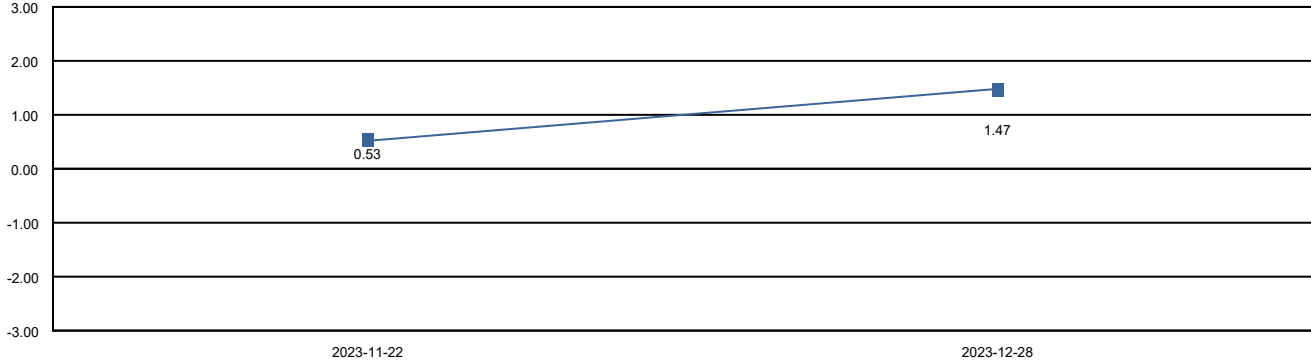

Peer group (UV-Kinetic)	3	8.00	U/L	16.20	11.60		0.71	Good
-------------------------	---	------	-----	-------	-------	--	------	------

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 6 of 22

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

AST

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	36	11.00	U/L	15.32	5.86	1.337	0.74	Good

ZScore

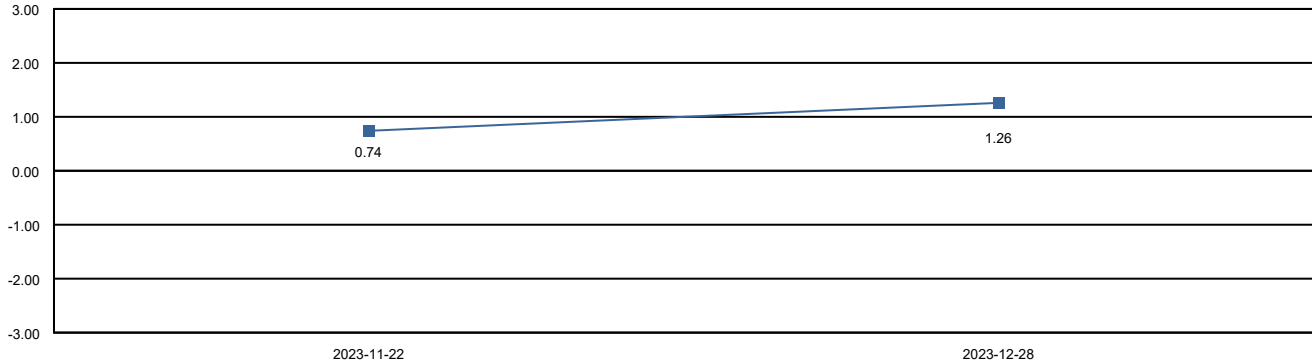

Peer group (UV-Kinetic)	3	11.00	U/L					N/A
-------------------------	---	--------------	-----	--	--	--	--	-----

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 7 of 22

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

BILIRUBIN


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (Others)	6	7.68	mg/dL	15.75	3.67		2.20	Questionable

ZScore

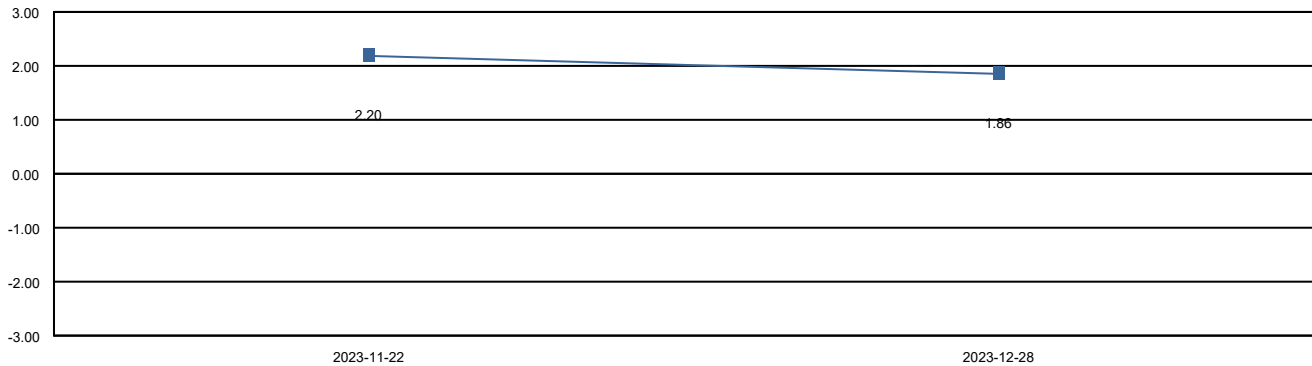

All Methods	35	7.68	mg/dL	17.82	6.56	1.577	1.55	Satisfactory
--------------------	-----------	-------------	-------	-------	------	-------	------	--------------

ZScore

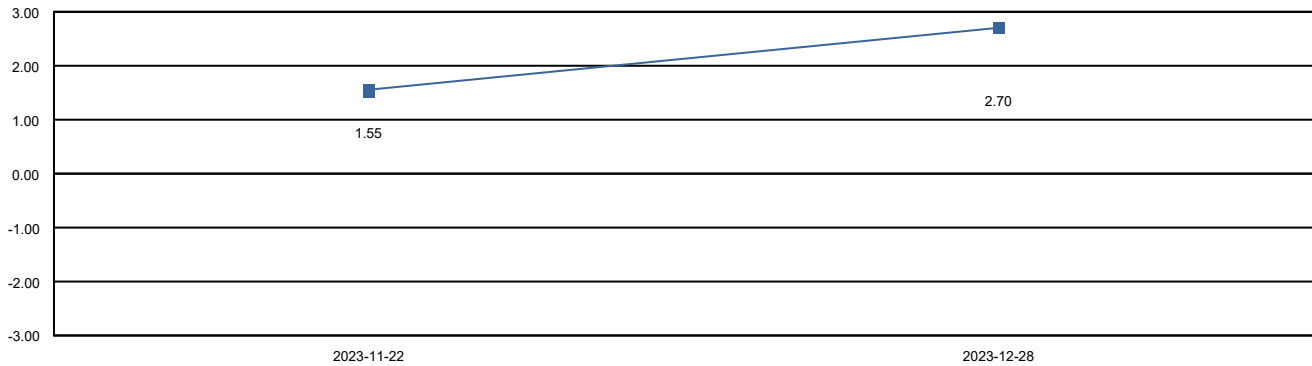

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 8 of 22

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

CALCIUM


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	27	8.50	mg/dL	9.71	1.92	0.462	0.63	Good

ZScore

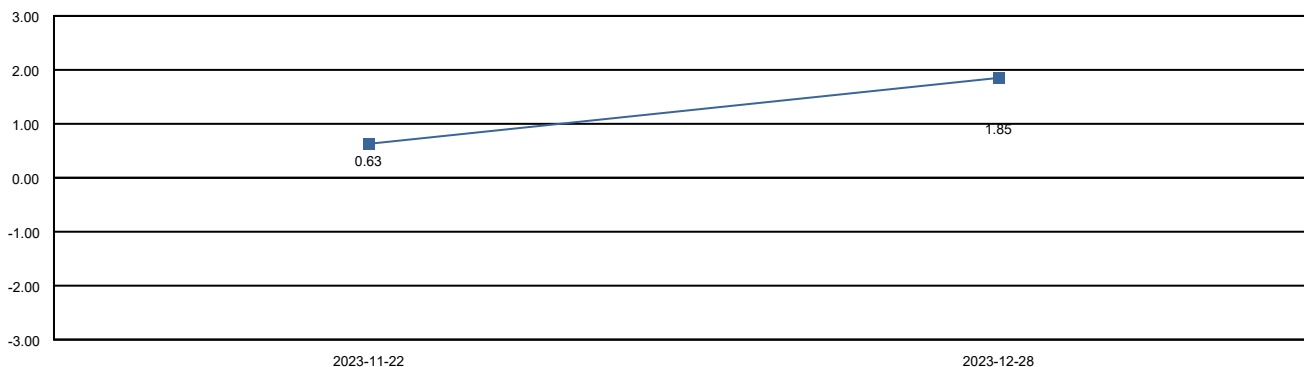


Peer group (Arsenazo)	8	8.50	mg/dL	9.15	2.67		0.24	Good
-----------------------	---	-------------	-------	------	------	--	------	------

ZScore

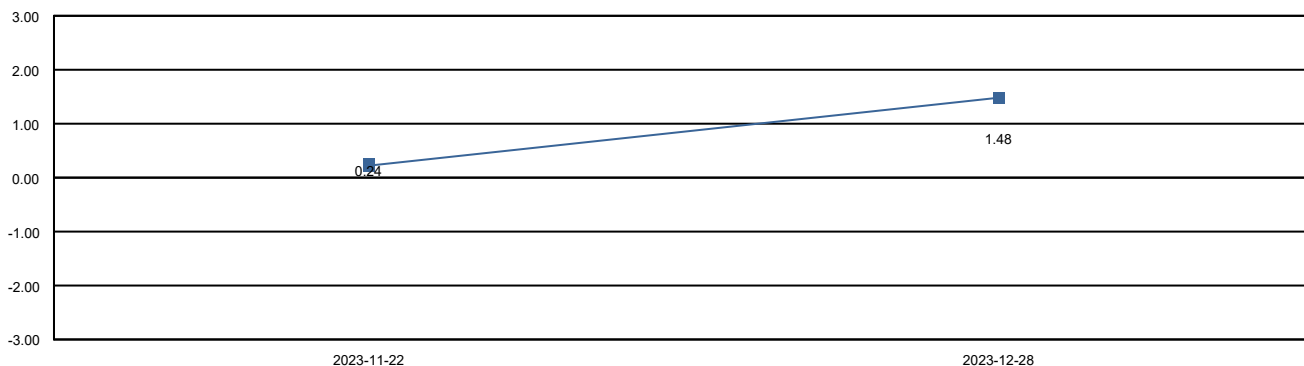

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 9 of 22



Neu-QAP

(an EXTERNAL QUALITY ASSURANCE PROGRAMME)

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY



PC-1047

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6

Report Date : 22/11/2023

Sample : SEP 2023

CHLORIDE

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	30	Not Recvd.	mmol/L	100.81	6.96	1.644		N/A

Authorised Signatory

Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor

Dr Venkatesh

Page 10 of 22

This report is for use only by the intended participant.



An external quality assurance program from
NEUBERG ANAND ACADEMY OF LABORATORY MEDICINE PVT.LTD.

Anand Tower, 54, Bowring Hospital Road,
Shivajinagar, Bangalore - 560001
+91-9902277355 · qap@naalm.com · www.naalm.com
CIN: U85300KA2018PTC115147

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

CHOLESTEROL


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (CHOD-POD)	10	130.81	mg/dL	138.10	3.50		2.08	Questionable

ZScore

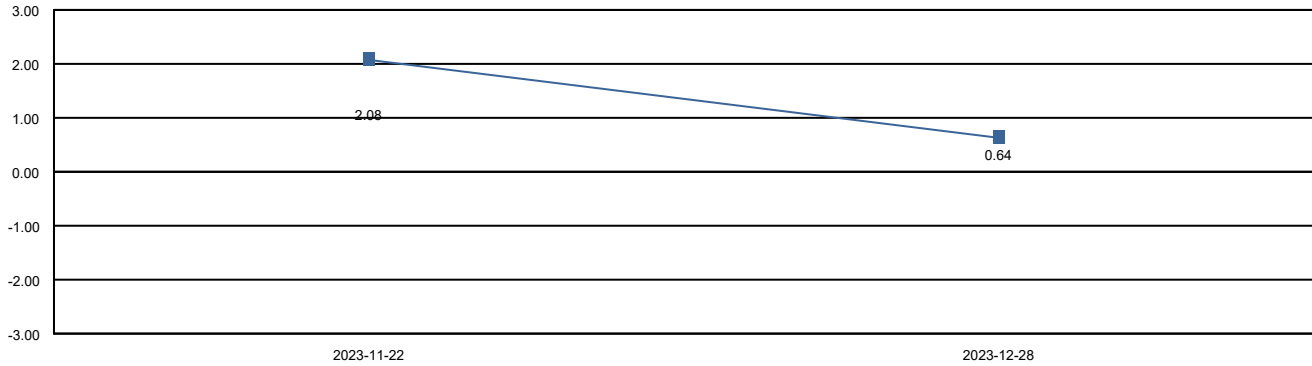

All Methods	34	130.81	mg/dL	134.47	8.28	2.029	0.44	Good
-------------	----	--------	-------	--------	------	-------	------	------

ZScore

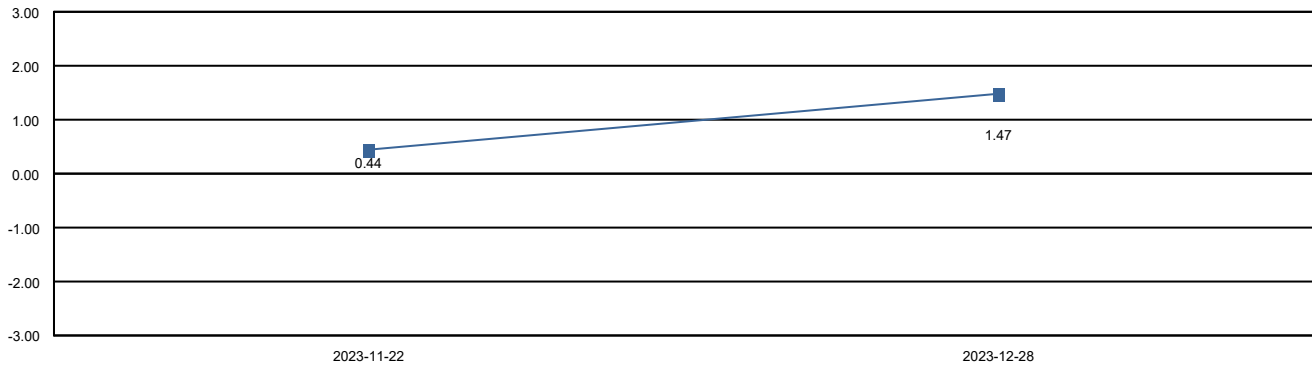

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 11 of 22

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

CREATININE


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	36	7.00	mg/dL	7.82	0.93	0.202	0.89	Good

ZScore

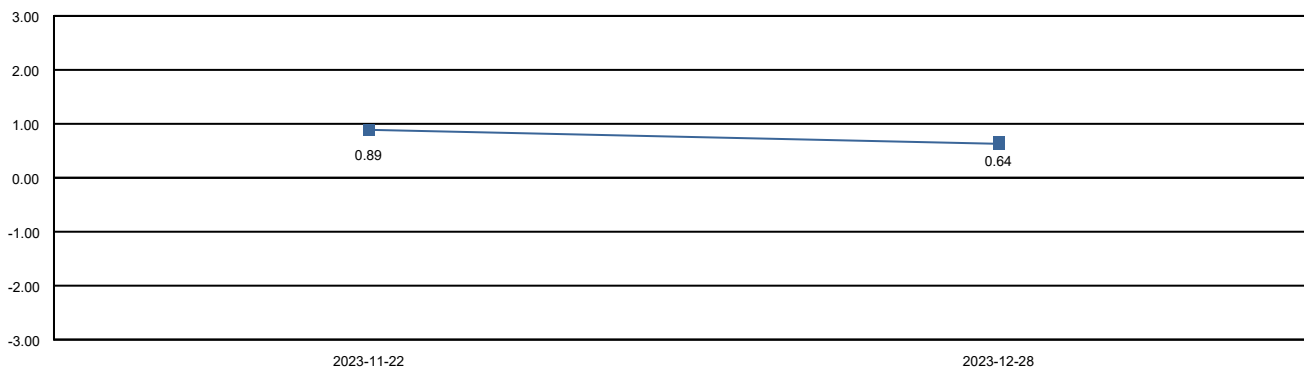


Peer group (Jaffe-Kinetic)	4	7.00	mg/dL	7.36	0.65		0.56	Good
----------------------------	---	-------------	-------	------	------	--	------	------

ZScore

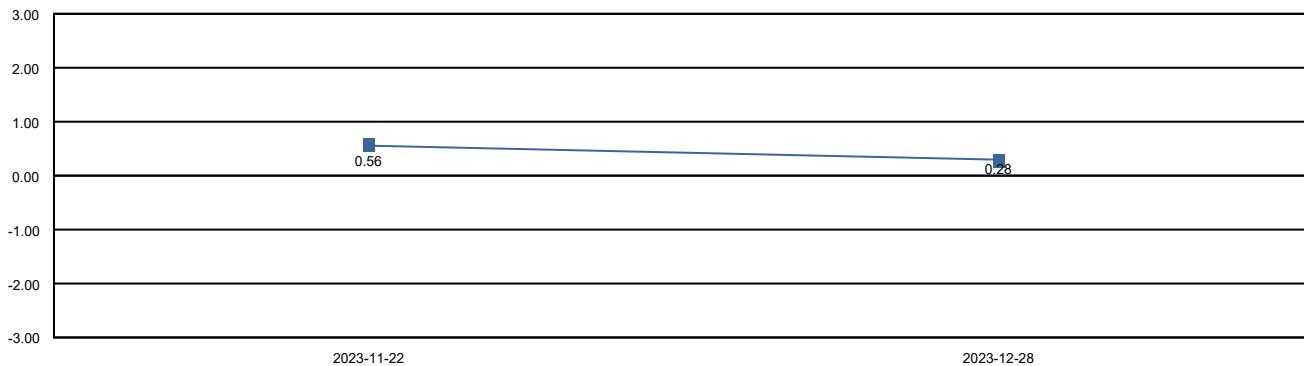

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 12 of 22



PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6

Report Date : 22/11/2023

Sample : SEP 2023

DIRECT BILIRUBIN

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	33	6.15	mg/dL	6.80	3.86	0.928	0.17	Good



Peer group (Others)	5	6.15	mg/dL	5.03	2.99		0.38	Good
---------------------	---	-------------	-------	------	------	--	------	------



Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh
Page 13 of 22

This report is for use only by the intended participant.



Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

GGTP

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (IFCC)	13	59.81	U/L	57.42	* 12.67	4.151	0.19	Good

ZScore

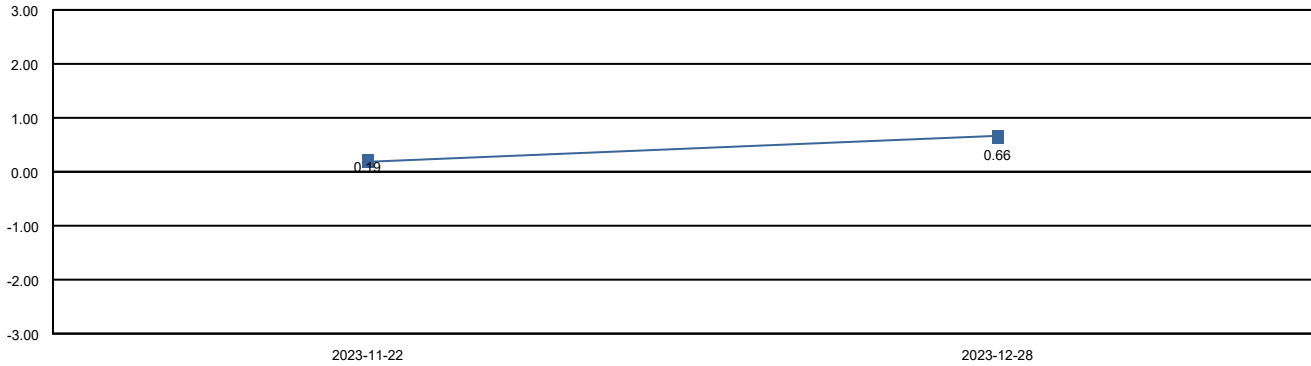

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

Page 14 of 22

This report is for use only by the intended participant.



Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

GLUCOSE


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	36	24.99	mg/dL	18.49	5.41	1.177	1.20	Satisfactory

ZScore

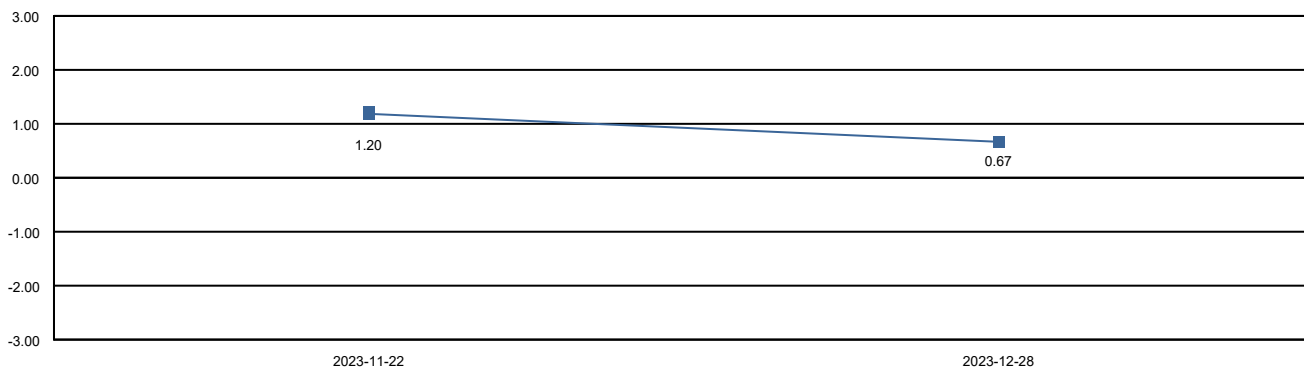


Peer group (GOD-POD)	12	24.99	mg/dL	20.25	4.86		0.97	Good
----------------------	----	--------------	-------	-------	------	--	------	------

ZScore

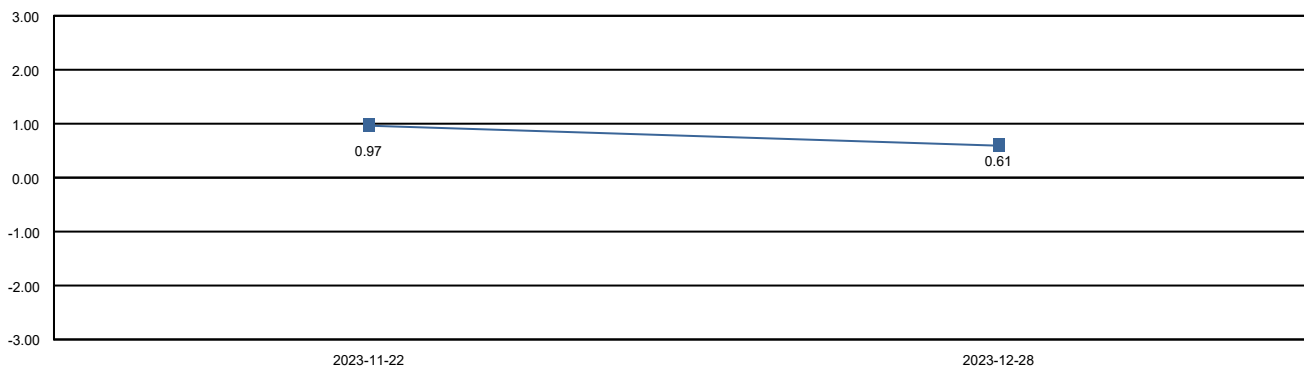

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 15 of 22

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

HDL-CHOL


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	29	26.47	mg/dL	54.05	10.45	2.785	2.64	Questionable

ZScore

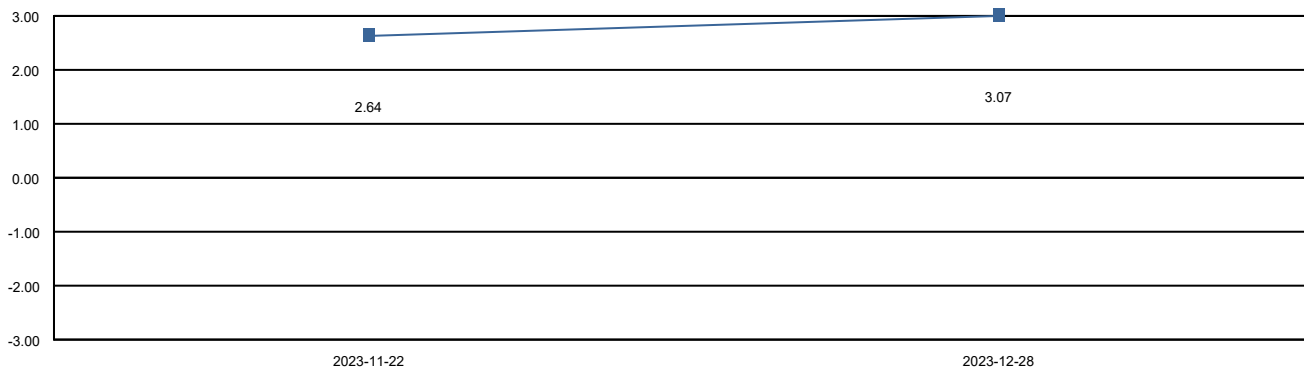


Peer group (Others)	5	26.47	mg/dL	56.20	14.25		2.09	Questionable
---------------------	---	--------------	-------	-------	-------	--	------	--------------

ZScore

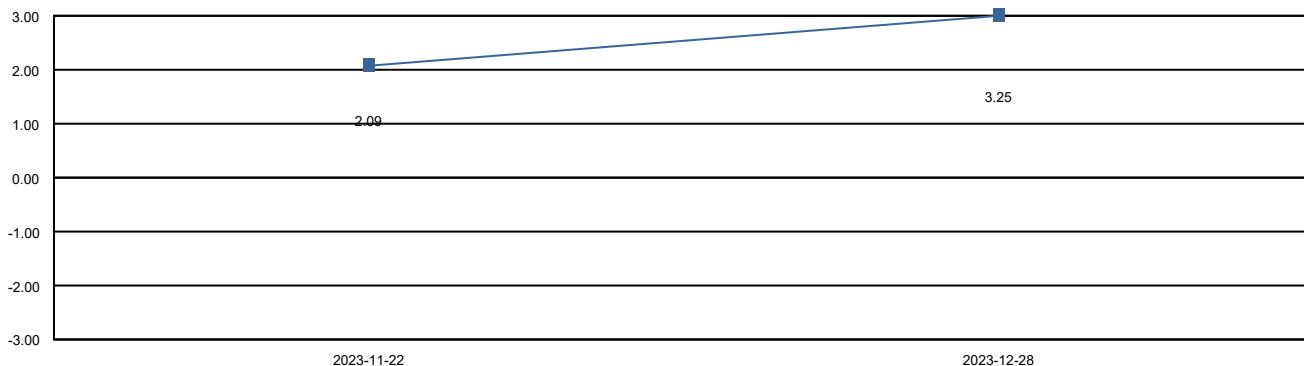

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 16 of 22



Neu-QAP

(an EXTERNAL QUALITY ASSURANCE PROGRAMME)

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY



PC-1047

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6

Report Date : 22/11/2023

Sample : SEP 2023

POTASSIUM

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	31	Not Recvd.	mmol/L	4.65	0.40	0.090		N/A

Authorised Signatory

Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor

Dr Venkatesh

Page 17 of 22

This report is for use only by the intended participant.



An external quality assurance program from
NEUBERG ANAND ACADEMY OF LABORATORY MEDICINE PVT.LTD.

Anand Tower, 54, Bowring Hospital Road,
Shivajinagar, Bangalore - 560001
+91-9902277355 · qap@naalm.com · www.naalm.com
CIN: U85300KA2018PTC115147



Neu-QAP

(an EXTERNAL QUALITY ASSURANCE PROGRAMME)

PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY



PC-1047

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6

Report Date : 22/11/2023

Sample : SEP 2023

SODIUM

Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	31	Not Recvd.	mmol/L	130.81	7.48	1.680		N/A

Authorised Signatory

Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor

Dr Venkatesh

Page 18 of 22

This report is for use only by the intended participant.



An external quality assurance program from
NEUBERG ANAND ACADEMY OF LABORATORY MEDICINE PVT.LTD.

Anand Tower, 54, Bowring Hospital Road,
Shivajinagar, Bangalore - 560001
+91-9902277355 · qap@naalm.com · www.naalm.com
CIN: U85300KA2018PTC115147

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

TOTAL PROTEIN


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	35	2.20	g/dL	2.08	0.57	0.121	0.20	Good

ZScore

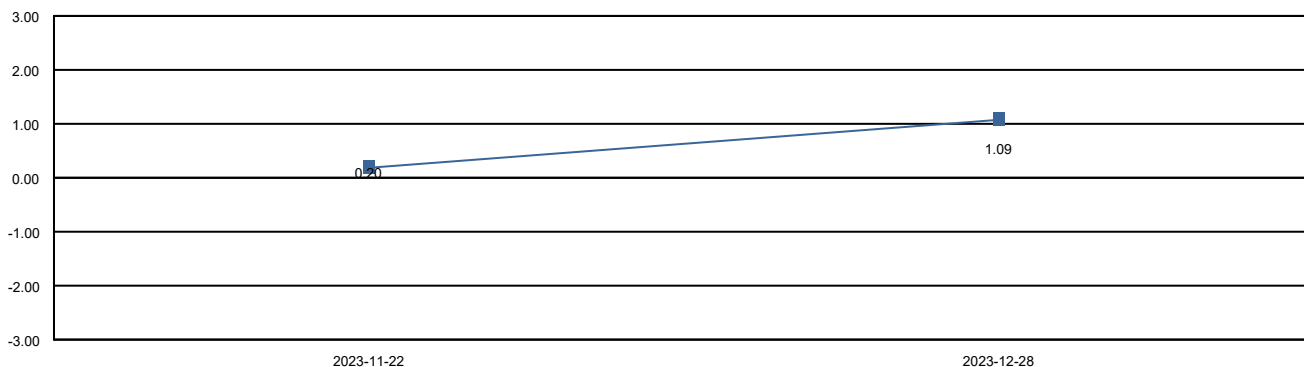


Peer group (Biuret)	27	2.20	g/dL	1.93	0.50	0.121	0.54	Good
---------------------	----	------	------	------	------	-------	------	------

ZScore

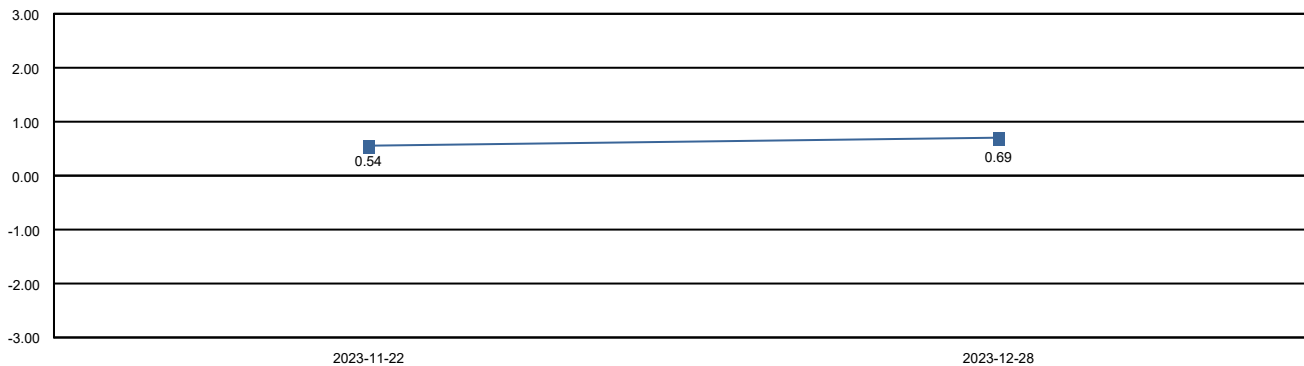

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh
Page 19 of 22

This report is for use only by the intended participant.



Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

TRIGLYCERIDES


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	30	108.00	mg/dL	122.19	23.04	6.005	0.62	Good

ZScore

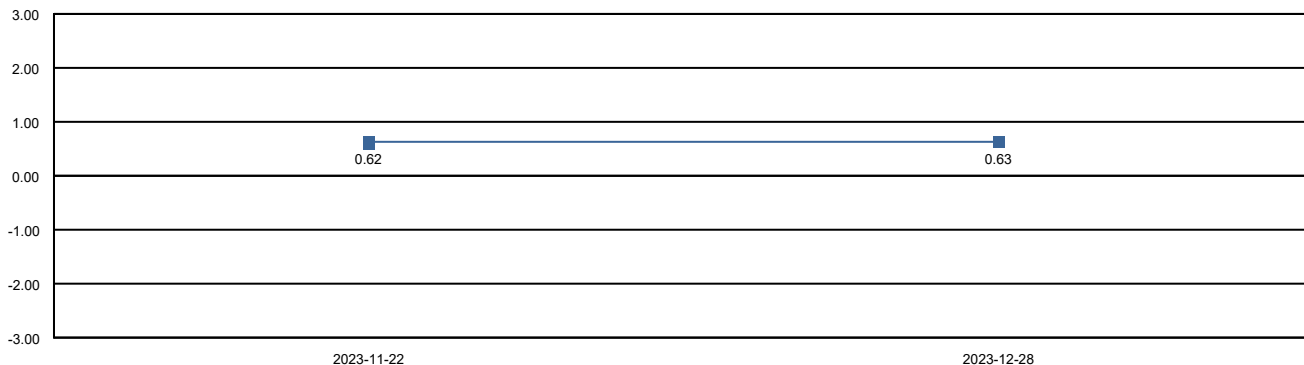

Peer group (Others)	1	108.00	mg/dL					N/A
---------------------	---	---------------	-------	--	--	--	--	-----

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

Page 20 of 22

This report is for use only by the intended participant.



PARTICIPANT FINAL ASSESSMENT REPORT (NORMAL)

PT SCHEME: BIOCHEMISTRY

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

UREA


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
Peer group (U V Kinetic GLDH)	7	46.00	mg/dL	54.00	5.62		1.42	Satisfactory

ZScore

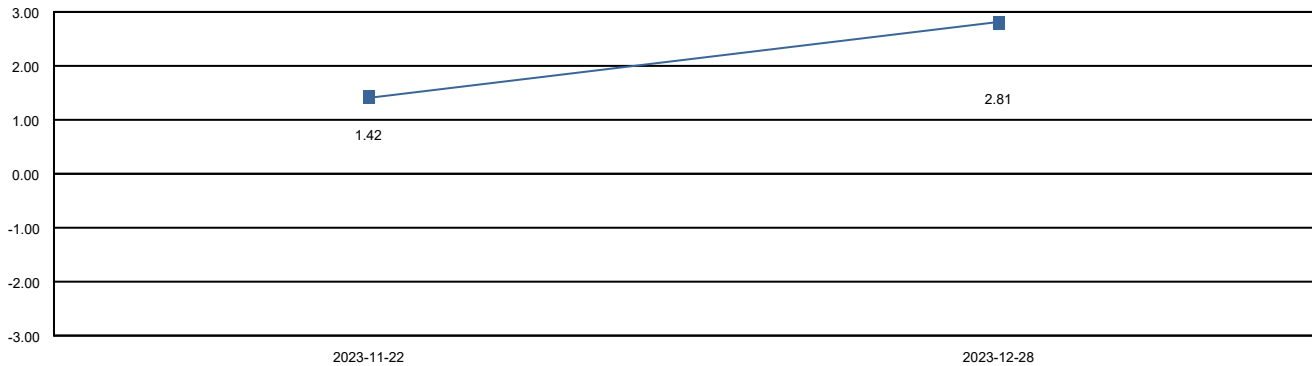

All Methods	36	46.00	mg/dL	56.61	7.87	1.739	1.35	Satisfactory
-------------	----	--------------	-------	-------	------	-------	------	--------------

ZScore

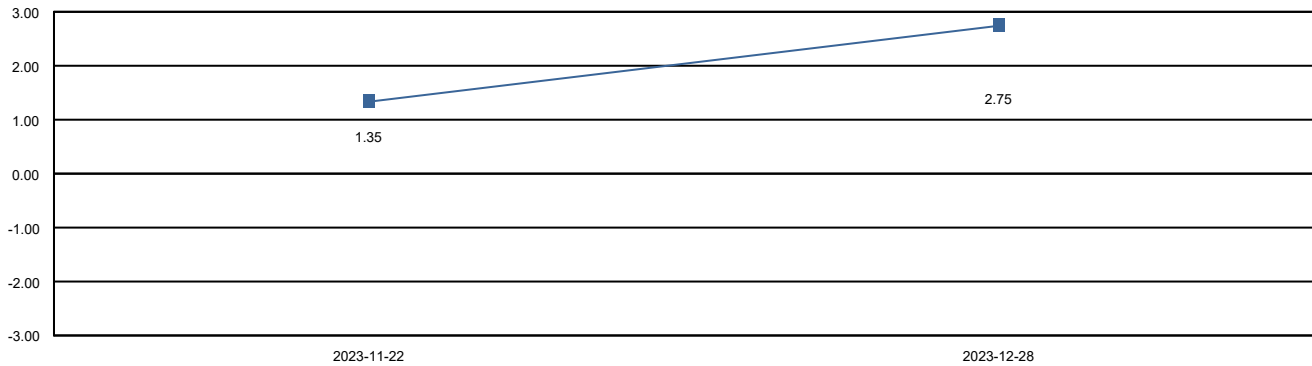

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

This report is for use only by the intended participant.

Page 21 of 22

Cycle No	C5
Ref.No.	NEUQAP608
Sample ID	NEUQAP BIO SERUM/2023/9/C5/S6


Report Date : 22/11/2023

Sample : SEP 2023

URIC ACID


Parameters	Labs(n)	Lab Value	Unit	Assigned value	SDPA	Um	Z-Score	Remarks
All Methods	34	8.42	mg/dL	8.12	1.74	0.372	0.17	Good

ZScore

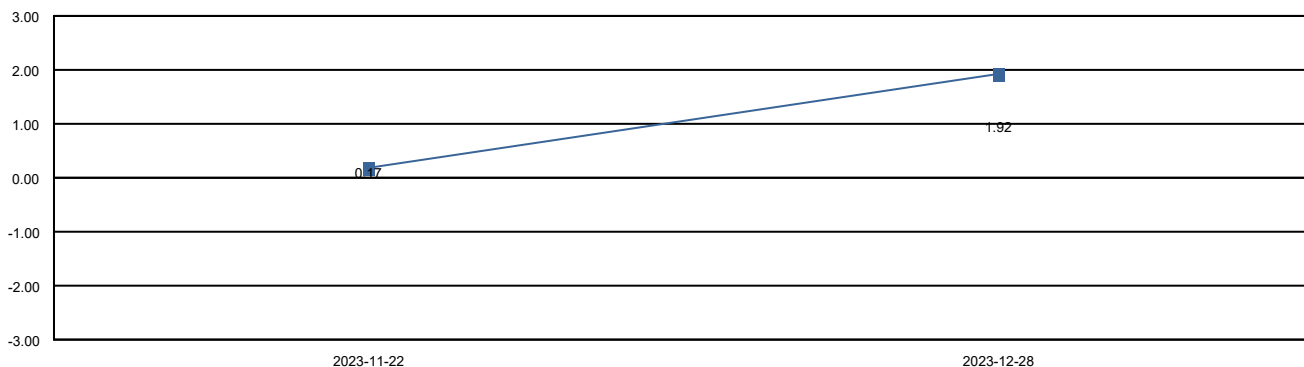

Peer group (Others)	4	8.42	mg/dL	6.89	2.12		0.72	Good
---------------------	---	-------------	-------	------	------	--	------	------


ZScore

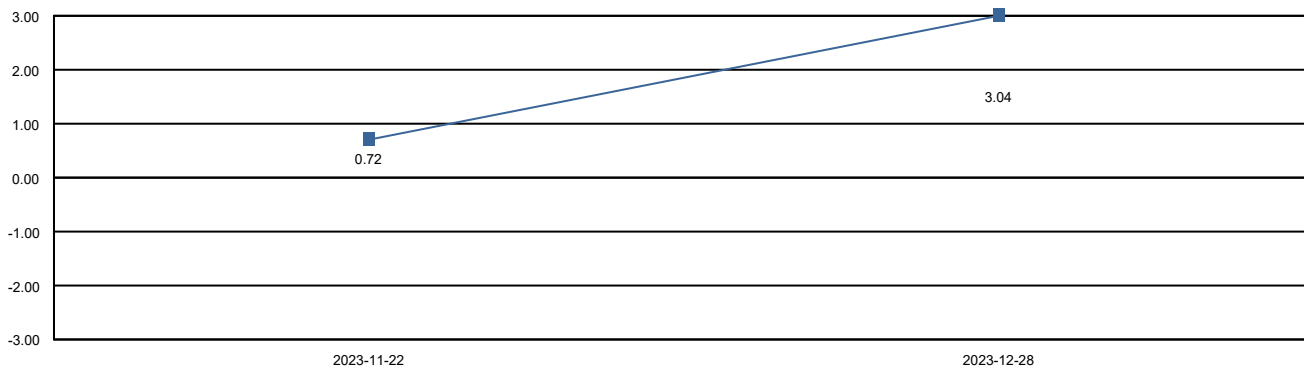

Note: Sample generation, homogeneity and stability testing activities are subcontracted to ISO 15189:2012 accredited laboratory . Lyophilisation of samples is subcontracted to ISO 9001:2015 manufacturing facility .

****End of report ****

Authorised Signatory



Dr. Sujay Prasad
Technical Manager and Program coordinator

* denotes adjusted SDPA as per ISO 13528:2015(E)
SDPA - Standard Deviation for Proficiency Assessment

Technical Advisor



Dr Venkatesh

Please refer to NEUQAP Web portal for all subcontracted activ
This report is for use only by the intended participant.

