


**MINDRAY BC 20S - CALIBRATION CERTIFICATE**

<b>Customer Name</b>	DR'S PATH LAB (A UNIT OF HARDEVI CHERITABLE TRUST) , BHARATPUR					
<b>Department</b>	Department of Pathology					
<b>Address</b>	: Plot No. 42 C , kothi Dalveer Singh , Near Multipurpose Chauraha Bharatpur					
				<b>Date of Calibration</b>	26-12-2023	
<b>Instrument</b>	<b>BC-5300 Auto Haematology Analyzer</b>			<b>Next Calibration Date</b>	25-03-2024	
<b>Serial No</b>	RD-73101503			<b>Calibrator Lot Number</b>	PLUS0523	
				<b>Calibrator Expiry date</b>	25-01-2024	
<b><u>Calibration Values</u></b>	<b><u>Parameter</u></b>	<b><u>Target</u></b>	<b><u>Range</u></b>	<b><u>Mean of Measured Values</u></b>	<b><u>Factor</u></b>	<b><u>Old Factor</u></b>
	WBC x 10 <sup>9</sup> /L	9.40	9.20-9.60	9.36	106.43	105.70
	RBC x10 <sup>12</sup> /L	4.43	4.35-4.51	4.39	107.42	109.20
	HGB g/dL	13.3	13.1-13.5	13.2	111.02	112.00
	MCV fl	89.0	87.0-91.0	88.7	102.42	100.50
	PLT x 10 <sup>9</sup> /L	239	227-251	228	105.57	113.00

This is to certify that the Mindray BC 20S Hematology Analyzer with Serial No: RD-73101503, installed at DR'S PATH LAB, Bharatpur has been calibrated using the standard reference material PLUS0620 Calibrator.

Reviewed By :

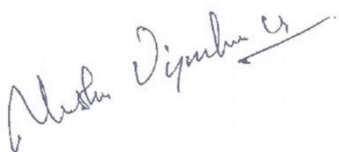


26/12/2023

Manager – Application  
Golden Harvest Industries.