



Metropolis Healthcare Ltd., EQAS

KRSNAA DIAGNOSTICS LTD, BATALA (1034)

Outlier And Analyte Summary Report

Outlier Details For Cycle No 230310 and Sample No 01

Report Date : 19/12/2023

Analyte	Instrument	Result Value	Standard Unit
X Widal test - ParaTyphi B-H antigen (BH)	Manual	1:160	-
Legend @ : Acceptable X : Unacceptable # : Not Evaluated ⌚ Delayed Result Entry			

Problem Classification: _____

Corrective Action: _____

Reviewed by: _____

Dated: _____

Instrument : J Mitra


Analyte	Standard Unit	Result Value	Accepted Value
@ HBsAg	IU/mL	Non-reactive	Non-reactive
@ HCV	IU/mL	Non-reactive	Non-reactive
@ HIV Ab	S/CO	Non-reactive	Non-reactive

Instrument : Manual

Analyte	Standard Unit	Result Value	Accepted Value
@ RPR (Syphilis Serology)	-	Non-reactive	Non-reactive
@ Dengue NS 1	RU/ml	Negative	Negative
@ Widal test - Typhi O antigen (TO)	-	1:80	1:80, NoA
@ Widal test - Typhi H antigen (TH)	-	1:80	1:80, NoA
@ Widal test - ParaTyphi A-H antigen (AH)	-	No Agglutination	1:80, NoA
X Widal test - ParaTyphi B-H antigen (BH)	-	1:160	1:80, NoA
@ Dengue IgM	RU/ml	Negative	Negative
@ Dengue IgG	RU/ml	Negative	Negative

Legend @ : Acceptable
 @ : Acceptable
 X : Unacceptable
 # : Not Evaluated
 ⌚ : Delayed Result Entry

Total Parameters	11
Not Evaluated Parameters	0
Evaluated Parameters	11
Outlier Parameters (X)	1
EQAS Score Immunoassay Extended	90.91 %



Dr Puneet Kumar Nigam
 PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A
 Kohinoor Mall, Kirool Road, Kurla (W),
 Mumbai - 400070



Metropolis Healthcare Ltd., EQAS

KRSNAA DIAGNOSTICS LTD, BATALA (1034)

Outlier And Analyte Summary Report

Outlier Details For Cycle No 230310 and Sample No 02

Report Date : 19/12/2023

Analyte	Instrument	Result Value	Standard Unit
No Outlier			
Legend @ : Acceptable X : Unacceptable # : Not Evaluated ⌚ : Delayed Result Entry			

Problem Classification: _____

Corrective Action: _____

Reviewed by: _____ **Dated:** _____

Instrument : J Mitra


Analyte	Standard Unit	Result Value	Accepted Value
@ HBsAg	IU/mL	Reactive	Reactive
@ HCV	IU/mL	Non-reactive	Non-reactive
@ HIV Ab	S/CO	HIV-1 Ab Reactive	HIV-1 Ab Reactive

Instrument : Manual

Analyte	Standard Unit	Result Value	Accepted Value
@ RPR (Syphilis Serology)	-	Non-reactive	Non-reactive
@ Dengue NS 1	RU/ml	Negative	Negative
@ Widal test - Typhi O antigen (TO)	-	1:80	1:80,NoA
@ Widal test - Typhi H antigen (TH)	-	1:80	1:80,NoA
@ Widal test - ParaTyphi A-H antigen (AH)	-	No Agglutination	1:80,NoA
@ Widal test - ParaTyphi B-H antigen (BH)	-	No Agglutination	1:80,NoA
@ Dengue IgM	RU/ml	Negative	Negative
@ Dengue IgG	RU/ml	Negative	Negative

Legend @ : Acceptable
 @ : Acceptable
 X : Unacceptable
 # : Not Evaluated
 ⌚ : Delayed Result Entry

Total Parameters	11
Not Evaluated Parameters	0
Evaluated Parameters	11
Outlier Parameters (X)	0
EQAS Score Immunoassay Extended	100.00 %



Dr Puneet Kumar Nigam
 PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A
 Kohinoor Mall, Kiroil Road, Kurla (W),
 Mumbai - 400070



Metropolis Healthcare Ltd., EQAS

KRSNAA DIAGNOSTICS LTD, BATALA (1034)

Outlier And Analyte Summary Report

Outlier Details For Cycle No 230310 and Sample No 03

Report Date : 19/12/2023

Analyte	Instrument	Result Value	Standard Unit
No Outlier			
Legend @ : Acceptable X : Unacceptable # : Not Evaluated ⌚ Delayed Result Entry			

Problem Classification: _____

Corrective Action: _____

Reviewed by: _____


Dated: _____

Instrument : J Mitra

Analyte	Standard Unit	Result Value	Accepted Value
@ HBsAg	IU/mL	Reactive	Reactive
@ HCV	IU/mL	Reactive	Reactive
@ HIV Ab	S/CO	HIV-1 Ab Reactive	HIV-1 Ab Reactive

Legend @ : Acceptable
 @ : Acceptable
 X : Unacceptable
 # : Not Evaluated
 ⌚ : Delayed Result Entry

Total Parameters	3
Not Evaluated Parameters	0
Evaluated Parameters	3
Outlier Parameters (X)	0
EQAS Score Immunoassay Extended	100.00 %



Dr Puneet Kumar Nigam
 PT coordinator & Technical Manager, MHL EQAS
 Unit No. 409-416.
 Commercial Building - 1A
 Kohinoor Mall, Kiroi Road, Kurla (W),
 Mumbai - 400070

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023


Immunoassay Extended, Dengue IgG, -

	N
■ All Methods	103
■ Immunochromatography - (Your Method)	89
■ Manual - (Your Analyzer)	96

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

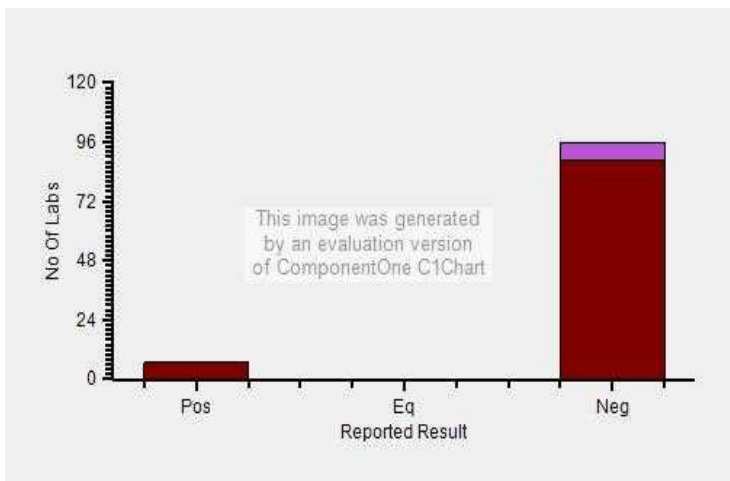

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

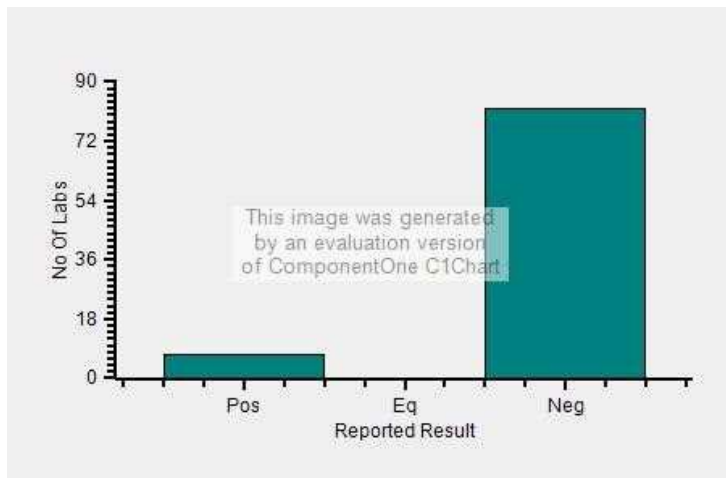

Frequency Histogram Your Analyzer

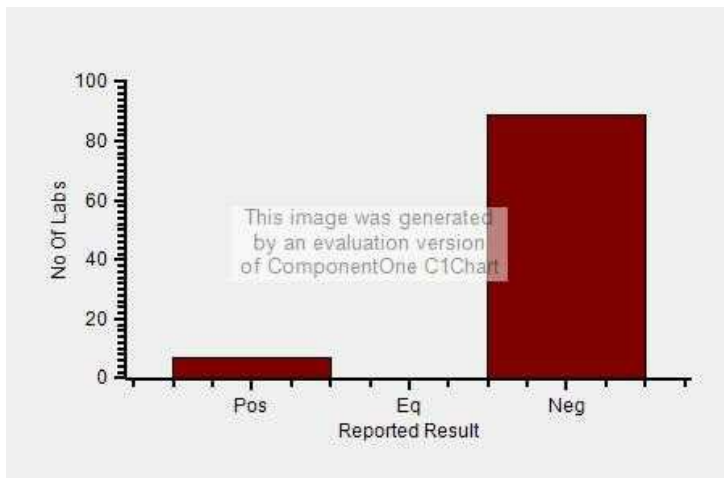

Reported Results Legends :-

- Pos** : Positive
- Eq** : Equivocal
- BL** : Borderline
- Neg** : Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023


Immunoassay Extended, Dengue IgM, -

	N
■ All Methods	103
■ Immunochromatography - (Your Method)	89
■ Manual - (Your Analyzer)	96

<table border="0" style="width: 100%;"> <tr> <td style="width: 60%;">Your Result</td> <td style="text-align: right;">Negative</td> </tr> <tr> <td>Result Expected</td> <td style="text-align: right;">Neg</td> </tr> </table>	Your Result	Negative	Result Expected	Neg
Your Result	Negative			
Result Expected	Neg			

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

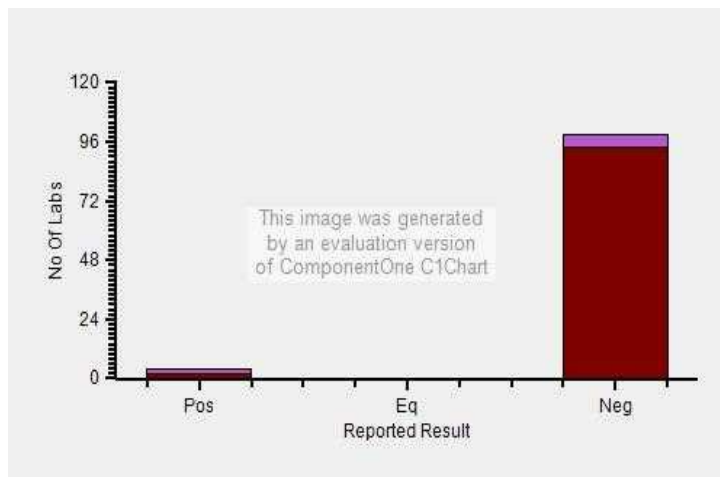

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 01

Sample Date : 25/11/2023

Frequency Histogram Your Method

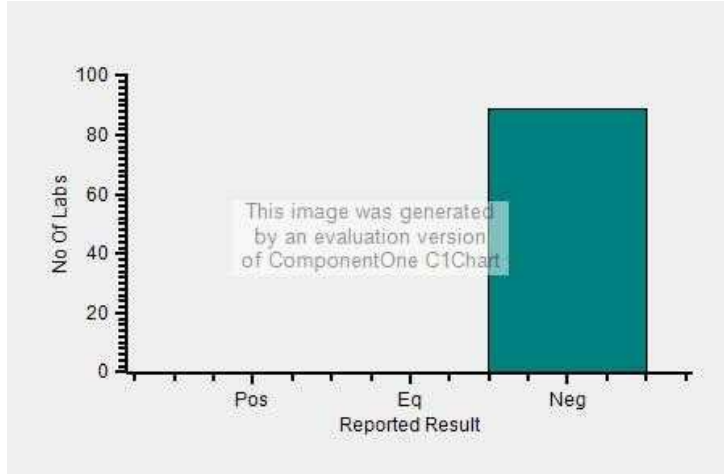

Frequency Histogram Your Analyzer

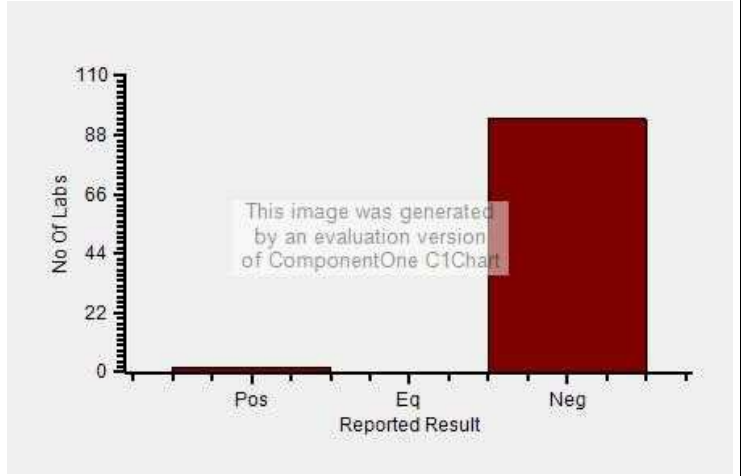

Reported Results Legends :-

- Pos** : Positive
- Eq** : Equivocal
- BL** : Borderline
- Neg** : Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Cycle No : 230310

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01

Report Date : 19/12/2023

Sample Date : 25/11/2023


Immunoassay Extended, Dengue NS 1, -

	N
■ All Methods	208
■ Immunochromatography - (Your Method)	184
■ Manual - (Your Analyzer)	196

Your Result Negative Result Expected Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

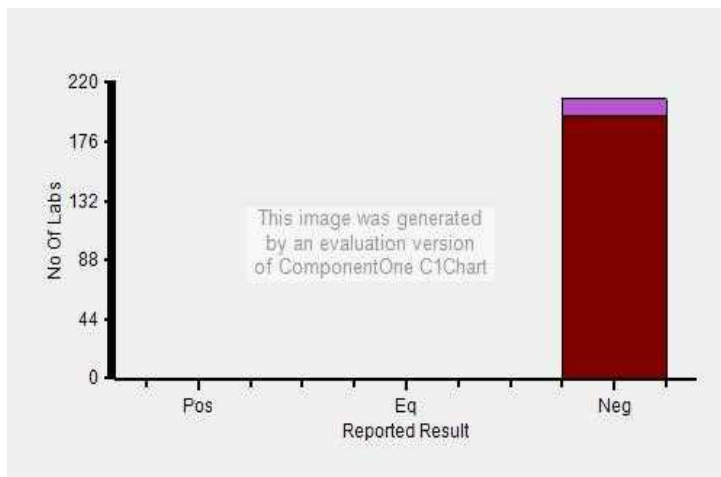

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

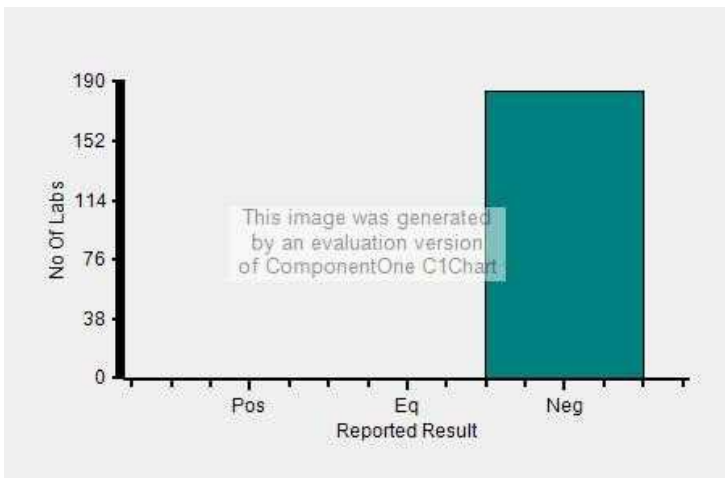

Frequency Histogram Your Analyzer

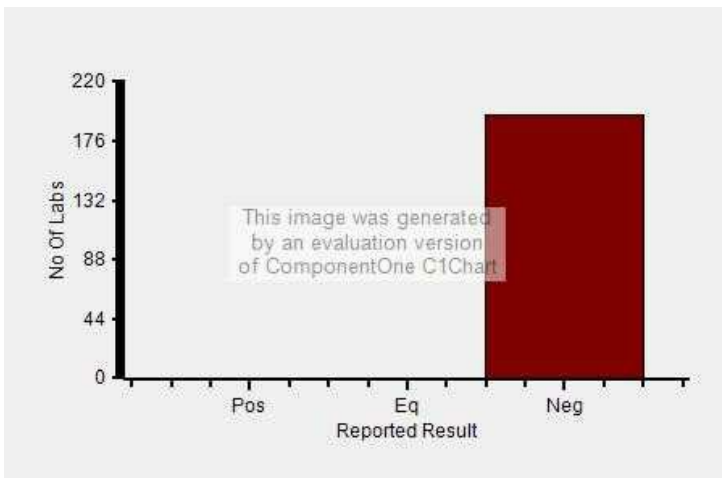

Reported Results Legends :-

- Pos** : Positive
- Eq** : Equivocal
- BL** : Borderline
- Neg** : Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Cycle No : 230310

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01

Report Date : 19/12/2023

Sample Date : 25/11/2023


Immunoassay Extended, HBsAg, -

	N
■ All Methods	288
■ Immunochromatography - (Your Method)	209
■ J Mitra - (Your Analyzer)	36

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

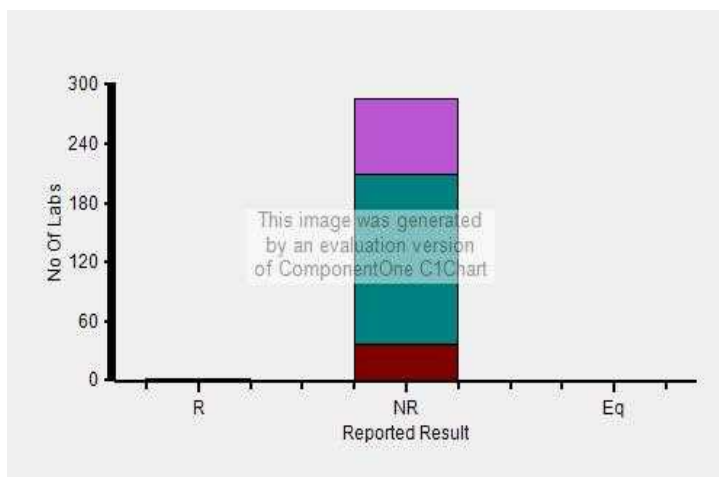

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 01

Sample Date : 25/11/2023

Frequency Histogram Your Method

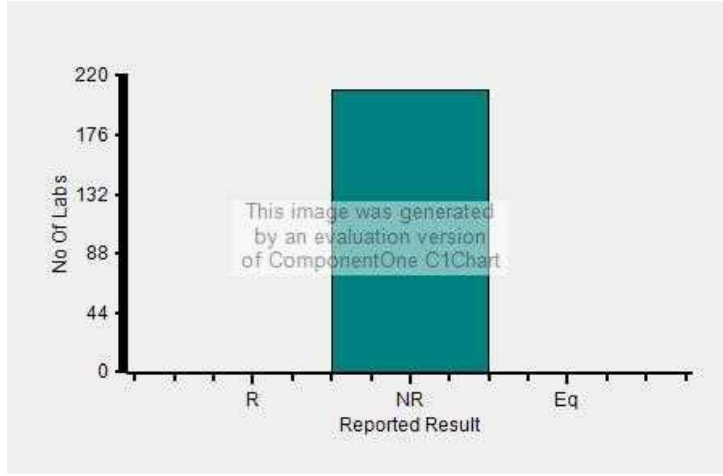

Frequency Histogram Your Analyzer

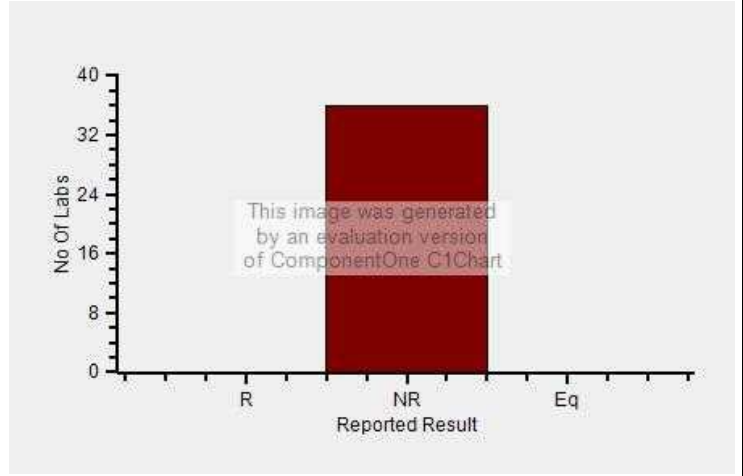

Reported Results Legends :-

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Cycle No : 230310

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01

Report Date : 19/12/2023

Sample Date : 25/11/2023


Immunoassay Extended, HCV, Nil

	N
■ All Methods	263
■ Immunofiltration - (Your Method)	31
■ J Mitra - (Your Analyzer)	35

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

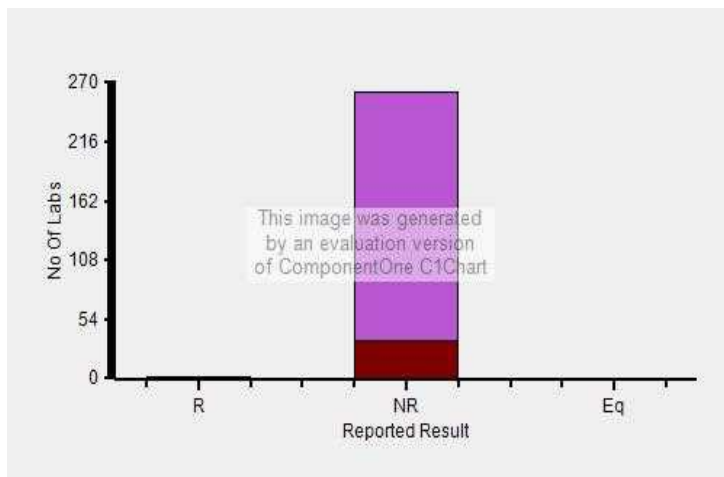

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 01

Sample Date : 25/11/2023

Frequency Histogram Your Method

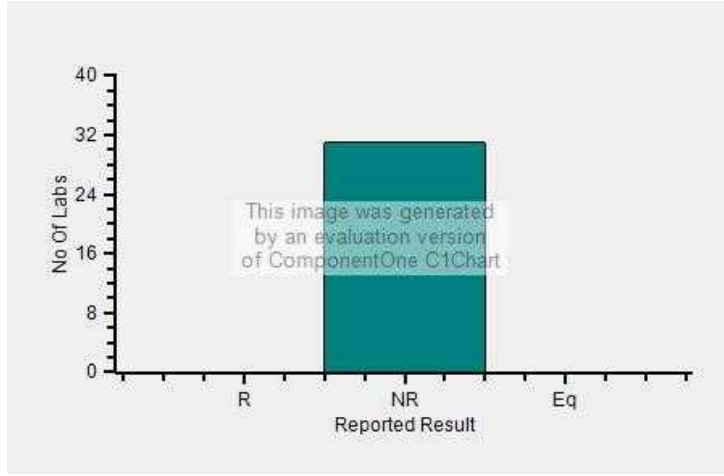

Frequency Histogram Your Analyzer

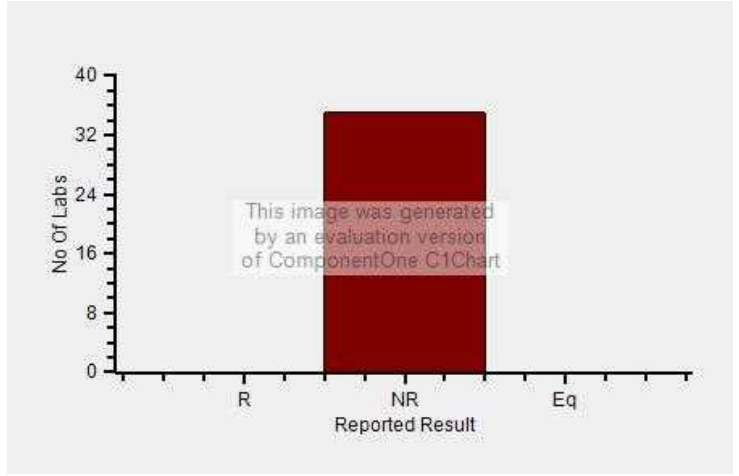

Reported Results Legends :-

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023


Immunoassay Extended, HIV Ab, S/CO

	N
■ All Methods	190
■ Immunofiltration - (Your Method)	32
■ J Mitra - (Your Analyzer)	36

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

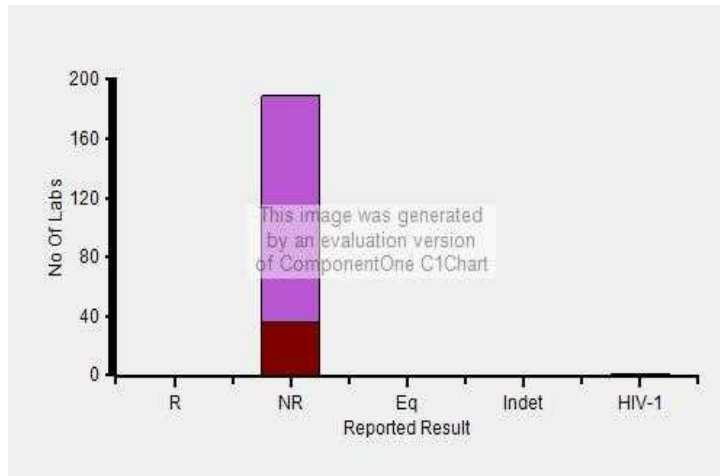

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

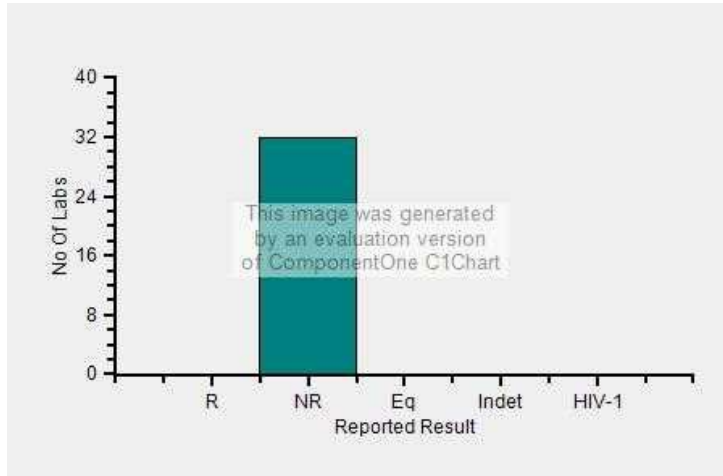

Frequency Histogram Your Analyzer

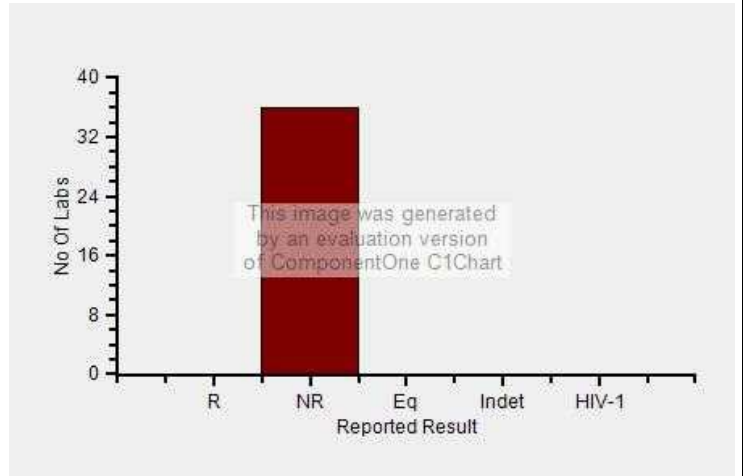

Reported Results Legends :-

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal
- Indet** : Indeterminate
- HIV-1** : HIV-1 Ab Reactive
- HIV-2** : HIV-2 Ab Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Cycle No : 230310

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01

Report Date : 19/12/2023

Sample Date : 25/11/2023


Immunoassay Extended, RPR (Syphilis Serology), -

	N
■ All Methods	234
■ Immunochromatography - (Your Method)	91
■ Manual - (Your Analyzer)	234

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

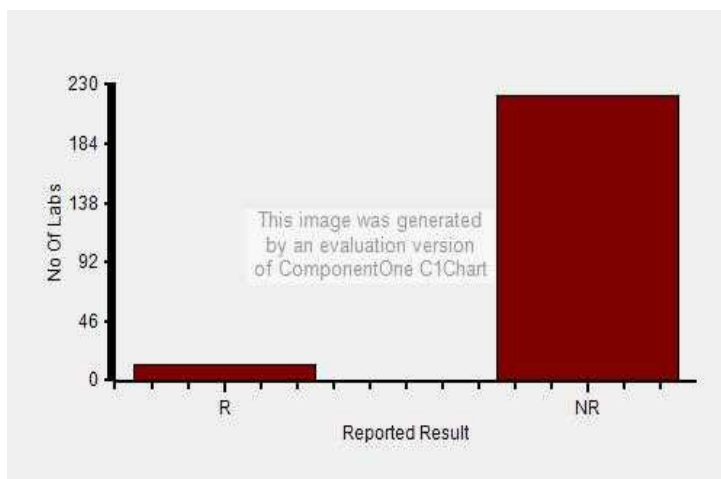

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

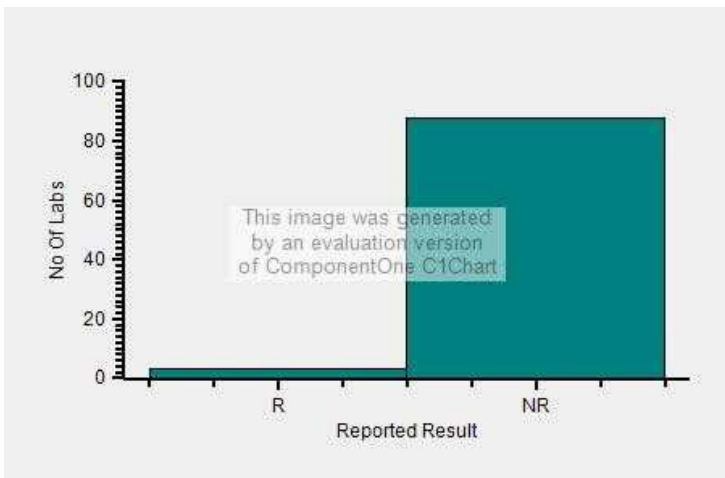

Frequency Histogram Your Analyzer

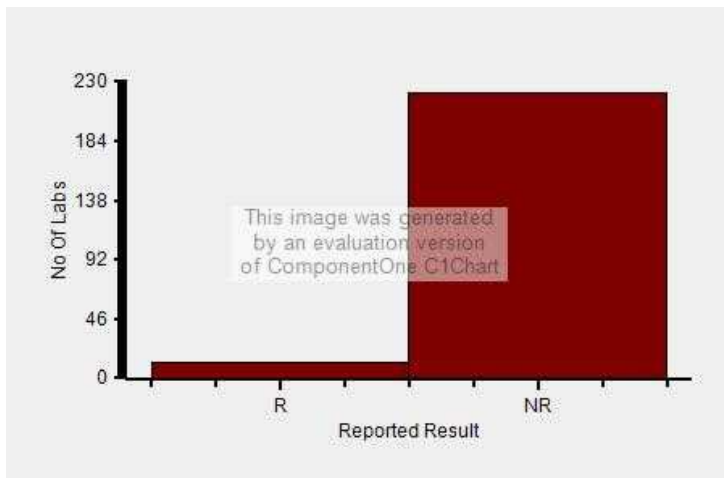

Reported Results Legends :-

R	: Reactive
NR	: Non-reactive
WR	: Weak Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023

Immunoassay Extended, Widal test - ParaTyphi A-H antigen (AH), -

	N
■ All Methods	219
■ Tube Agglutination - (Your Method)	49
■ Manual - (Your Analyzer)	219


Evaluation Based On - Method wise Peer Grouping

Your Result No Agglutination

Result Expected 1:80,NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

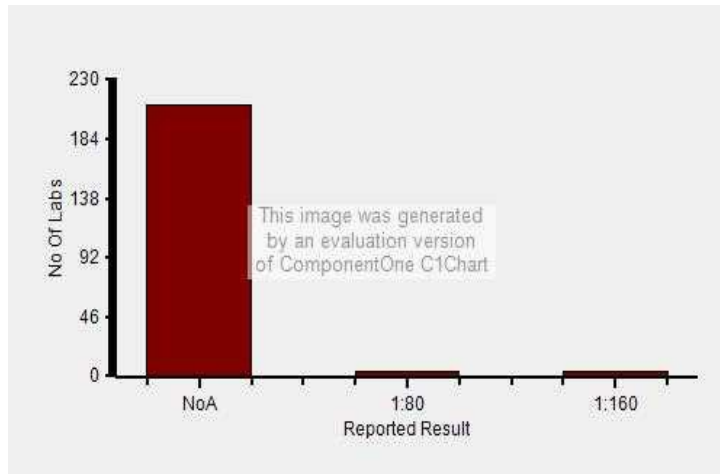

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 01

Sample Date : 25/11/2023

Frequency Histogram Your Method

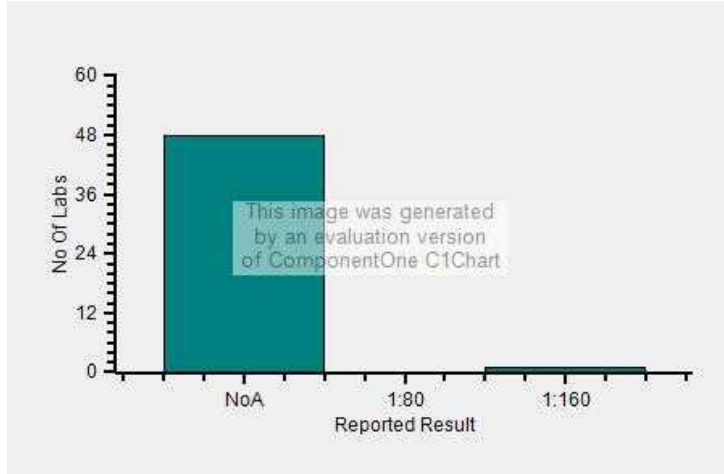

Frequency Histogram Your Analyzer

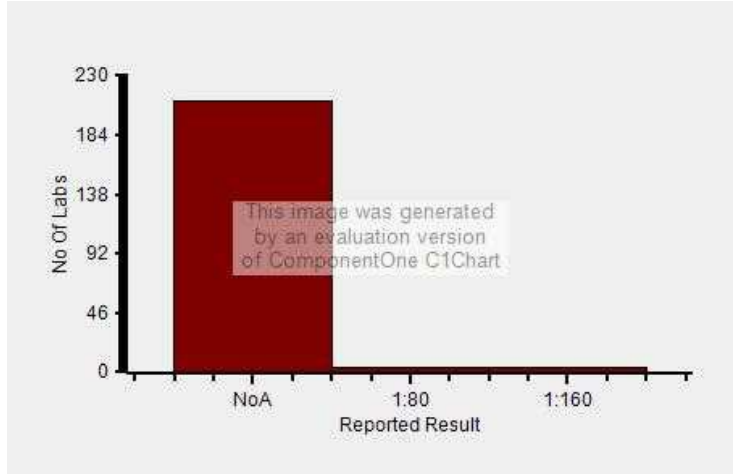

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023


Immunoassay Extended, Widal test - ParaTyphi B-H antigen (BH), -

	N
■ All Methods	219
■ Tube Agglutination - (Your Method)	49
■ Manual - (Your Analyzer)	219

Evaluation Based On - Method wise Peer Grouping	
Your Result	1:160
Result Expected	1:80,NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

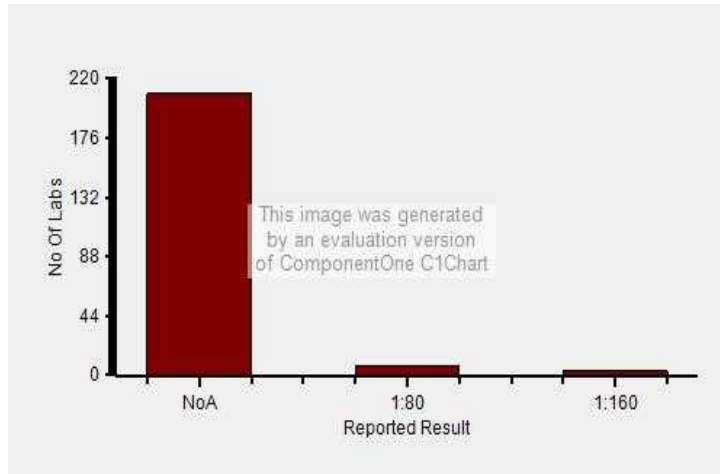

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

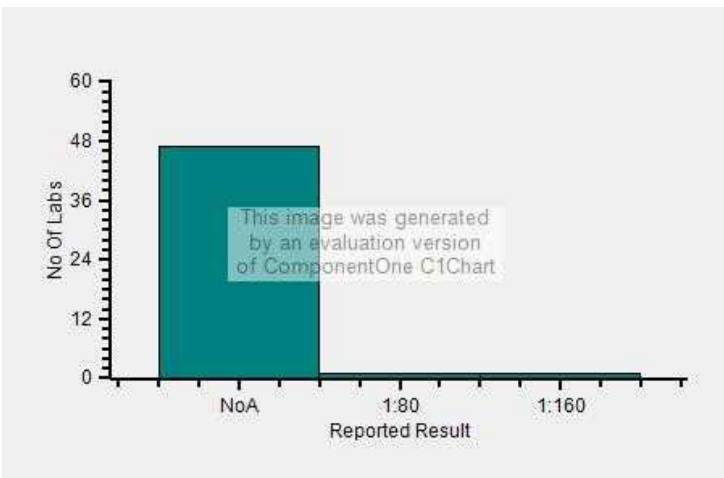

Frequency Histogram Your Analyzer

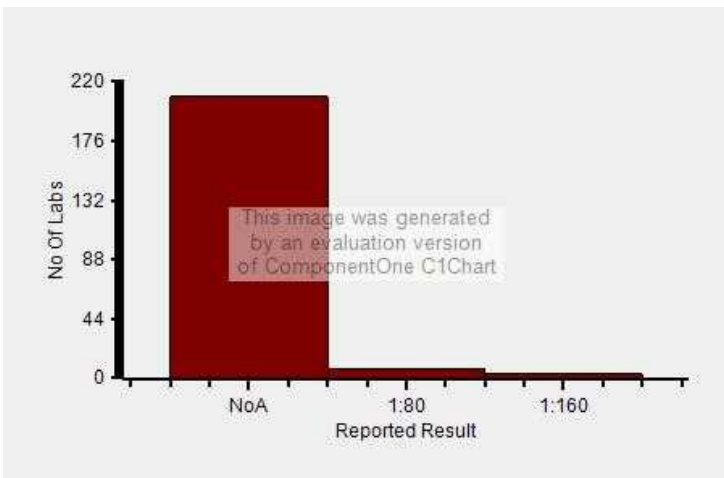

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Cycle No : 230310

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01

Report Date : 19/12/2023

Sample Date : 25/11/2023


Immunoassay Extended, Widal test - Typhi H antigen (TH), -

	N
■ All Methods	238
■ Tube Agglutination - (Your Method)	51
■ Manual - (Your Analyzer)	238

Evaluation Based On - Method wise Peer Grouping	
Your Result	1:80
Result Expected	1:80,NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

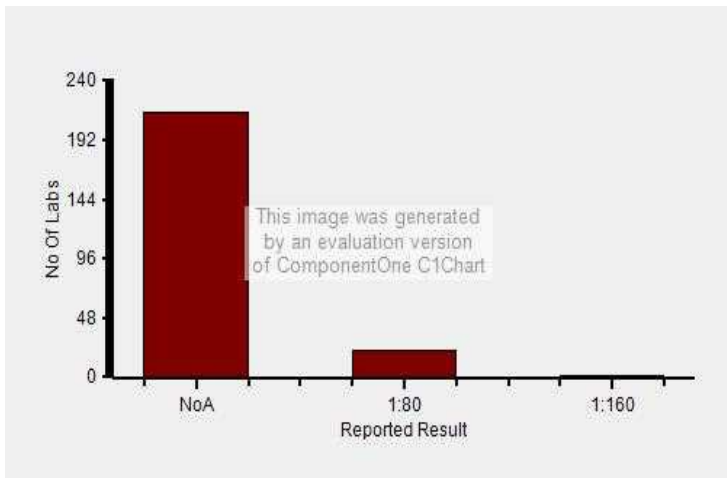

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

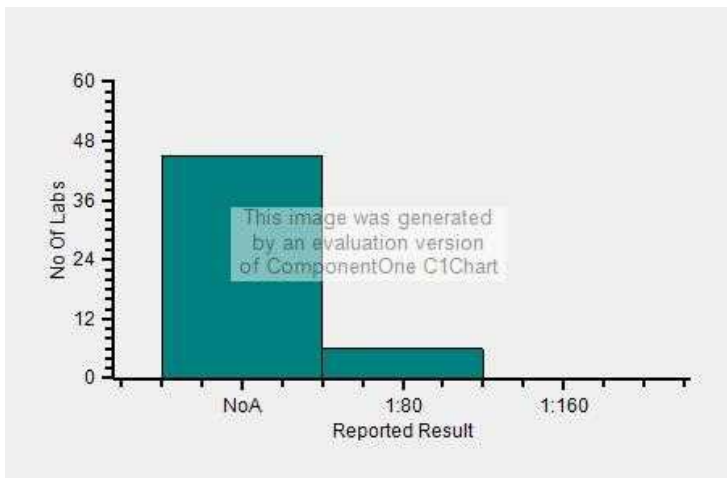

Frequency Histogram Your Analyzer

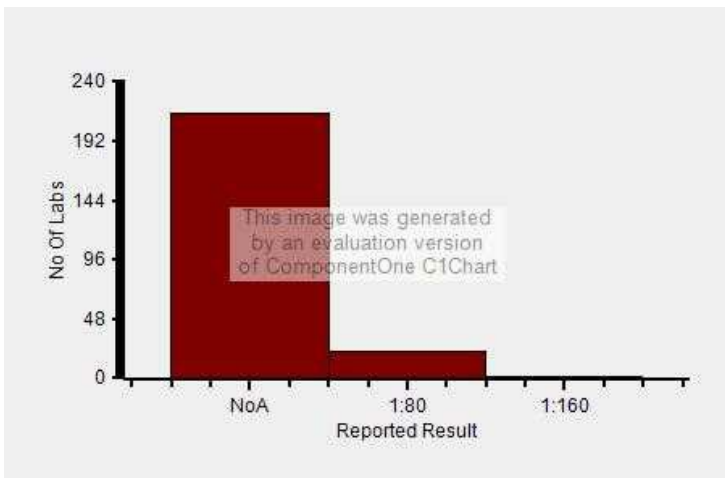

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Cycle No : 230310

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 01

Report Date : 19/12/2023

Sample Date : 25/11/2023


Immunoassay Extended, Widal test - Typhi O antigen (TO), -

	N
■ All Methods	238
■ Tube Agglutination - (Your Method)	51
■ Manual - (Your Analyzer)	238

Evaluation Based On - Method wise Peer Grouping	
Your Result	1:80
Result Expected	1:80,NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

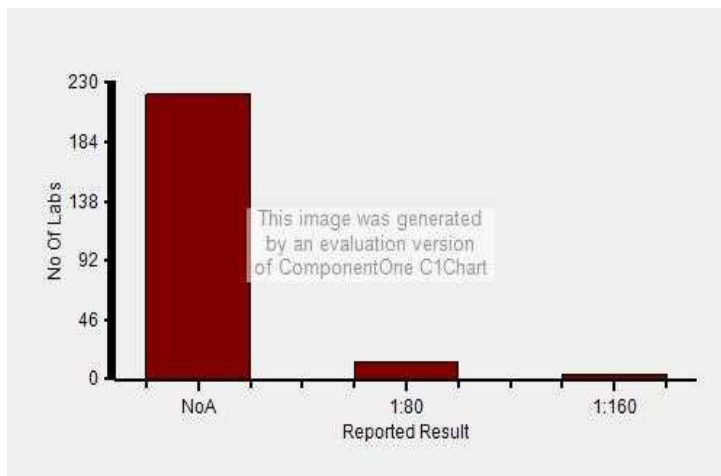

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 01

Sample Date : 25/11/2023

Frequency Histogram Your Method

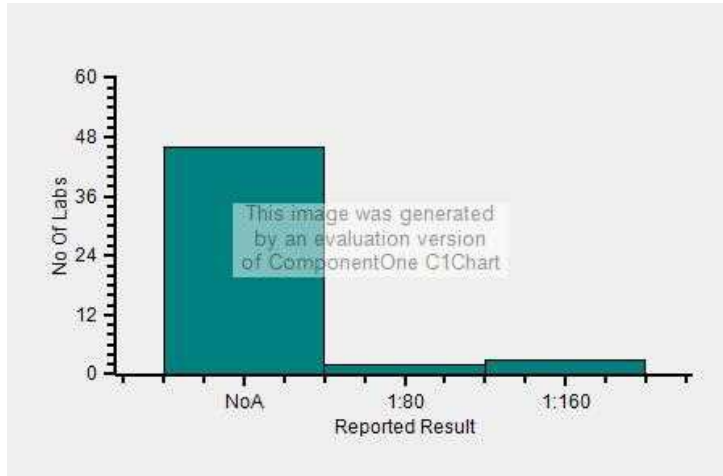

Frequency Histogram Your Analyzer

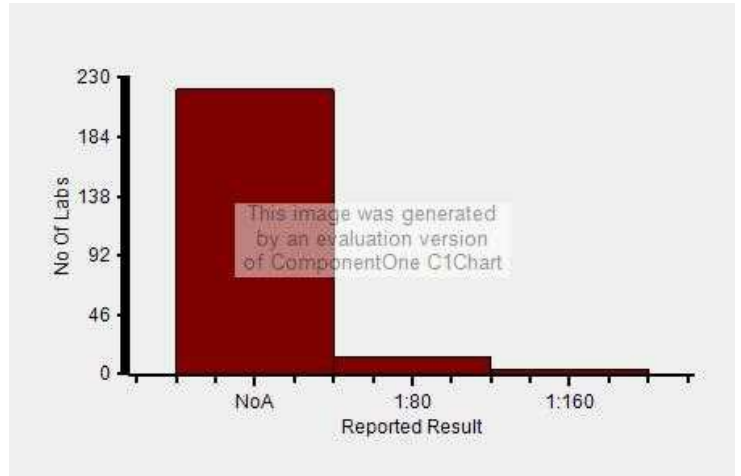

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416.
Commercial Building - 1A
Kohinoor Mall, Kirool Road, Kurla (W),
Mumbai - 400070

This is a computer generated report hence signature is not required



PC-1022

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023

Immunoassay Extended, Dengue IgG, -

■ All Methods

■ Immunochromatography - (Your Method)


■ Manual - (Your Analyzer)

N
 100
 86
 93

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

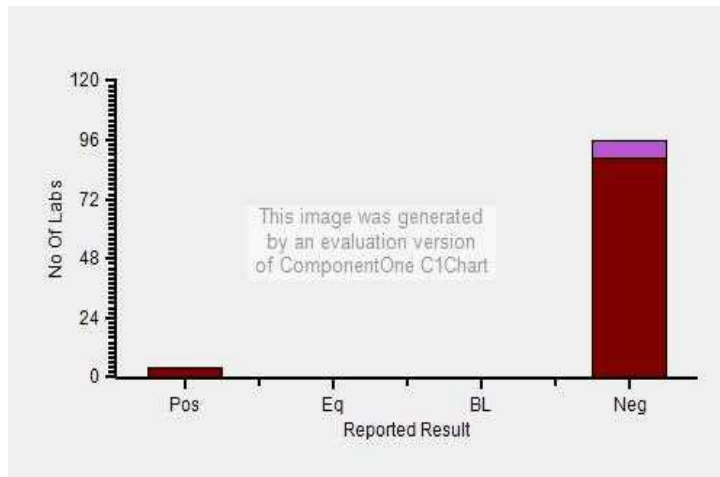

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 02


Report Date : 19/12/2023

Sample Date : 07/10/2023

Frequency Histogram Your Method

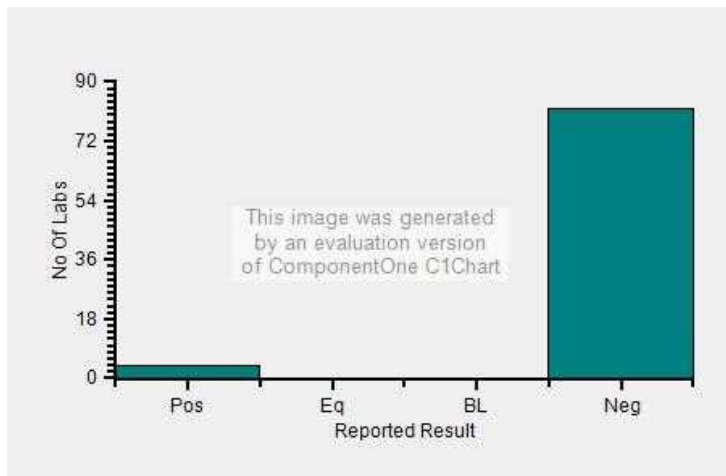

Frequency Histogram Your Analyzer

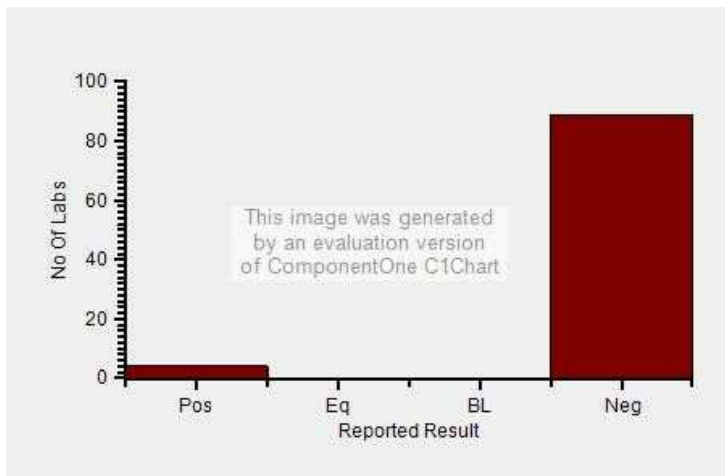

Reported Results Legends :-

- Pos** : Positive
- Eq** : Equivocal
- BL** : Borderline
- Neg** : Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023


Immunoassay Extended, Dengue IgM, -

	N
■ All Methods	100
■ Immunochromatography - (Your Method)	86
■ Manual - (Your Analyzer)	93

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

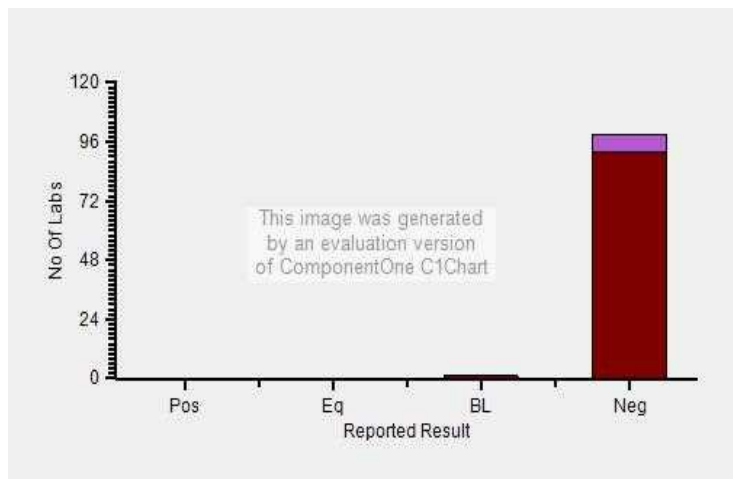

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 02

Sample Date : 07/10/2023

Frequency Histogram Your Method

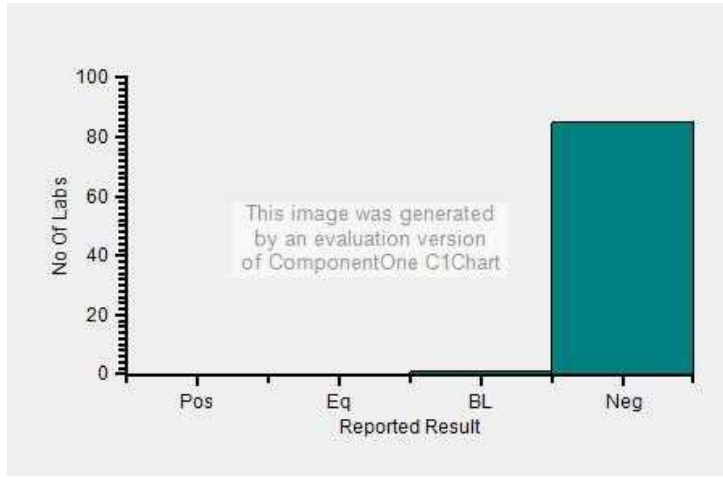

Frequency Histogram Your Analyzer

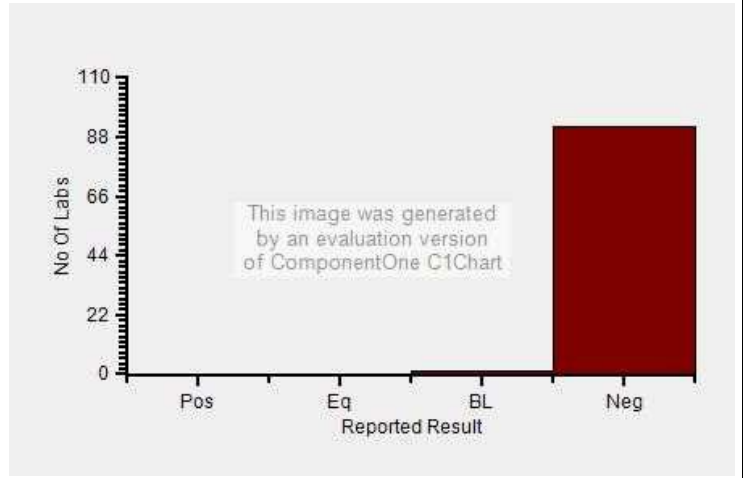

Reported Results Legends :-

Pos	: Positive
Eq	: Equivocal
BL	: Borderline
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023


Immunoassay Extended, Dengue NS 1, -

	N
■ All Methods	207
■ Immunochromatography - (Your Method)	183
■ Manual - (Your Analyzer)	195

Your Result	Negative
Result Expected	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

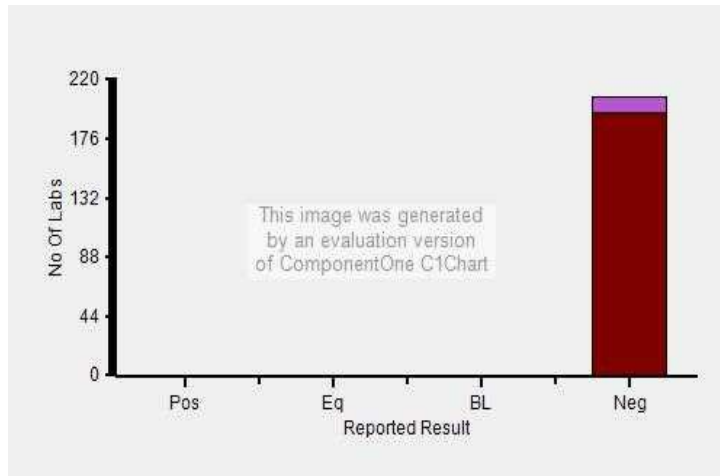

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 02

Sample Date : 07/10/2023

Frequency Histogram Your Method

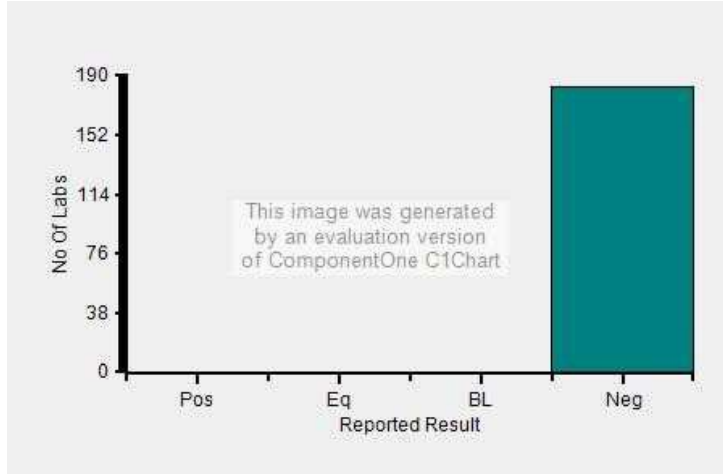

Frequency Histogram Your Analyzer

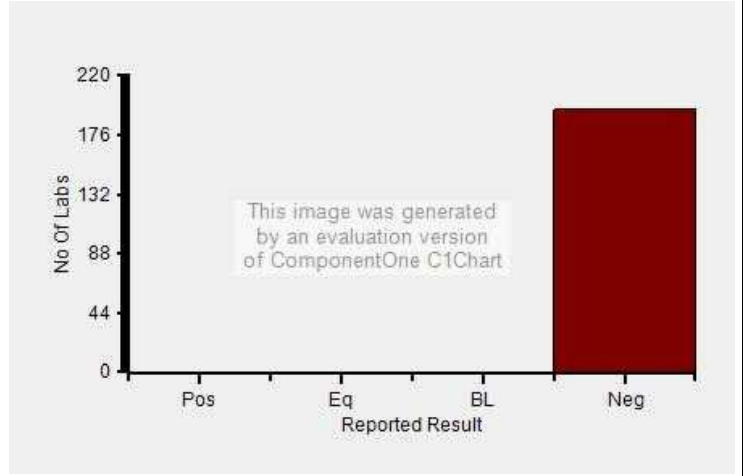

Reported Results Legends :-

Pos	: Positive
Eq	: Equivocal
BL	: Borderline
Neg	: Negative

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023


Immunoassay Extended, HBsAg, -

	N
■ All Methods	285
■ Immunochromatography - (Your Method)	205
■ J Mitra - (Your Analyzer)	33

Your Result	Reactive
Result Expected	R

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

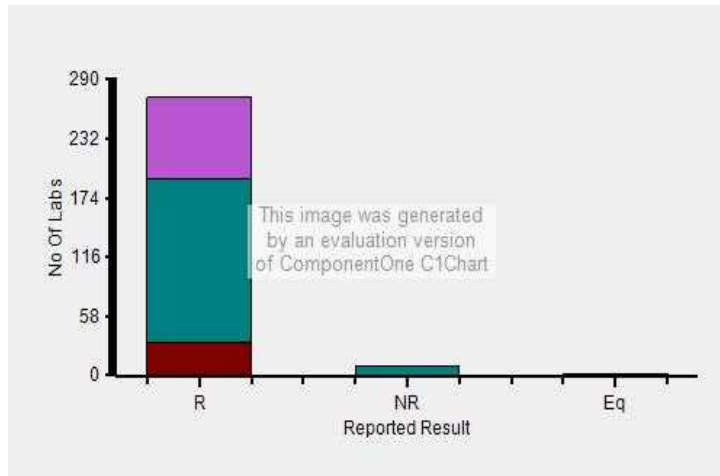

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 02


Report Date : 19/12/2023

Sample Date : 07/10/2023

Frequency Histogram Your Method

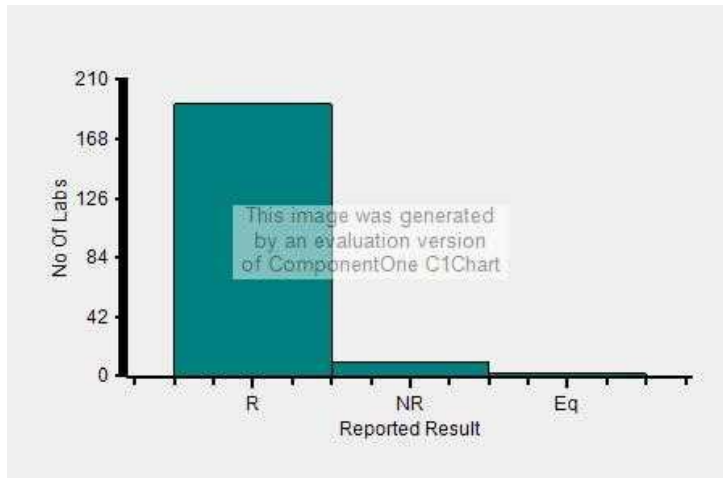

Frequency Histogram Your Analyzer

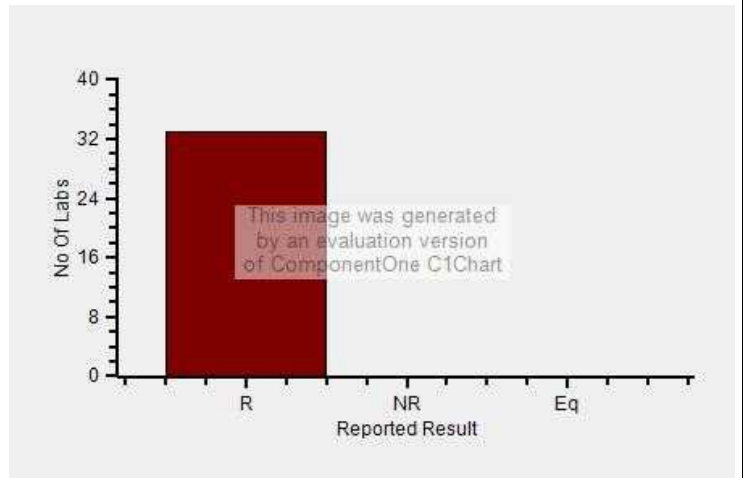

Reported Results Legends :-

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023


Immunoassay Extended, HCV, Nil

	N
■ All Methods	263
■ Immunofiltration - (Your Method)	31
■ J Mitra - (Your Analyzer)	35

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

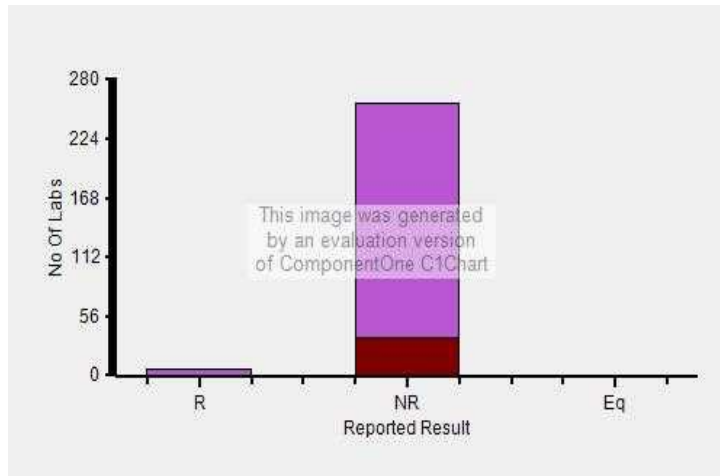

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 02

Sample Date : 07/10/2023

Frequency Histogram Your Method

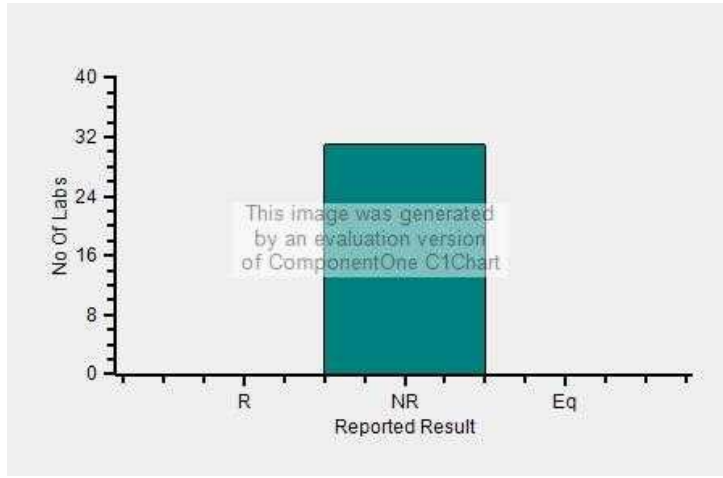

Frequency Histogram Your Analyzer

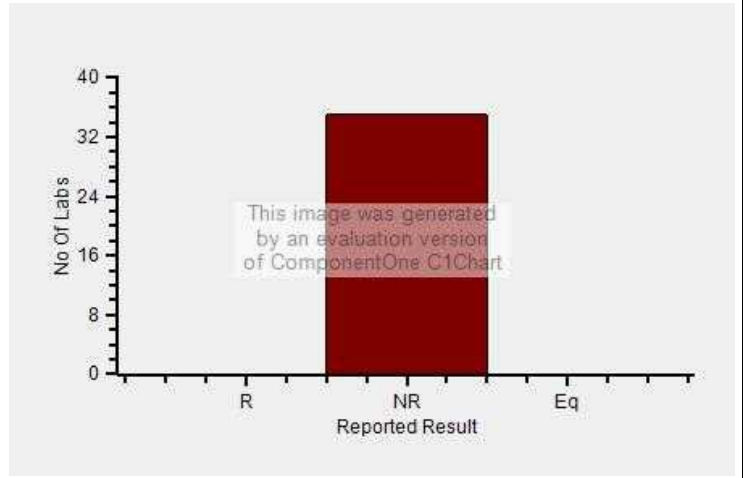

Reported Results Legends :-

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023


Immunoassay Extended, HIV Ab, S/CO

	N
■ All Methods	182
■ Immunofiltration - (Your Method)	32
■ J Mitra - (Your Analyzer)	34

Your Result	HIV-1 Ab Reactive
Result Expected	HIV-1

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

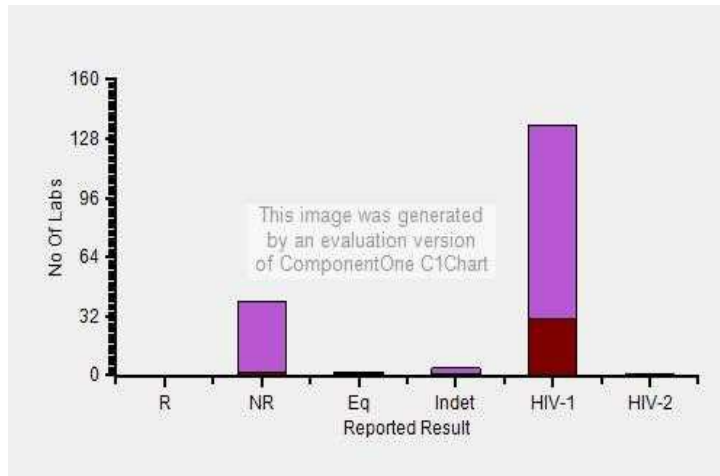

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 02


Report Date : 19/12/2023

Sample Date : 07/10/2023

Frequency Histogram Your Method

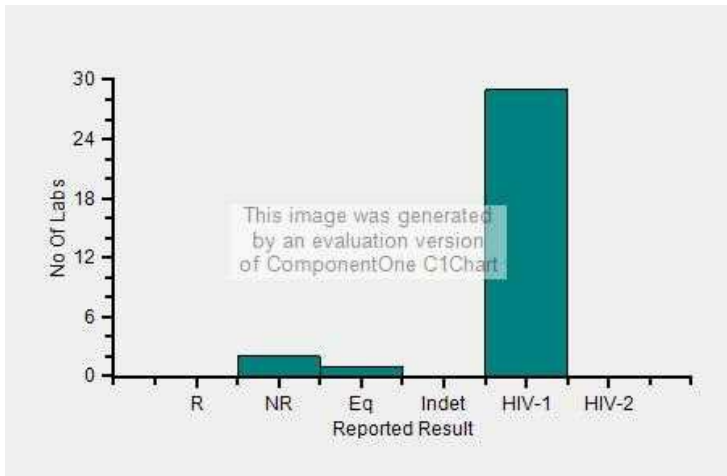

Frequency Histogram Your Analyzer

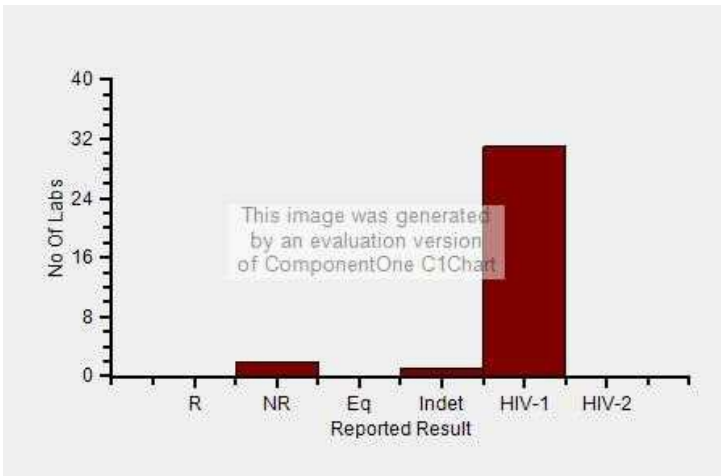

Reported Results Legends :-

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal
- Indet** : Indeterminate
- HIV-1** : HIV-1 Ab Reactive
- HIV-2** : HIV-2 Ab Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023


Immunoassay Extended, RPR (Syphilis Serology), -

	N
■ All Methods	235
■ Immunochromatography - (Your Method)	92
■ Manual - (Your Analyzer)	235

Your Result	Non-reactive
Result Expected	NR

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

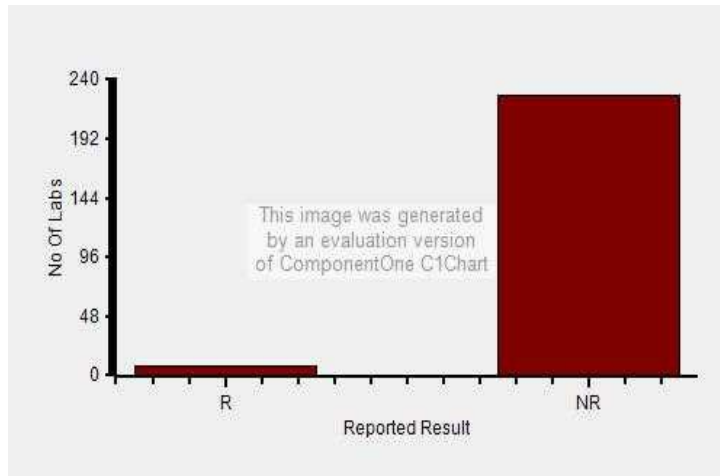

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 02

Sample Date : 07/10/2023

Frequency Histogram Your Method

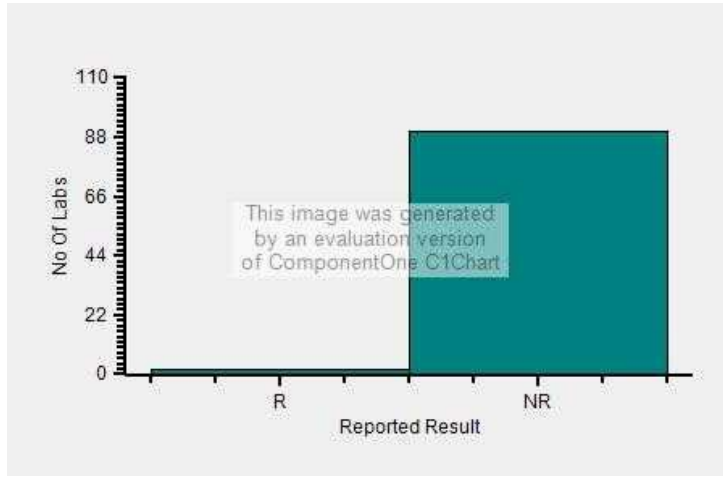

Frequency Histogram Your Analyzer

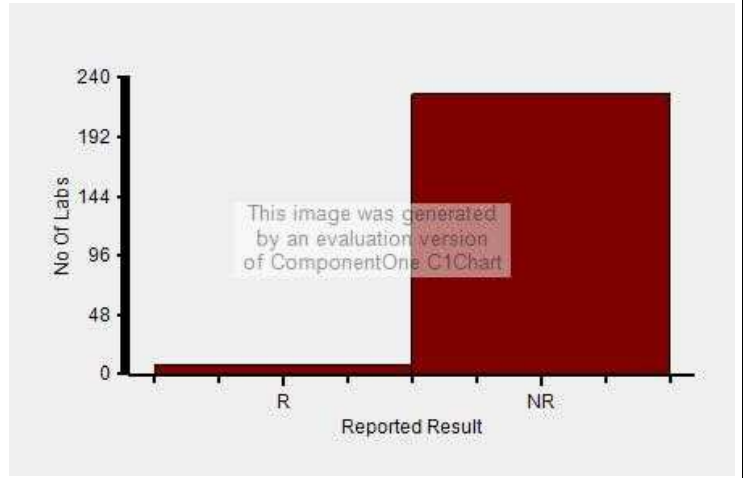

Reported Results Legends :-

R : Reactive

NR : Non-reactive

WR : Weak Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023

Immunoassay Extended, Widal test - ParaTyphi A-H antigen (AH), -

	N
■ All Methods	218
■ Tube Agglutination - (Your Method)	48
■ Manual - (Your Analyzer)	218


Evaluation Based On - Method wise Peer Grouping

Your Result No Agglutination

Result Expected 1:80,NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

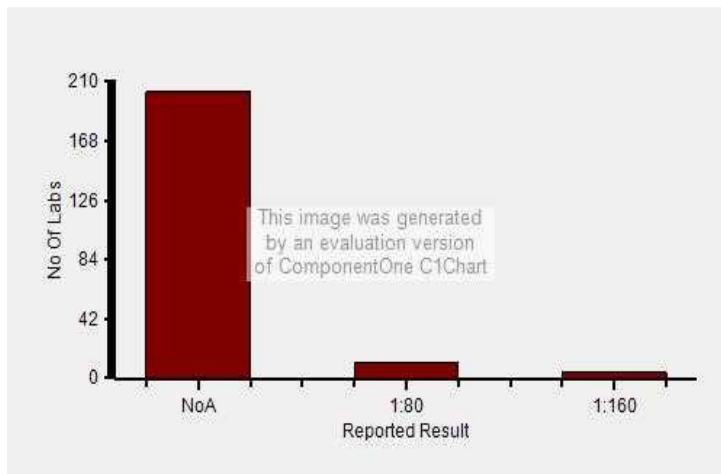

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 02


Report Date : 19/12/2023

Sample Date : 07/10/2023

Frequency Histogram Your Method

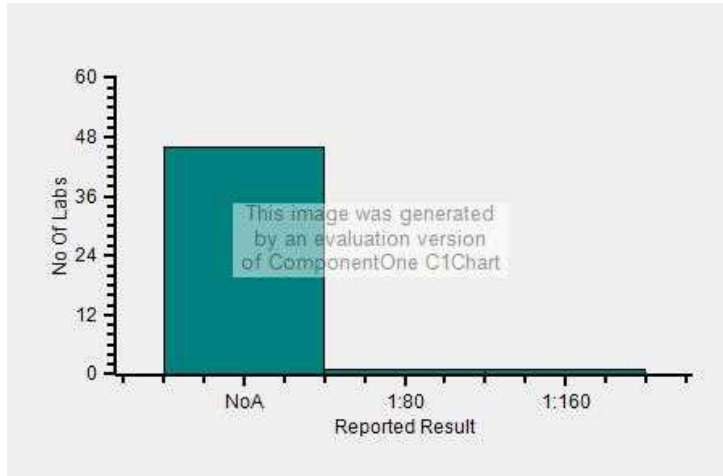

Frequency Histogram Your Analyzer

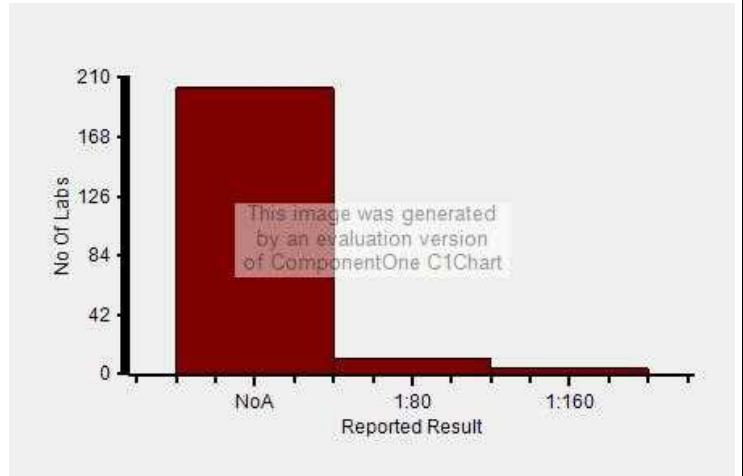

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023

Immunoassay Extended, Widal test - ParaTyphi B-H antigen (BH), -

	N
■ All Methods	218
■ Tube Agglutination - (Your Method)	48
■ Manual - (Your Analyzer)	218


Evaluation Based On - Method wise Peer Grouping

Your Result No Agglutination

Result Expected 1:80, NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

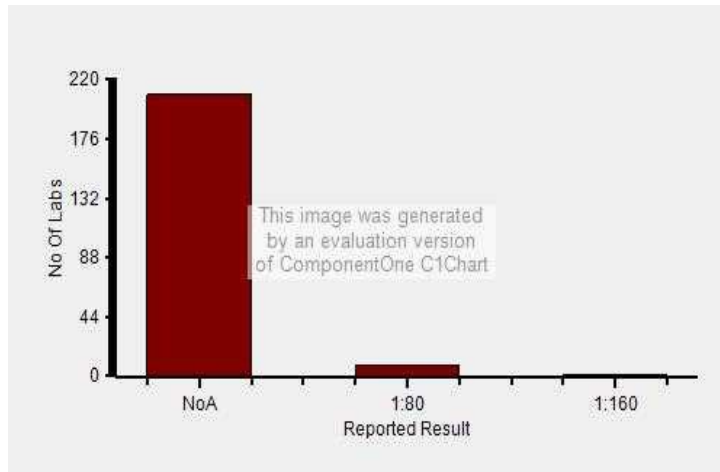

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 02

Sample Date : 07/10/2023

Frequency Histogram Your Method

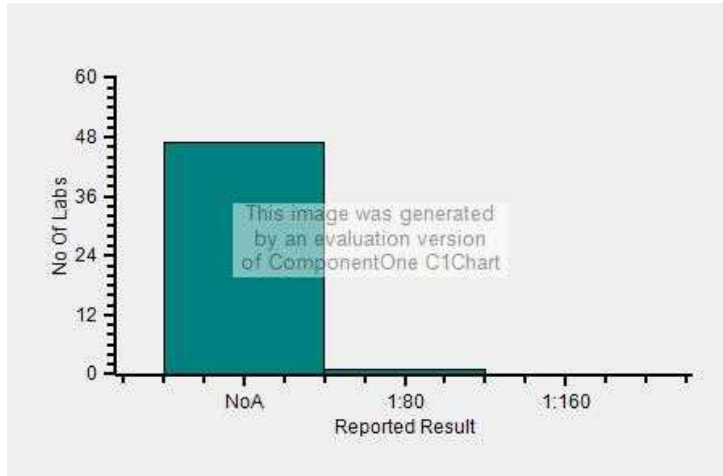

Frequency Histogram Your Analyzer

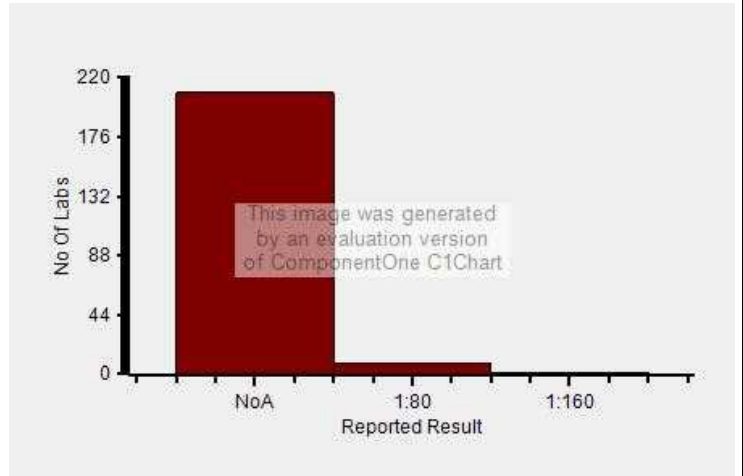

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023


Immunoassay Extended, Widal test - Typhi H antigen (TH), -

	N
■ All Methods	237
■ Tube Agglutination - (Your Method)	50
■ Manual - (Your Analyzer)	237

Evaluation Based On - Method wise Peer Grouping	
Your Result	1:80
Result Expected	1:80,NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

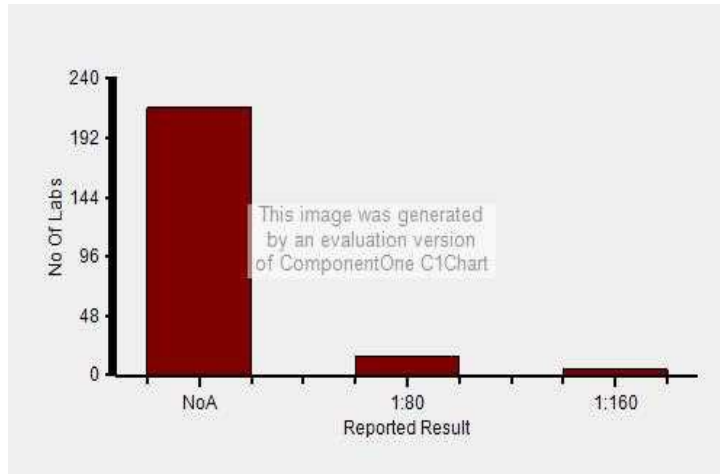

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 02


Report Date : 19/12/2023

Sample Date : 07/10/2023

Frequency Histogram Your Method

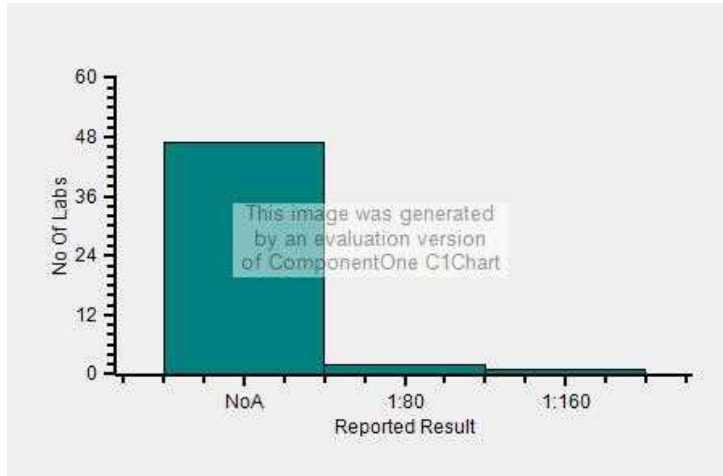

Frequency Histogram Your Analyzer

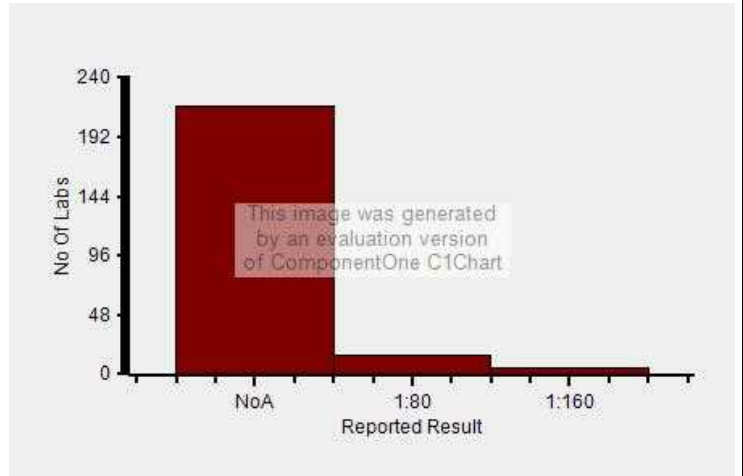

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 02

Sample Date : 07/10/2023


Immunoassay Extended, Widal test - Typhi O antigen (TO), -

	N
■ All Methods	237
■ Tube Agglutination - (Your Method)	50
■ Manual - (Your Analyzer)	237

Evaluation Based On - Method wise Peer Grouping	
Your Result	1:80
Result Expected	1:80,NoA

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

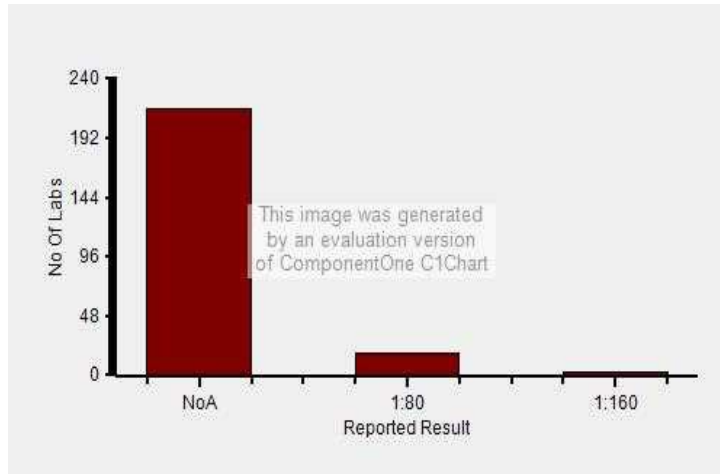

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 02

Sample Date : 07/10/2023

Frequency Histogram Your Method

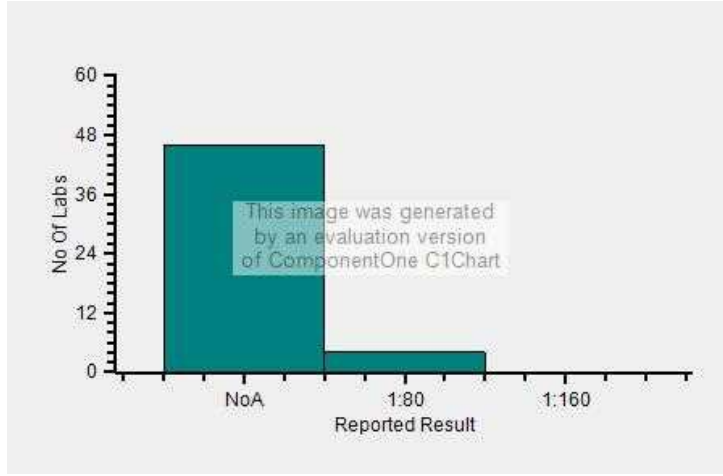

Frequency Histogram Your Analyzer

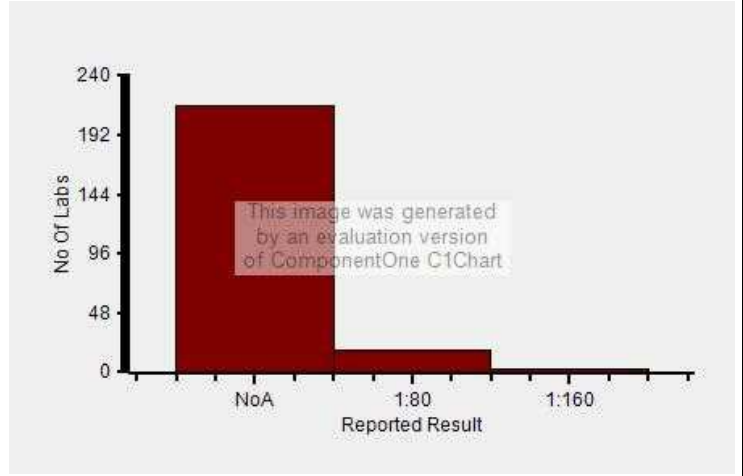

Reported Results Legends :-

NoA	: No Agglutination
1:80	: 1:80
1:160	: 1:160
1:320	: 1:320
1:640	: 1:640
>1:640	: >1:640

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416.
Commercial Building - 1A
Kohinoor Mall, Kirool Road, Kurla (W),
Mumbai - 400070

This is a computer generated report hence signature is not required



PC-1022

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 03

Sample Date : 07/10/2023


Immunoassay Extended, HBsAg, -

	N
■ All Methods	277
■ Immunochromatography - (Your Method)	200
■ J Mitra - (Your Analyzer)	34

Your Result	Reactive
Result Expected	R

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

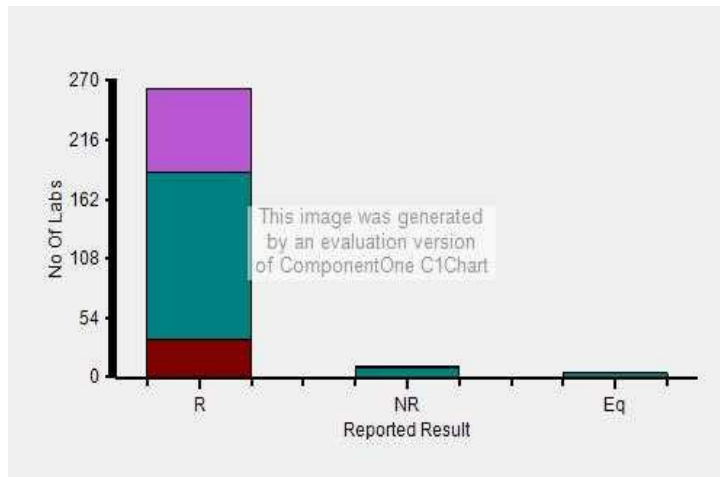

Lab : 1034

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 03


Report Date : 19/12/2023

Sample Date : 07/10/2023

Frequency Histogram Your Method

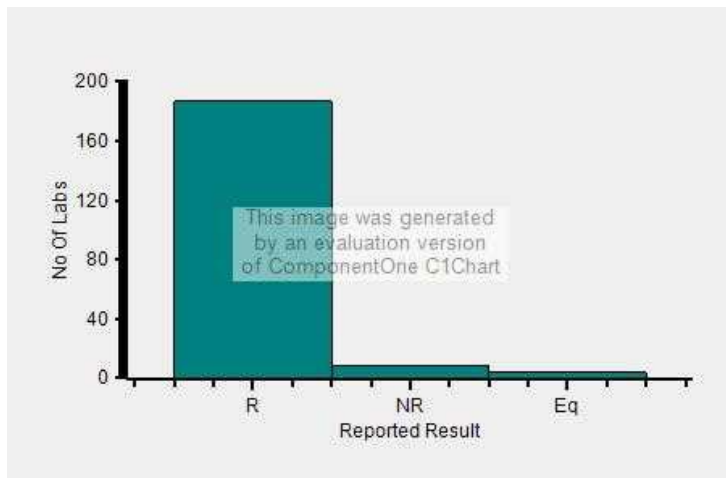

Frequency Histogram Your Analyzer

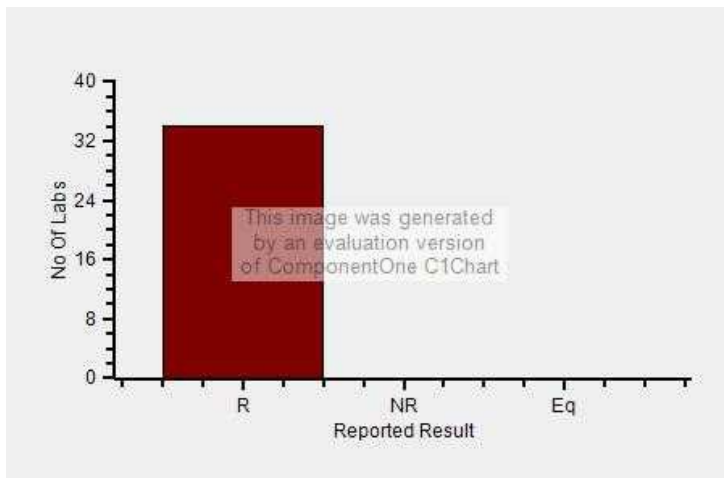

Reported Results Legends :-

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 03

Sample Date : 07/10/2023


Immunoassay Extended, HCV, Nil

	N
■ All Methods	254
■ Immunofiltration - (Your Method)	31
■ J Mitra - (Your Analyzer)	34

Your Result	Reactive
Result Expected	R

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

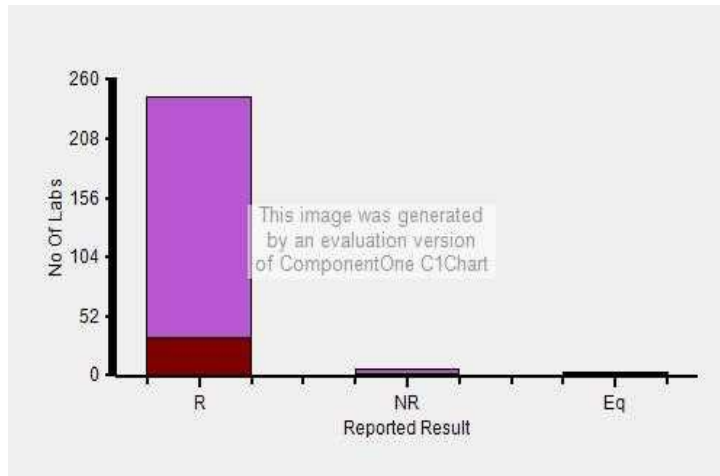

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 03

Sample Date : 07/10/2023

Frequency Histogram Your Method

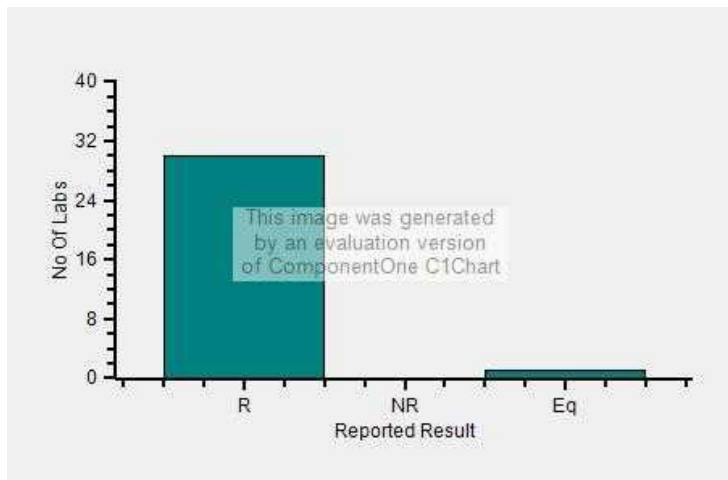

Frequency Histogram Your Analyzer

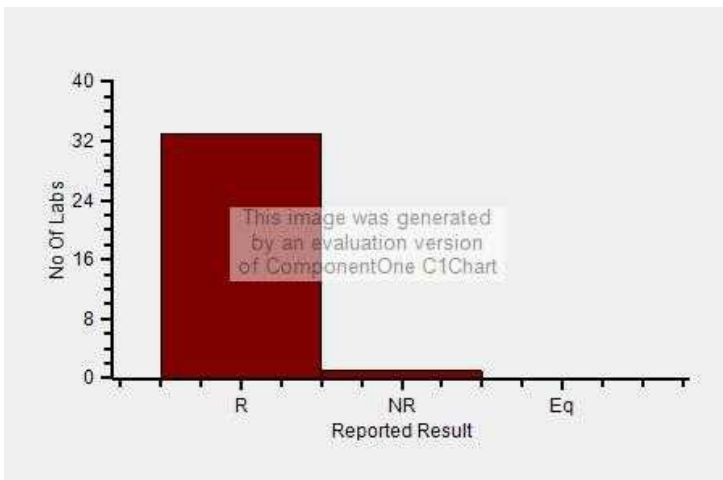

Reported Results Legends :-

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error



Lab : 1034

Cycle No : 230310

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA

Sample No : 03

Report Date : 19/12/2023

Sample Date : 07/10/2023


Immunoassay Extended, HIV Ab, S/CO

	N
■ All Methods	177
■ Immunofiltration - (Your Method)	32
■ J Mitra - (Your Analyzer)	34

Your Result	HIV-1 Ab Reactive
Result Expected	HIV-1

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

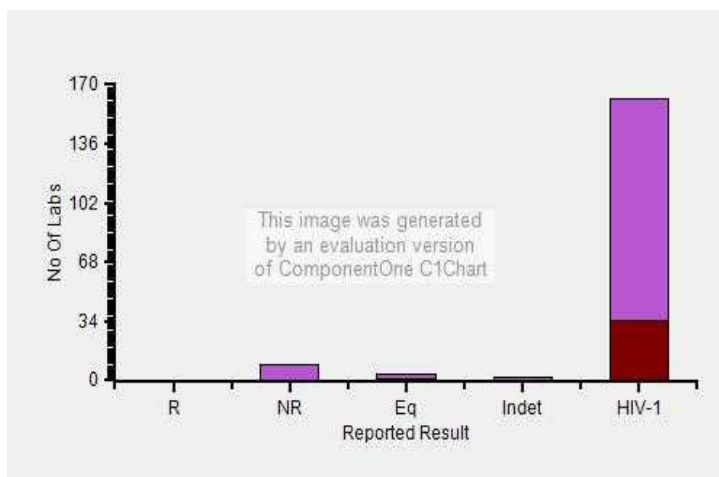

Lab : 1034

Lab Name : KRSNAA DIAGNOSTICS LTD, BATALA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 03

Sample Date : 07/10/2023

Frequency Histogram Your Method

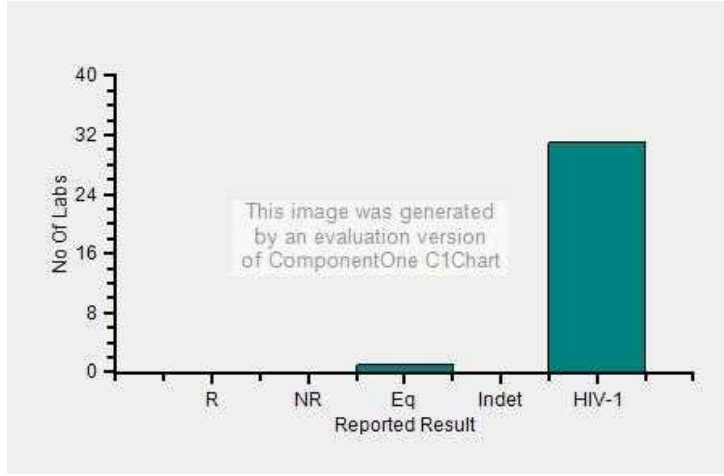

Frequency Histogram Your Analyzer

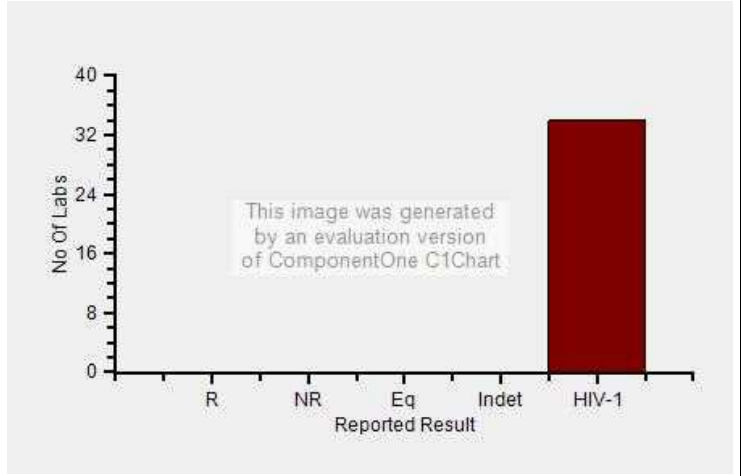

Reported Results Legends :-

- R** : Reactive
- NR** : Non-reactive
- Eq** : Equivocal
- Indet** : Indeterminate
- HIV-1** : HIV-1 Ab Reactive
- HIV-2** : HIV-2 Ab Reactive

Comments :

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
 - Two out of two pass - Acceptable performance
 - One out of two pass - Review for random error & take action if appropriate
 - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
 - All pass - Acceptable performance
 - Two out of three pass - Review for random error & take action if appropriate
 - One out of three pass - Unacceptable performance, Review for systematic error
 - All failed - Unacceptable performance, Review for systematic error

Dr Puneet Kumar Nigam

Dr Puneet Kumar Nigam
PT coordinator & Technical Manager, MHL EQAS
Unit No. 409-416.
Commercial Building - 1A
Kohinoor Mall, Kirool Road, Kurla (W),
Mumbai - 400070

This is a computer generated report hence signature is not required



PC-1022