


Calibration Trace

No.	Test Name	Calibration Type	S1Abs.	K	A	B	C	Test Date	Calibration N...
1	GLU3	2 point linear	0.0258	315.5700	0.0000	0.0000	0.0000	18-01-2024 17:46:46	RANDOX CAL 3
2	GLU3	2 point linear	0.0198	648.5353	0.0000	0.0000	0.0000	26-11-2023 10:39:14	RANDOX CAL 3
3	GLU3	2 point linear	0.0153	307.6694	0.0000	0.0000	0.0000	21-10-2023 11:58:20	RANDOX CAL 3
4	GLU3	2 point linear	0.0152	449.7544	0.0000	0.0000	0.0000	21-10-2023 11:36:09	RANDOX CAL 3
5	GLU3	2 point linear	0.0998	349.6764	0.0000	0.0000	0.0000	25-08-2023 12:07:25	RANDOX
6	GLU3	2 point linear	0.0968	12024.1...	0.0000	0.0000	0.0000	22-08-2023 13:58:55	DIACAL
7	GLU3	2 point linear	0.0974	341.7502	0.0000	0.0000	0.0000	23-07-2023 12:20:45	RANDOX CAL 3
8	GLU3	2 point linear	0.0940	336.3579	0.0000	0.0000	0.0000	13-07-2023 12:04:48	RANDOX CAL 3
9	GLU3	2 point linear	0.0929	392.6432	0.0000	0.0000	0.0000	11-07-2023 11:10:32	RANDOX CAL 3
10	GLU3	2 point linear	0.0500	366.0912	0.0000	0.0000	0.0000	09-07-2023 12:12:03	RANDOX CAL 3
11	GLU3	2 point linear	0.0497	293.2622	0.0000	0.0000	0.0000	02-07-2023 10:48:09	RANDOX CAL 3
12	GLU3	2 point linear	0.0156	324.8884	0.0000	0.0000	0.0000	02-06-2023 14:44:43	RANDOX CAL 3
13	GLU3	2 point linear	0.0151	221.4808	0.0000	0.0000	0.0000	02-06-2023 11:47:44	RANDOX CAL 3




Standard	<0>	<1>	<2>	<3>	<4>	<5>	<6>	<7>	Apply Trace
Concentration	0.0	278.0							Reaction Curve
Abs.	0.0258	0.9067							Return



Calibration Trace


No.	Test Name	Calibration Type	S1Abs.	K	A	B	C	Test Date	Calibration N...
1	CHO1	2 point linear	0.0507	591.4980	0.0000	0.0000	0.0000	18-01-2024 17:48:46	RANDOX CAL 3
2	CHO1	2 point linear	0.0502	559.3574	0.0000	0.0000	0.0000	12-12-2023 12:23:45	RANDOX CAL 3
3	CHO1	2 point linear	0.0487	586.7318	0.0000	0.0000	0.0000	26-11-2023 10:41:14	DIACAL
4	CHO1	2 point linear	0.0366	588.2068	0.0000	0.0000	0.0000	22-08-2023 14:00:55	DIACAL
5	CHO1	2 point linear	0.0427	590.8596	0.0000	0.0000	0.0000	23-07-2023 12:22:45	RANDOX CAL 3
6	CHO1	2 point linear	0.0425	585.9088	0.0000	0.0000	0.0000	13-07-2023 12:06:48	RANDOX CAL 3
7	CHO1	2 point linear	0.0418	679.1855	0.0000	0.0000	0.0000	11-07-2023 11:12:32	RANDOX CAL 3
8	CHO1	2 point linear	0.0409	668.4457	0.0000	0.0000	0.0000	09-07-2023 12:14:03	RANDOX CAL 3
9	CHO1	2 point linear	0.0421	533.7698	0.0000	0.0000	0.0000	02-07-2023 10:49:45	RANDOX CAL 3
10	CHO1	2 point linear	0.0271	631.1855	0.0000	0.0000	0.0000	02-06-2023 14:46:43	RANDOX CAL 3
11	CHO1	2 point linear	0.0275	423.1418	0.0000	0.0000	0.0000	02-06-2023 11:49:44	RANDOX CAL 3
12	CHO1	2 point linear	0.0422	525.5774	0.0000	0.0000	0.0000	30-05-2023 12:46:35	RANDOX CAL 3
13	CHO1	2 point linear	0.0276	561.8343	0.0000	0.0000	0.0000	03-05-2023 11:34:47	RANDOX CAL 3

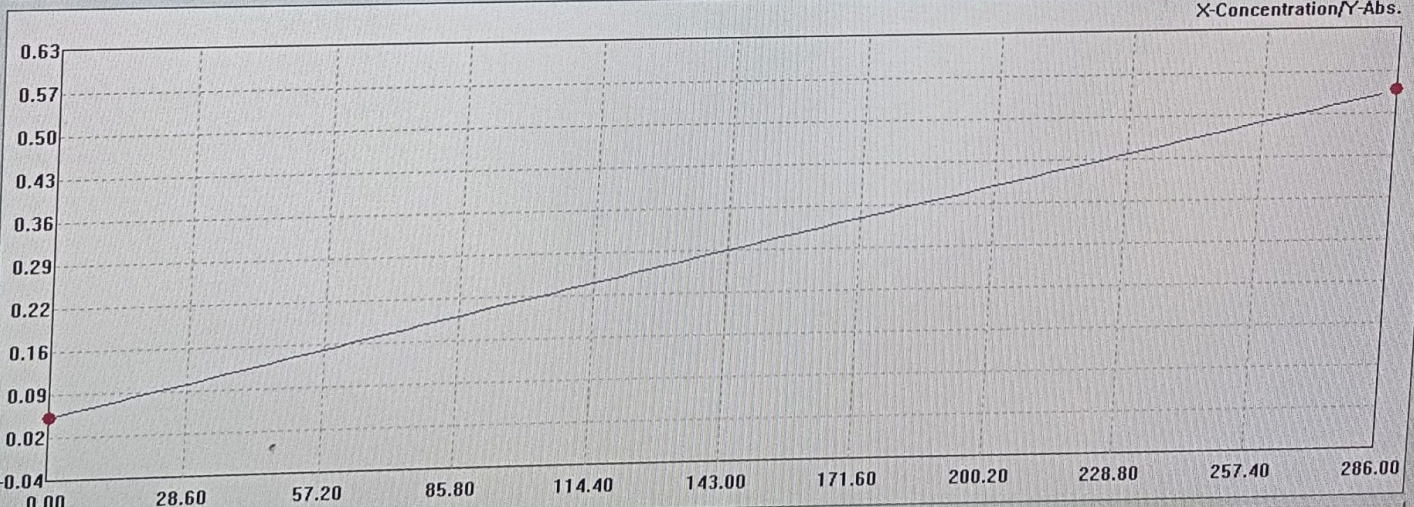

Standard	<0>	<1>	<2>	<3>	<4>	<5>	<6>	<7>	Apply Trace
Concentration	0.00	286.00							Reaction Curve
Abs.	0.0507	0.5342							Return


Calibration Trace

No.	Test Name	Calibration Type	S1Abs.	K	A	B	C	Test Date	Calibration N...
1	AST1	2 point linear	-0.0006	-2478.9...	0.0000	0.0000	0.0000	18-01-2024 17:51:34	RANDOX CAL 3
2	AST1	2 point linear	-0.0009	-2388.1...	0.0000	0.0000	0.0000	12-12-2023 12:24:57	RANDOX CAL 3
3	AST1	2 point linear	-0.0004	-2135.0...	0.0000	0.0000	0.0000	30-11-2023 12:19:52	DIA CAL
4	AST1	2 point linear	-0.0002	-1778.1...	0.0000	0.0000	0.0000	30-11-2023 11:36:14	DIA CAL
5	AST1	2 point linear	-0.0003	-2206.5...	0.0000	0.0000	0.0000	26-11-2023 10:43:38	DIA CAL
6	AST1	2 point linear	-0.0002	-2550.7...	0.0000	0.0000	0.0000	21-10-2023 11:58:44	DIA CAL
7	AST1	2 point linear	-0.0005	-3474.2...	0.0000	0.0000	0.0000	21-10-2023 11:36:57	RANDOX CAL 3
8	AST1	2 point linear	-0.0003	-3511.8...	0.0000	0.0000	0.0000	11-10-2023 12:22:10	RANDOX CAL 3
9	AST1	2 point linear	-0.0003	-3586.3...	0.0000	0.0000	0.0000	10-10-2023 13:13:06	RANDOX CAL 3
10	AST1	2 point linear	-0.0004	-3339.8...	0.0000	0.0000	0.0000	08-10-2023 12:19:05	RANDOX CAL 3
11	AST1	2 point linear	-0.0010	-3777.7...	0.0000	0.0000	0.0000	03-10-2023 10:54:11	RANDOX CAL 3
12	AST1	2 point linear	-0.0004	-698.2219	0.0000	0.0000	0.0000	22-08-2023 14:03:19	DIACAL
13	AST1	2 point linear	-0.0001	-7206.1...	0.0000	0.0000	0.0000	23-07-2023 12:25:00	RANDOX CAL 3

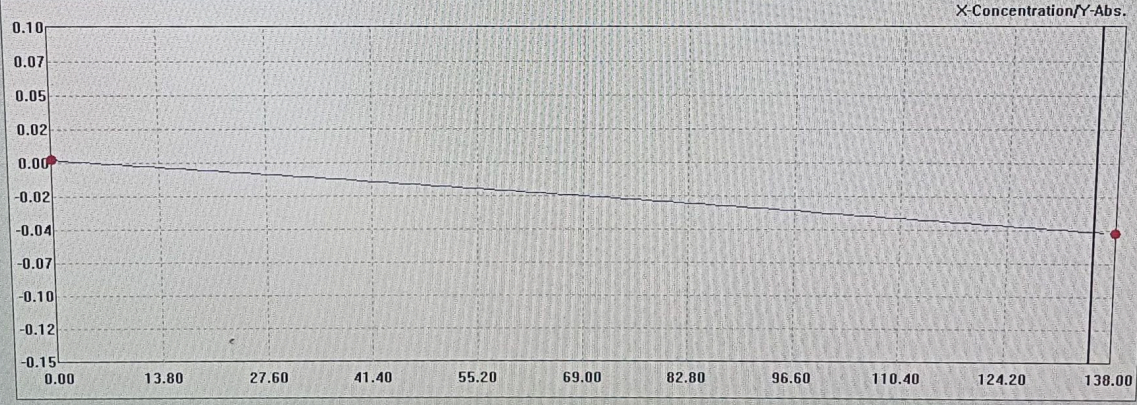

Standard	<0>	<1>	<2>	<3>	<4>	<5>	<6>	<7>	Apply Trace
Concentration	0.0	138.0							Reaction Curve
Abs.	-0.0006	-0.0563							Return

Calibration Trace

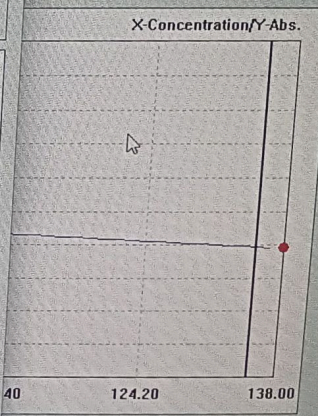

<6> <7>

Save

Calibration Trace

No.	Test Name	Calibration Type	S1Abs.	K	A	B	C	Test Date	Calibration N...
1	CREA-J1	2 point linear	0.0021	105.1728	0.0000	0.0000	0.0000	18-01-2024 17:47:10	RANDOX 3
2	CREA-J1	2 point linear	0.0021	105.0021	0.0000	0.0000	0.0000	14-01-2024 10:18:53	DIACAL
3	CREA-J1	2 point linear	0.0022	92.5935	0.0000	0.0000	0.0000	08-01-2024 17:06:56	DIACAL
4	CREA-J1	2 point linear	0.0031	155.7848	0.0000	0.0000	0.0000	08-01-2024 11:26:18	DIACAL
5	CREA-J1	2 point linear	0.0024	100.3913	0.0000	0.0000	0.0000	28-12-2023 14:57:24	DIACAL
6	CREA-J1	2 point linear	0.0022	104.2376	0.0000	0.0000	0.0000	30-11-2023 12:19:04	DIA CAL
7	CREA-J1	2 point linear	0.0024	106.0509	0.0000	0.0000	0.0000	30-11-2023 11:34:14	RANDOX CAL 3
8	CREA-J1	2 point linear	0.0028	103.6906	0.0000	0.0000	0.0000	27-11-2023 11:19:39	RANDOX CAL 3
9	CREA-J1	2 point linear	0.0024	156.2754	0.0000	0.0000	0.0000	26-11-2023 10:39:38	RANDOX CAL 3
10	CREA-J1	2 point linear	0.0026	112.4521	0.0000	0.0000	0.0000	15-11-2023 11:30:37	RANDOX CAL 3
11	CREA-J1	2 point linear	0.0029	151.4924	0.0000	0.0000	0.0000	14-11-2023 11:07:09	RANDOX CAL 3
12	CREA-J1	2 point linear	0.0028	97.6697	0.0000	0.0000	0.0000	03-11-2023 12:13:22	RANDOX CAL 3
13	CREA-J1	2 point linear	0.0028	102.1589	0.0000	0.0000	0.0000	11-10-2023 12:21:46	RANDOX CAL 3



Standard	<0>	<1>	<2>	<3>	<4>	<5>	<6>	<7>	Apply Trace
Concentration	0.00	4.22							Reaction Curve
Abs.	0.0021	0.0422							Return

C

Calibration Tr

X-Concentr

3.42

<6>

<7>

Save