

# Calibration Curve

Calibration Method: 2 Point Linear

Calibration Time: 20-01-2024 22:49:37


Test Item: GLU

Absorbance: 0.0561

Calibrator: 1

S1 Abs	K	A	B	C
0.0561	401.2739	0	0	0

Calibration	Concentration	Abs.	Calibration	Concentration	Abs.
1.	0	0.0561	6.	0	0
2.	189	0.5271	7.	0	0
3.	0	0	8.	0	0
4.	0	0	9.	0	0
5.	0	0	10.	0	0

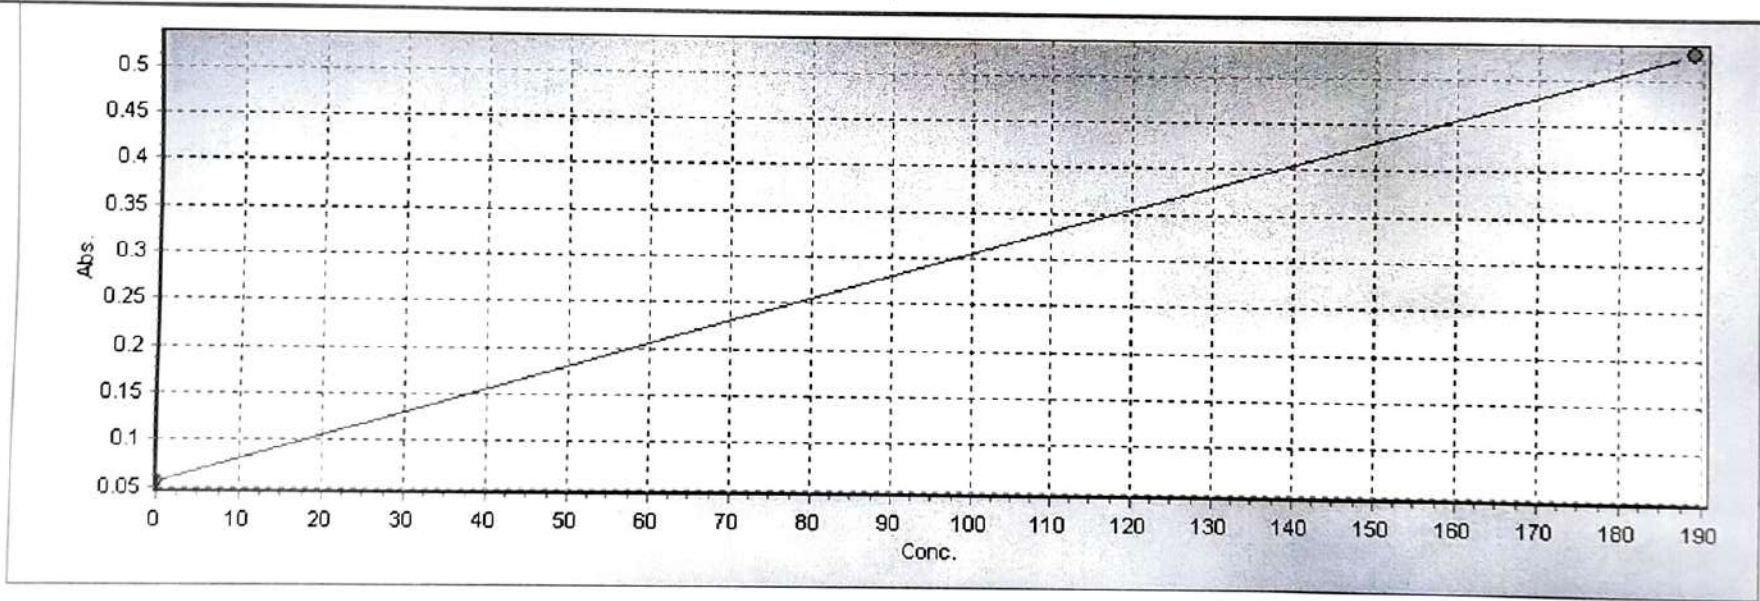

# Calibration Curve

Calibration Method: 2 Point Linear

Calibration Time: 16-02-2024 20:03:31


Test Item: CRE-E

Absorbance: 0.0012

Calibrator: 1

S1 Abs	K	A	B	C
0.0012	66.4921	0	0	0

Calibration	Concentration	Abs.	Calibration	Concentration	Abs.
1.	0	0.0012	6.	0	0
2.	3.81	0.0585	7.	0	0
3.	0	0	8.	0	0
4.	0	0	9.	0	0
5.	0	0	10.	0	0

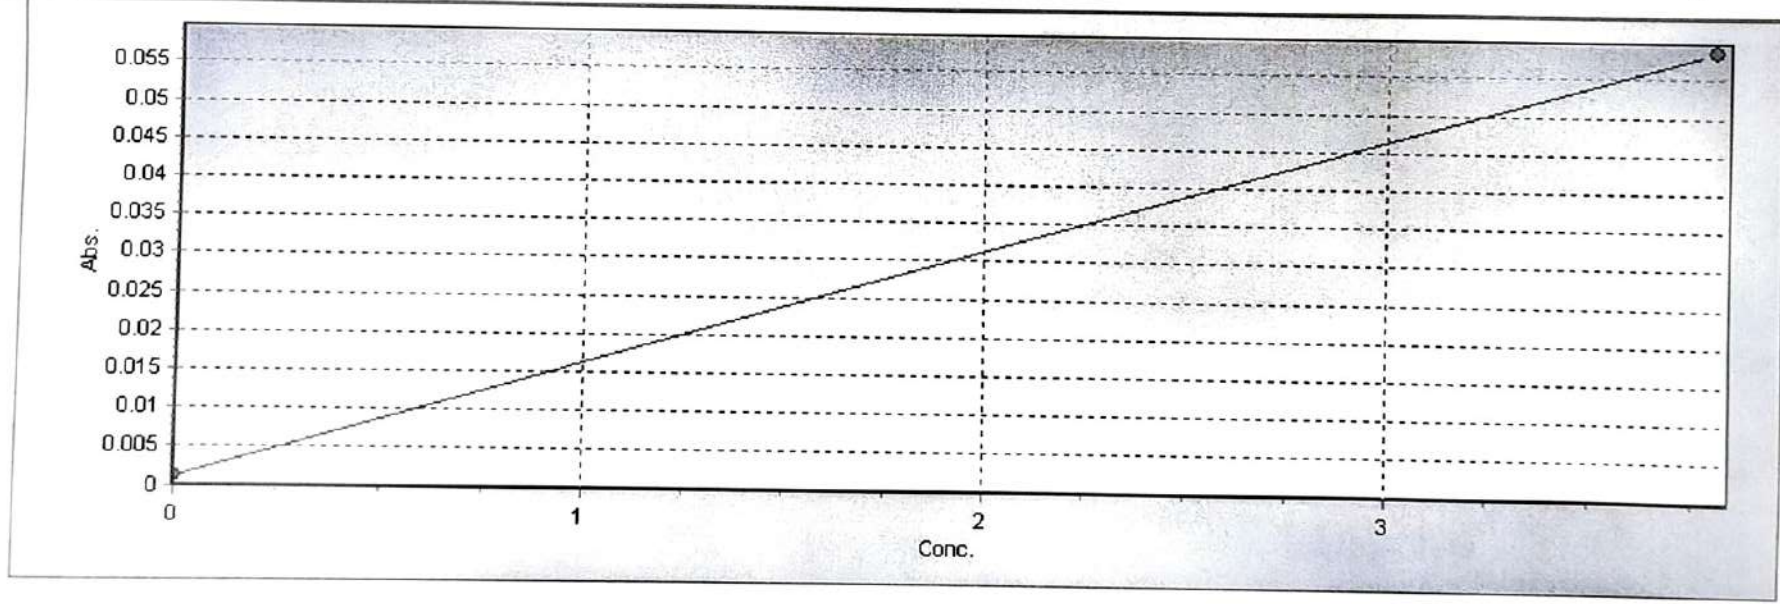

# Calibration Curve

Calibration Method: 2 Point Linear

Calibration Time: 20-01-2024 22:51:45


Test Item: TG

Absorbance: 0.088

Calibrator: 1

S1 Abs	K	A	B	C
0.088	839.895	0	0	0

Calibration	Concentration	Abs.	Calibration	Concentration	Abs.
1.	0	0.088	6.	0	0
2.	144	0.25945	7.	0	0
3.	0	0	8.	0	0
4.	0	0	9.	0	0
5.	0	0	10.	0	0

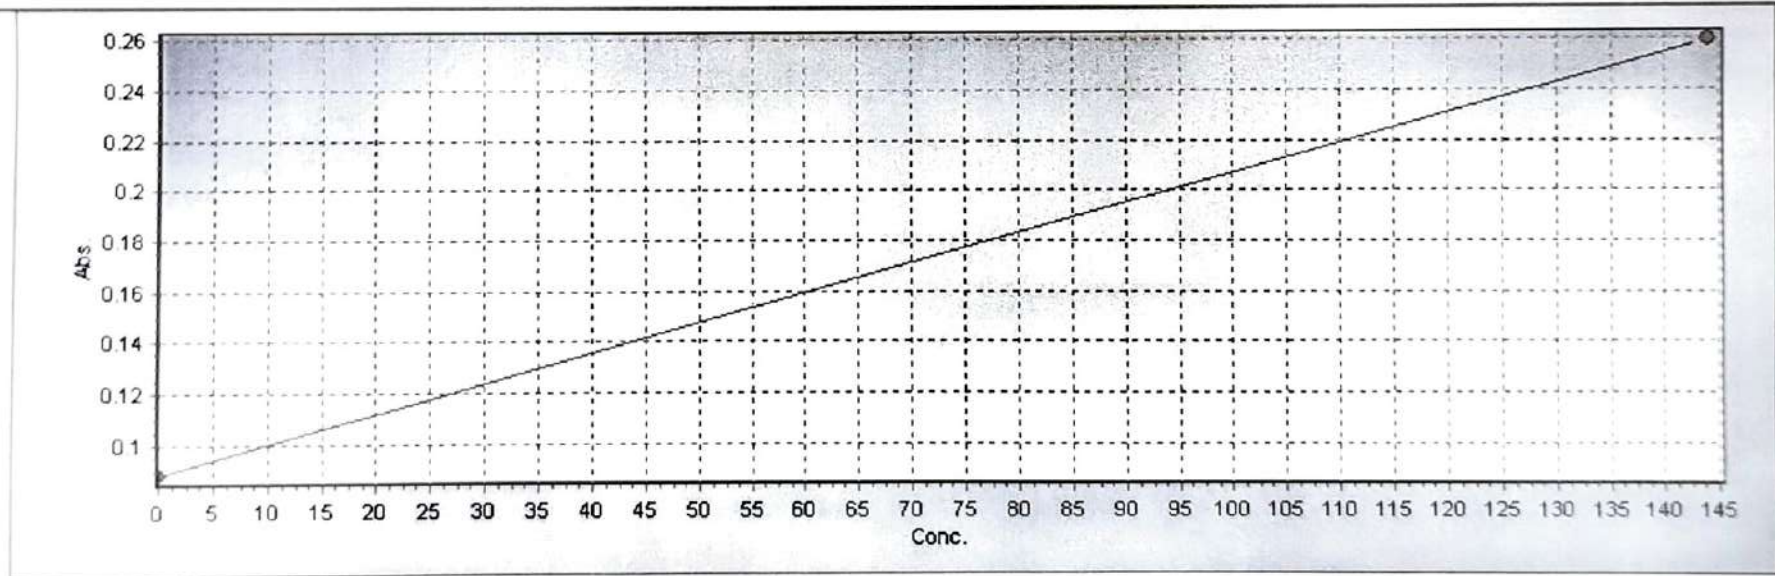

# Calibration Curve

Calibration Method: 2 Point Linear

Calibration Time: 20-01-2024 22:50:30


Test Item: TC

Absorbance: 0.02005

Calibrator: 1

S1 Abs	K	A	B	C
0.02005	674.6785	0	0	0

Calibration	Concentration	Abs.	Calibration	Concentration	Abs.
1.	0	0.02005	6.	0	0
2.	160	0.2572	7.	0	0
3.	0	0	8.	0	0
4.	0	0	9.	0	0
5.	0	0	10.	0	0

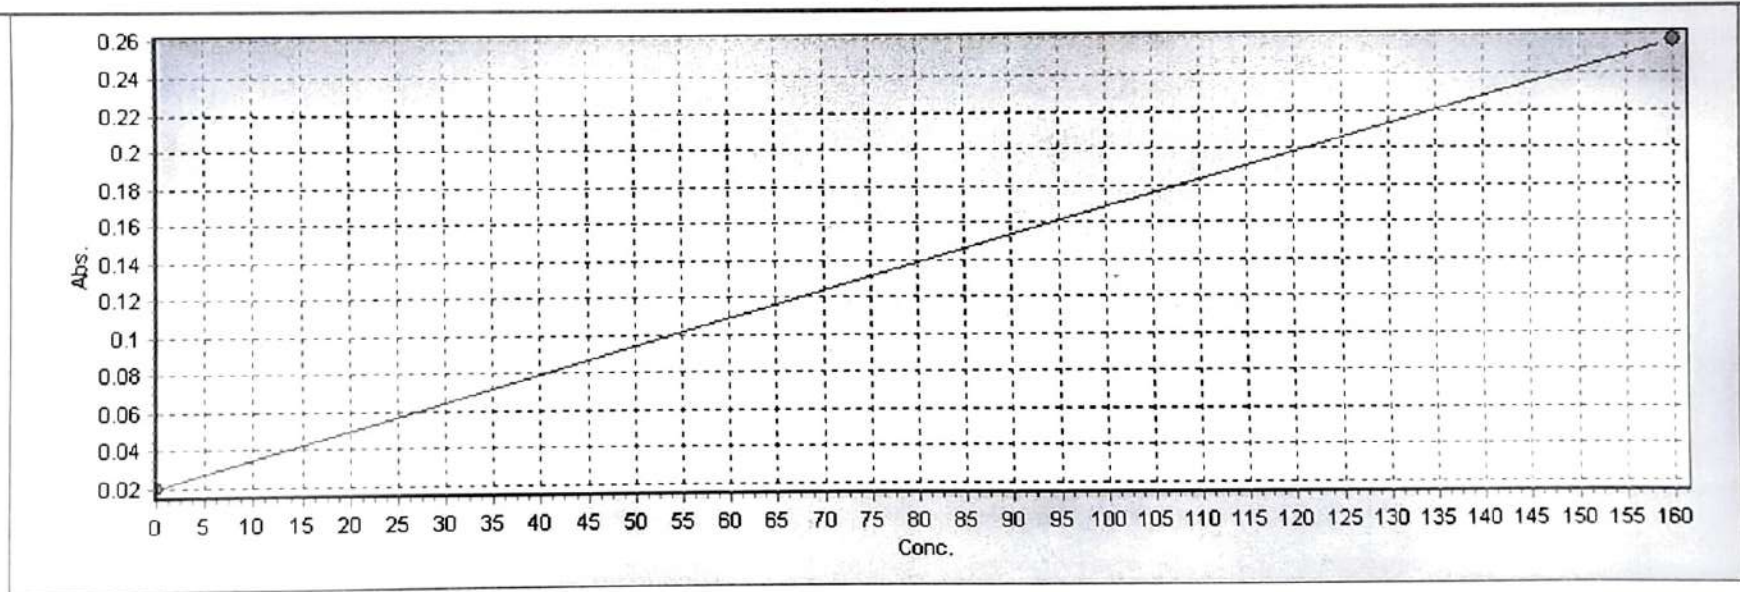

# Calibration Curve

Calibration Method: 2 Point Linear

Calibration Time: 24-02-2024 14:05:13

Test Item: ALB

Absorbance: 0.15455

Calibrator: 1

S1 Abs	K	A	B	C
0.15455	5.2708	0	0	0

Calibration	Concentration	Abs.	Calibration	Concentration	Abs.
1.	0	0.15455	6.	0	0
2.	3.64	0.84515	7.	0	0
3.	0	0	8.	0	0
4.	0	0	9.	0	0
5.	0	0	10.	0	0

