



# Metropolis Healthcare Ltd., EQAS

KRSNAA DIAGNOSTICS,LTD,MOGA (1054)

## Outlier And Analyte Summary Report

Outlier Details For Cycle No 230412 and Sample No 01

Report Date : 13/02/2024

Analyte	Instrument	Result Value	Standard Unit
No Outlier			
Legend @ : Acceptable X : Unacceptable # : Not Evaluated ⌚ Delayed Result Entry			

**Problem Classification:** \_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

**Corrective Action:** \_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

**Reviewed by:** \_\_\_\_\_

**Dated:** \_\_\_\_\_

Instrument : Manual

Analyte	Standard Unit	Result Value	Accepted Value
@ pH	-	6	5,5,5,6
@ Specific Gravity	-	1.030	1.020,1.025,1.030
@ Glucose (urine)	-	3+	+2,+3,+4
@ Protein (Urine)	-	2+	+1,+2,+3
@ Ketone (urine)	-	Negative	Neg
@ Blood (urine)	-	2+	+1,+2,+3
@ Bilirubin (urine)	-	Negative	Neg
@ Urobilinogen (urine)	-	Normal	Nor
@ Nitrite (urine)	-	Present	Pre

Legend @ : Acceptable	Total Parameters	9
@ : Acceptable	Not Evaluated Parameters	0
X : Unacceptable	Evaluated Parameters	9
# : Not Evaluated	Outlier Parameters (X)	0
⌚ : Delayed Result Entry	EQAS Score Clinical Path - Urine Routine Chemistry	100.00 %



**Dr Puneet Kumar Nigam**  
PT coordinator & Technical Manager, MHL EQAS  
Unit No. 409-416.  
Commercial Building - 1A  
Kohinoor Mall, Kirol Road, Kurla (W),  
Mumbai - 400070

Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 13/02/2024

Cycle No : 230412

Sample No : 01

Sample Date : 23/12/2023

Clinical Path - Urine Routine Chemistry, Bilirubin (urine), -

All Methods

N

343

Diazonium salt - (Your Method)

249


Manual - (Your Analyzer)

158

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	Negative
<b>Result Expected</b>	Neg

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

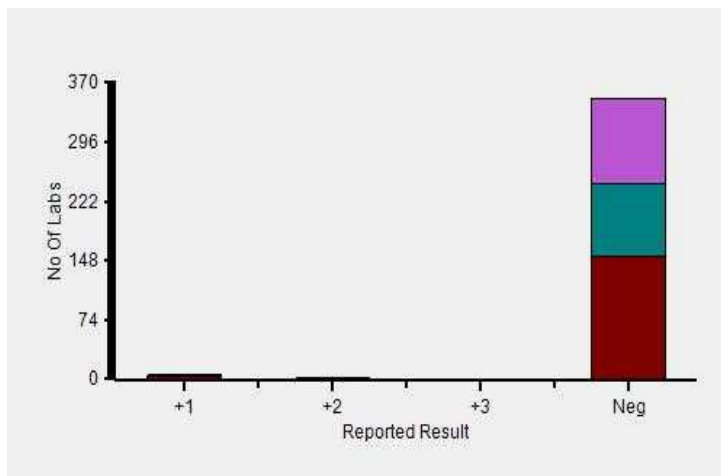

Lab : 1054

Cycle No : 230412


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 13/02/2024

Sample Date : 23/12/2023

Frequency Histogram Your Method

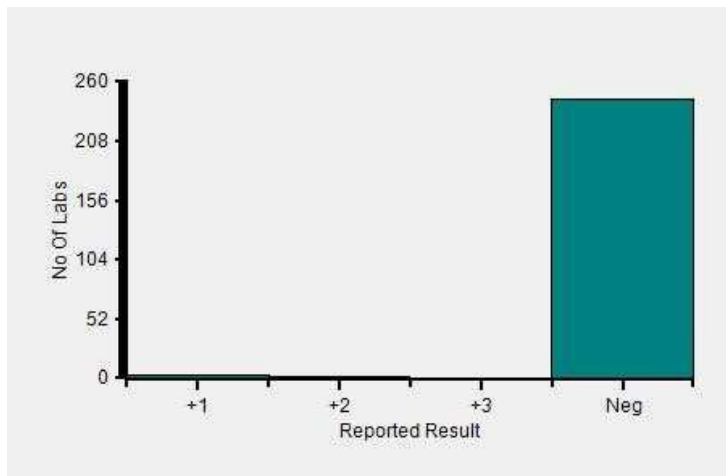

Frequency Histogram Your Analyzer

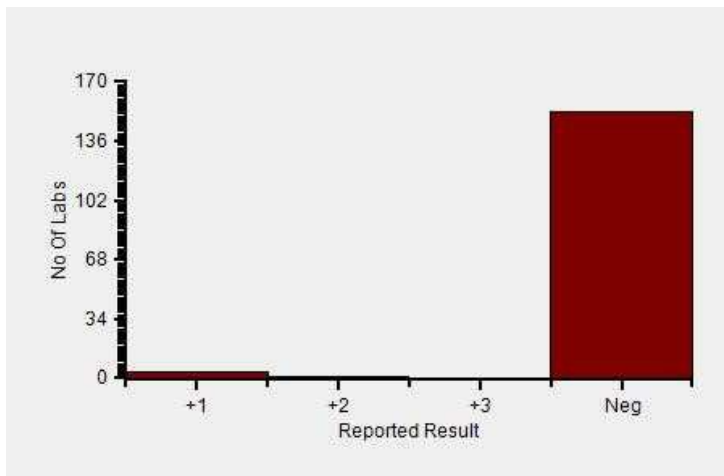

**Reported Results Legends :-**

<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>Neg</b>	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 13/02/2024

Cycle No : 230412

Sample No : 01

Sample Date : 23/12/2023

Clinical Path - Urine Routine Chemistry, Blood (urine), -


	<b>N</b>
<span style="color: purple;">■</span> All Methods	347
<span style="color: green;">■</span> Tetramethyl benzidine Reflectometric Analysis - (Your Method)	91
<span style="color: red;">■</span> Manual - (Your Analyzer)	159

**Evaluation Based On - Method wise Peer Grouping**

<b>Your Result</b>	2+
<b>Result Expected</b>	+1,+2,+3

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

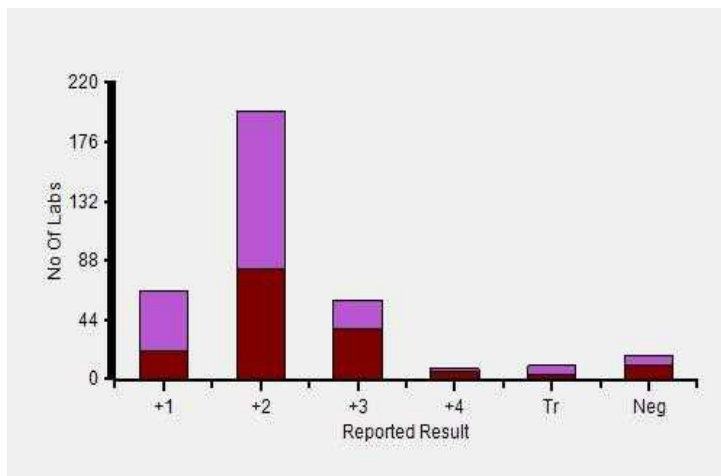

Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA


Report Date : 13/02/2024

Cycle No : 230412


Sample No : 01

Sample Date : 23/12/2023

Frequency Histogram Your Method

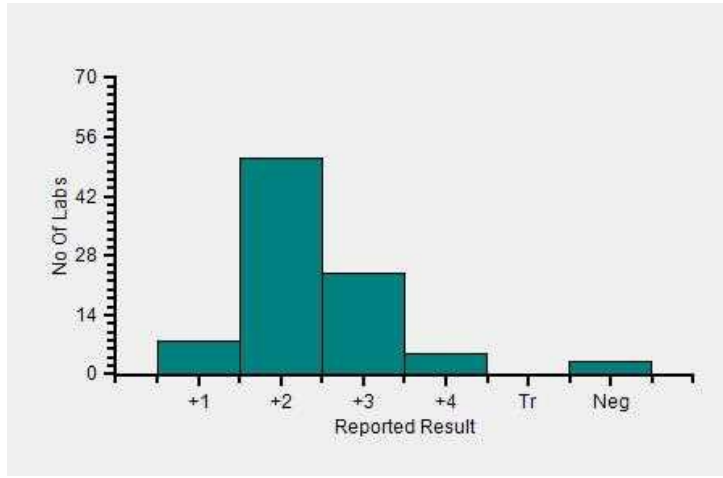

Frequency Histogram Your Analyzer

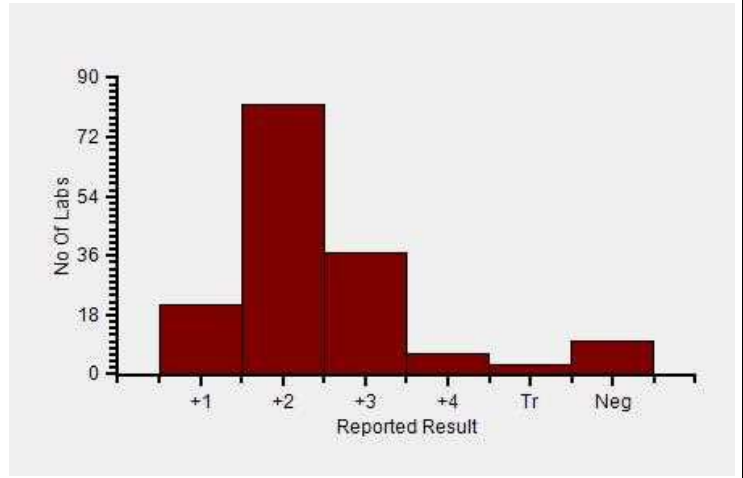

**Reported Results Legends :-**

<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>+4</b>	: 4+
<b>Tr</b>	: Trace
<b>Neg</b>	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 13/02/2024

Cycle No : 230412

Sample No : 01

Sample Date : 23/12/2023


Clinical Path - Urine Routine Chemistry, Glucose (urine), -

	<b>N</b>
<span style="color: purple;">■</span> All Methods	358
<span style="color: green;">■</span> Glucose oxidase peroxidase - (Your Method)	249
<span style="color: red;">■</span> Manual - (Your Analyzer)	169

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	3+
<b>Result Expected</b>	+2,+3,+4

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

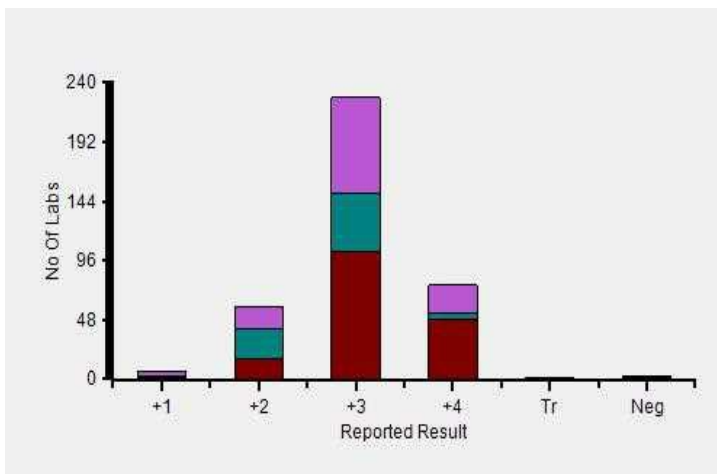

Lab : 1054

Cycle No : 230412


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 13/02/2024

Sample Date : 23/12/2023

Frequency Histogram Your Method

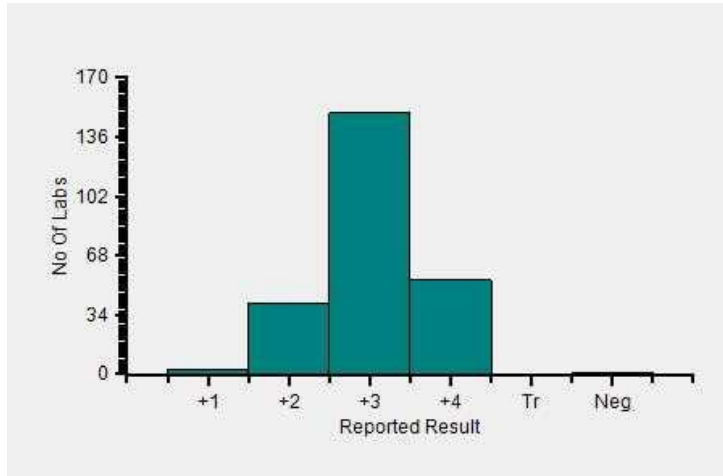

Frequency Histogram Your Analyzer

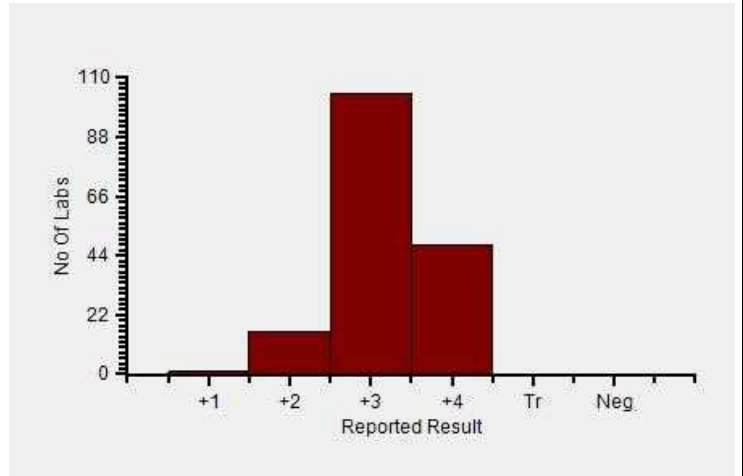

**Reported Results Legends :-**

<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>+4</b>	: 4+
<b>Tr</b>	: Trace
<b>Neg</b>	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- |                       |   |
|-----------------------|---|
| • Two out of two pass | - Acceptable performance                                |
| • One out of two pass | - Review for random error & take action if appropriate  |
| • Both failed         | - Unacceptable performance, Review for systematic error |

b) Reported on 3 samples:

- |                         |   |
|-------------------------|---|
| • All pass              | - Acceptable performance                                |
| • Two out of three pass | - Review for random error & take action if appropriate  |
| • One out of three pass | - Unacceptable performance, Review for systematic error |
| • All failed            | - Unacceptable performance, Review for systematic error |





Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 13/02/2024

Cycle No : 230412

Sample No : 01

Sample Date : 23/12/2023

Clinical Path - Urine Routine Chemistry, Ketone (urine), -

	<b>N</b>
■ All Methods	355
■ Sodium nitropruside Reflectometric Analysis - (Your Method)	201
■ Manual - (Your Analyzer)	166


**Evaluation Based On - Method wise Peer Grouping**

**Your Result** Negative

**Result Expected** Neg

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

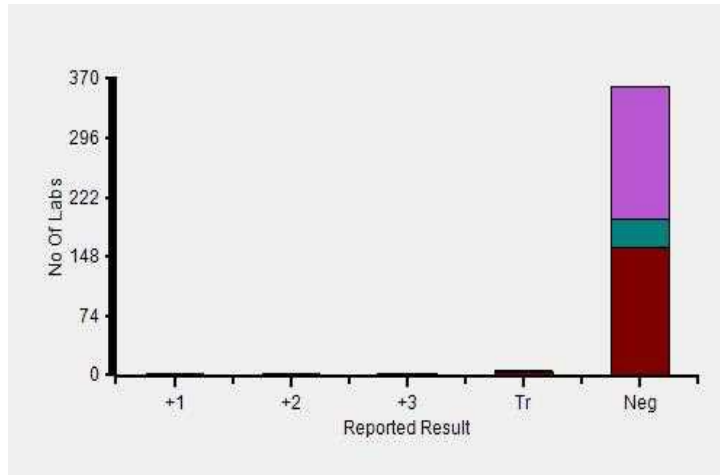

Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA


Report Date : 13/02/2024

Cycle No : 230412


Sample No : 01

Sample Date : 23/12/2023

Frequency Histogram Your Method

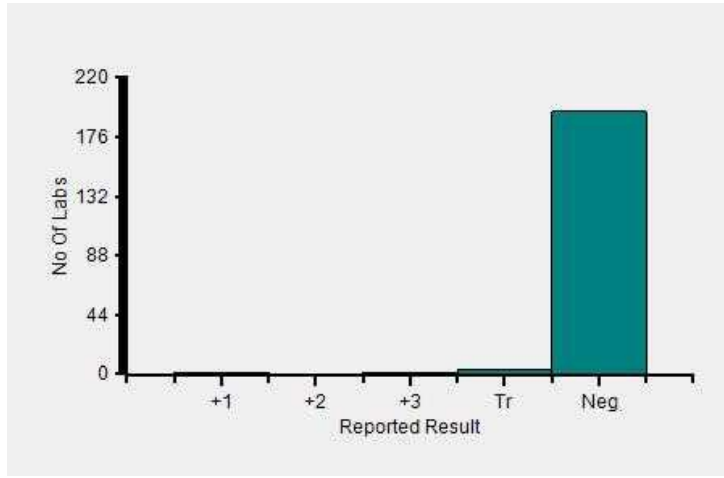

Frequency Histogram Your Analyzer

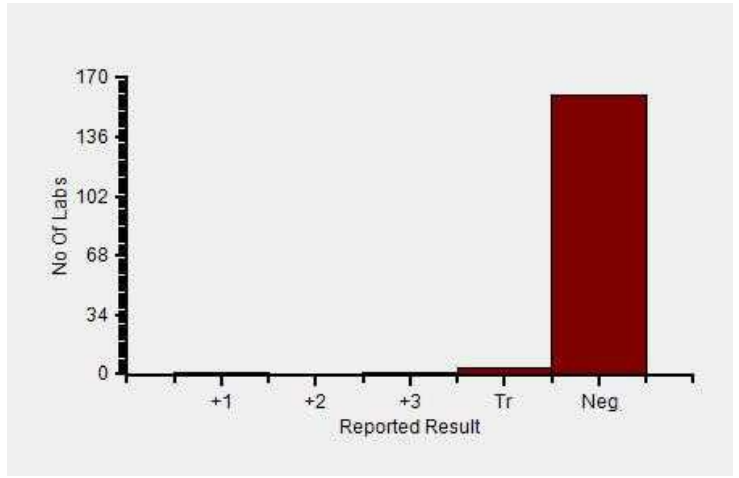

**Reported Results Legends :-**

<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>Tr</b>	: Trace
<b>Neg</b>	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 13/02/2024

Cycle No : 230412

Sample No : 01

Sample Date : 23/12/2023

Clinical Path - Urine Routine Chemistry, Nitrite (urine), -

All Methods

N

347

Tetrahydrobenzoquinoline - (Your Method)

180


Manual - (Your Analyzer)

159

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	Present
<b>Result Expected</b>	Pre

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

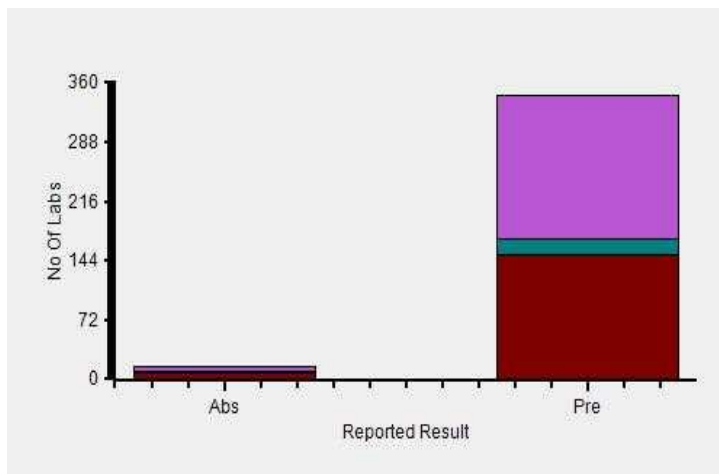

Lab : 1054

Cycle No : 230412


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 13/02/2024

Sample Date : 23/12/2023

Frequency Histogram Your Method

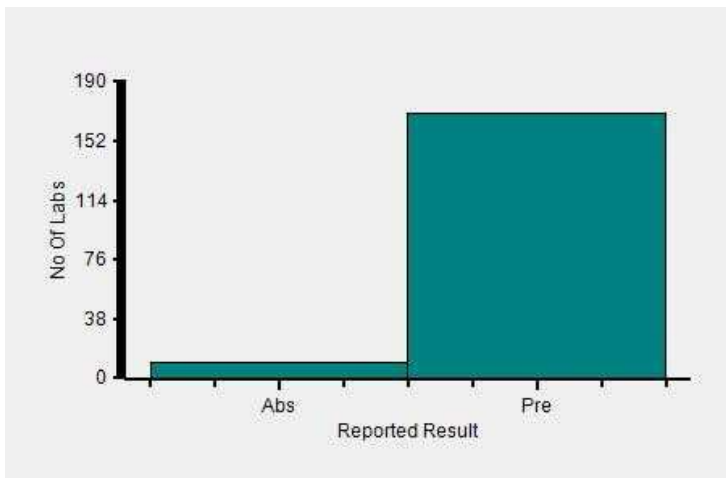

Frequency Histogram Your Analyzer

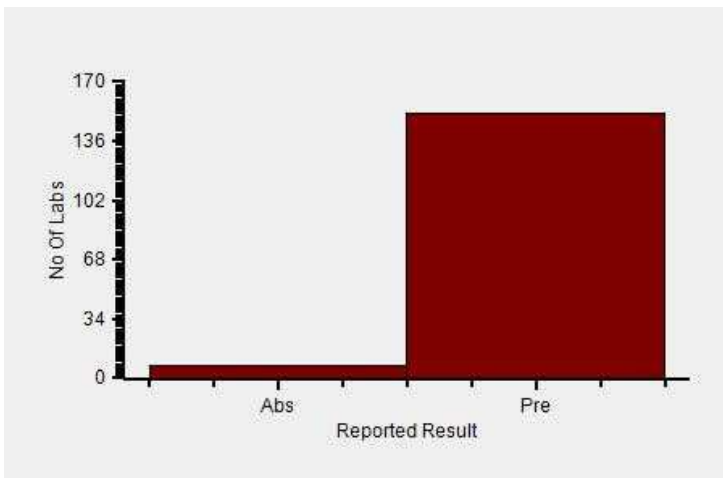

**Reported Results Legends :-**

**Abs** : Absent  
**Pre** : Present

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 13/02/2024

Cycle No : 230412

Sample No : 01

Sample Date : 23/12/2023

Clinical Path - Urine Routine Chemistry, pH, -

All Methods

N

356

Indicator Principle - (Your Method)

286


Manual - (Your Analyzer)

167

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	6
<b>Result Expected</b>	5,5.5,6

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

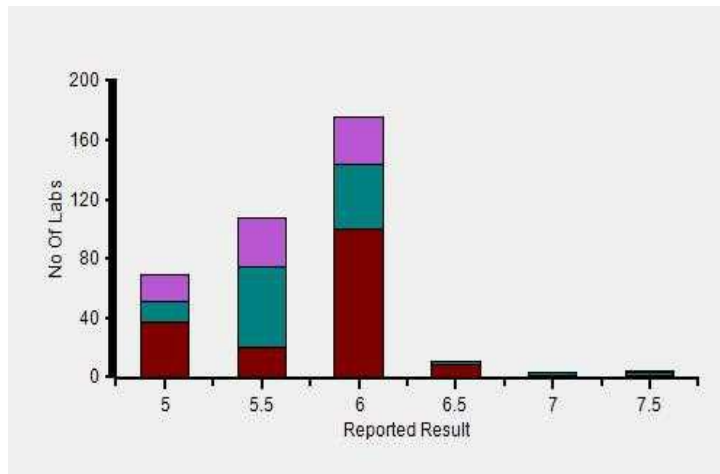

Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA


Report Date : 13/02/2024

Cycle No : 230412


Sample No : 01

Sample Date : 23/12/2023

Frequency Histogram Your Method

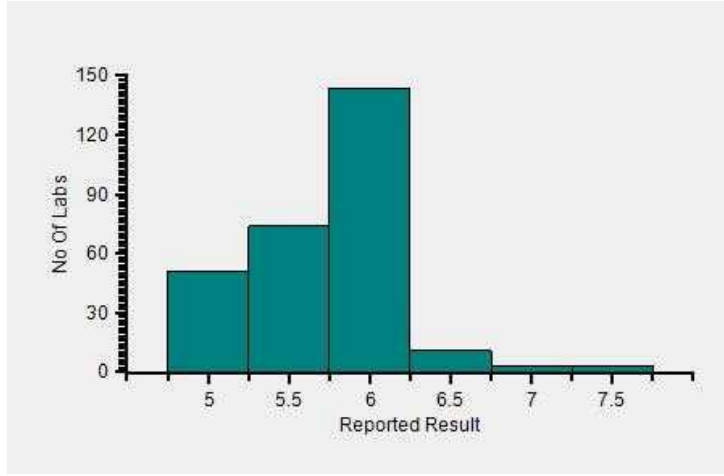

Frequency Histogram Your Analyzer

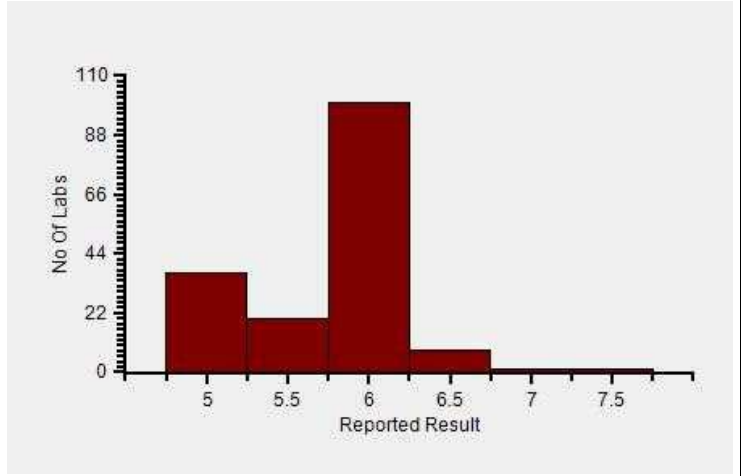

**Reported Results Legends :-**

5	: 5
5.5	: 5.5
6	: 6
6.5	: 6.5
7	: 7
7.5	: 7.5
8	: 8
8.5	: 8.5
9	: 9

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 13/02/2024

Cycle No : 230412

Sample No : 01

Sample Date : 23/12/2023

Clinical Path - Urine Routine Chemistry, Protein (Urine), -

■ All Methods

■ Tetra-bromophenol blue Reflectometric Analysis - (Your Method)

■ Manual - (Your Analyzer)

N

357


104

168

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	2+
<b>Result Expected</b>	+1,+2,+3

Note : # is an indication that this parameter has not been evaluated

Frequency Histogram

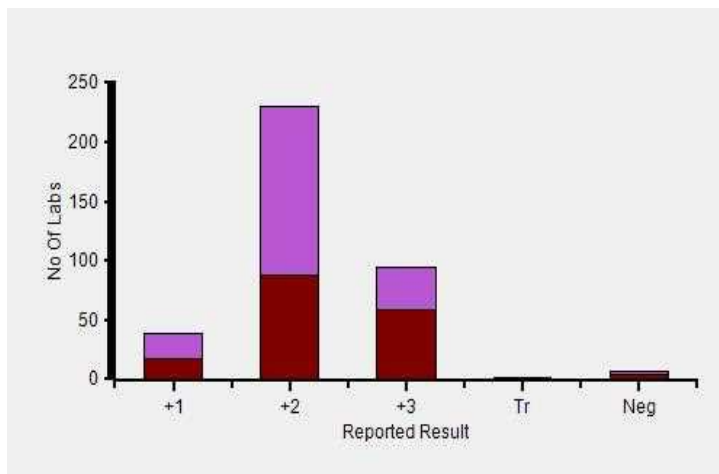

Lab : 1054

Cycle No : 230412


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 13/02/2024

Sample Date : 23/12/2023

Frequency Histogram Your Method

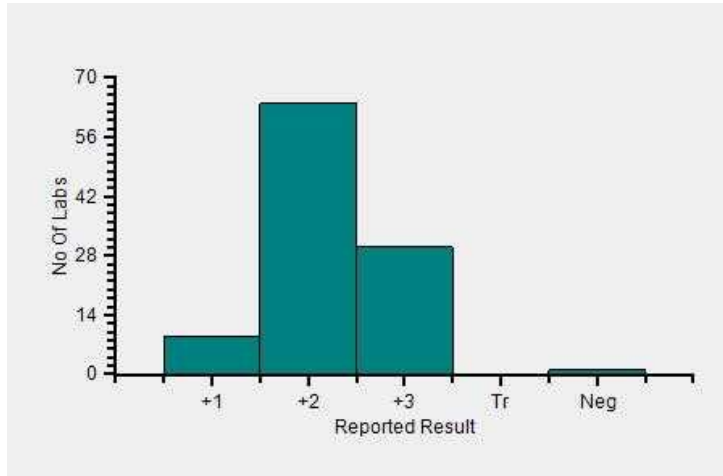

Frequency Histogram Your Analyzer

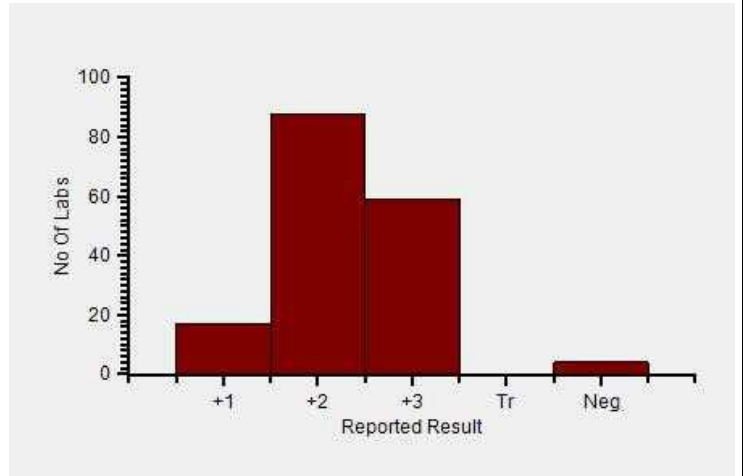

**Reported Results Legends :-**

<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>Tr</b>	: Trace
<b>Neg</b>	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error





Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 13/02/2024

Cycle No : 230412

Sample No : 01

Sample Date : 23/12/2023

Clinical Path - Urine Routine Chemistry, Specific Gravity, -


- All Methods
- pH Indicator dye - (Your Method)
- Manual - (Your Analyzer)

**N**  
 355  
 82  
 166

<b>Evaluation Based On - Method wise Peer Grouping</b>	
Your Result	1.030
Result Expected	1.020,1.025,1.030

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

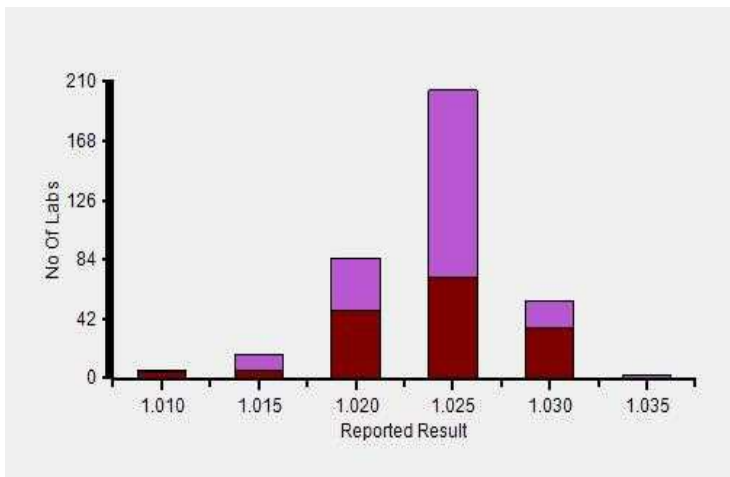

Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA


Report Date : 13/02/2024

Cycle No : 230412


Sample No : 01

Sample Date : 23/12/2023

Frequency Histogram Your Method

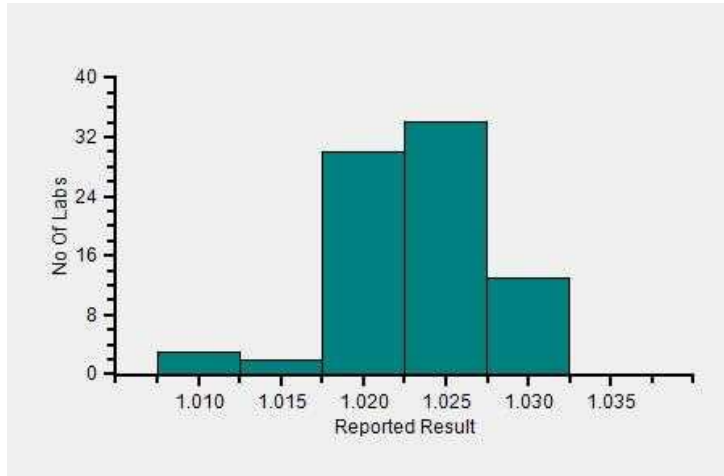

Frequency Histogram Your Analyzer

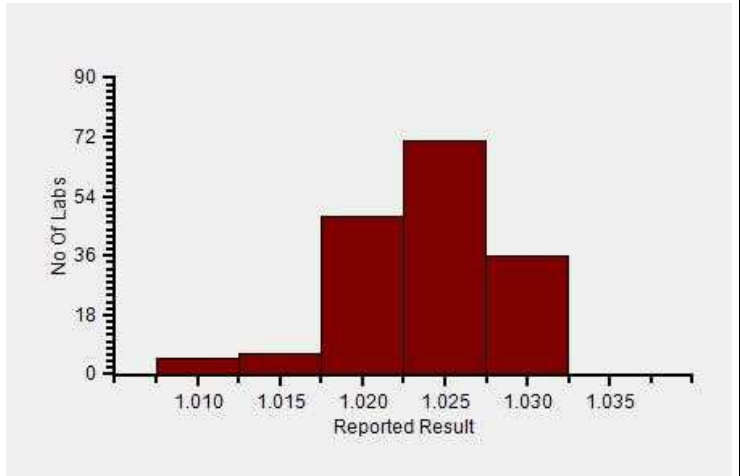

**Reported Results Legends :-**

<b>1.005</b>	: 1.005
<b>1.010</b>	: 1.010
<b>1.015</b>	: 1.015
<b>1.020</b>	: 1.020
<b>1.025</b>	: 1.025
<b>1.030</b>	: 1.030
<b>1.035</b>	: 1.035

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 13/02/2024

Cycle No : 230412

Sample No : 01

Sample Date : 23/12/2023


Clinical Path - Urine Routine Chemistry, Urobilinogen (urine), -

	<b>N</b>
■ All Methods	332
■ Diazonium salt - (Your Method)	139
■ Manual - (Your Analyzer)	151

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	Normal
<b>Result Expected</b>	Nor

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

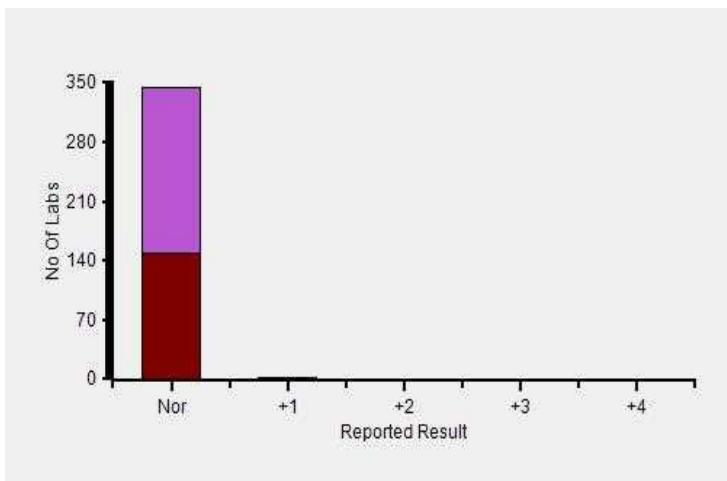

Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA


Report Date : 13/02/2024

Cycle No : 230412


Sample No : 01

Sample Date : 23/12/2023

Frequency Histogram Your Method

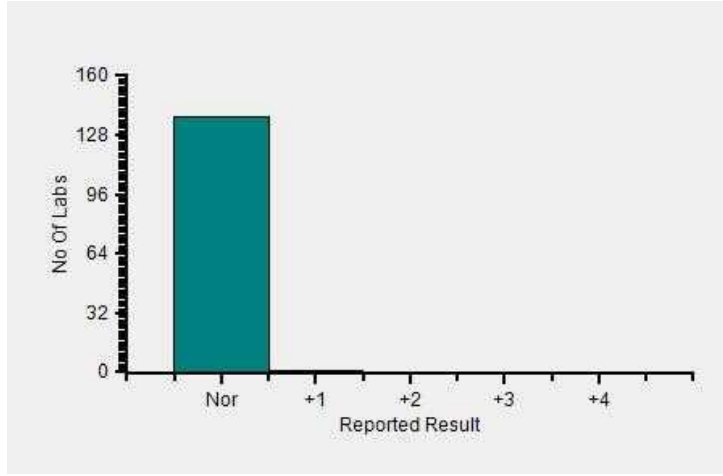

Frequency Histogram Your Analyzer

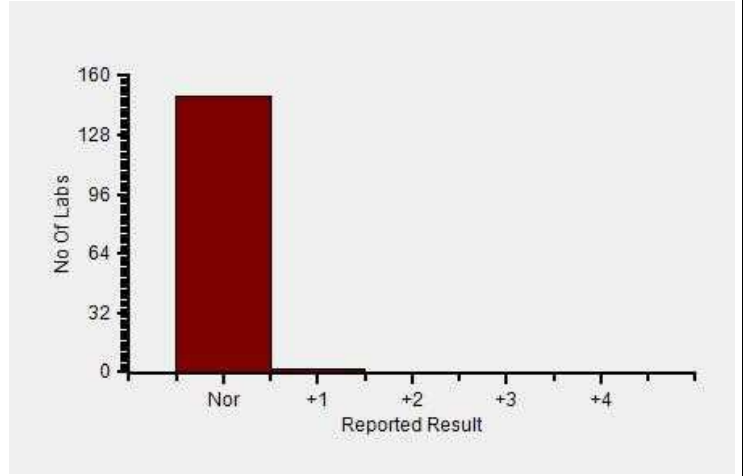

**Reported Results Legends :-**

<b>Nor</b>	: Normal
<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>+4</b>	: 4+

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**

Unit No. 409-416.  
Commercial Building - 1A  
Kohinoor Mall, Kirool Road, Kurla (W),  
Mumbai - 400070

This is a computer generated report hence signature is not required



PC-1022

End of Report

Page 18 of 18



# Metropolis Healthcare Ltd., EQAS

KRSNAA DIAGNOSTICS,LTD,MOGA (1054)

## Outlier And Analyte Summary Report

Outlier Details For Cycle No 230310 and Sample No 01

Report Date : 19/12/2023

Analyte	Instrument	Result Value	Standard Unit
X Ketone (urine)	Manual	1+	-
X Nitrite (urine)	Manual	Absent	-
Legend @ : Acceptable X : Unacceptable # : Not Evaluated ⌚ Delayed Result Entry			

Problem Classification: \_\_\_\_\_

\_\_\_\_\_  
\_\_\_\_\_

Corrective Action: \_\_\_\_\_

\_\_\_\_\_  
\_\_\_\_\_

Reviewed by: \_\_\_\_\_


Dated: \_\_\_\_\_

Instrument : Manual

Analyte	Standard Unit	Result Value	Accepted Value
@ pH	-	6	6,6.5,7
@ Specific Gravity	-	1.020	1.015,1.020,1.025
@ Glucose (urine)	-	4+	+2,+3,+4
@ Protein (Urine)	-	3+	+1,+2,+3
X Ketone (urine)	-	1+	Neg
@ Blood (urine)	-	2+	+1,+2,+3
@ Bilirubin (urine)	-	Negative	Neg
@ Urobilinogen (urine)	-	Normal	Nor
X Nitrite (urine)	-	Absent	Pre

Legend @ : Acceptable	Total Parameters	9
@ : Acceptable	Not Evaluated Parameters	0
X : Unacceptable	Evaluated Parameters	9
# : Not Evaluated	Outlier Parameters (X)	2
⌚ : Delayed Result Entry	EQAS Score Clinical Path - Urine Routine Chemistry	77.78 %



**Dr Puneet Kumar Nigam**  
PT coordinator & Technical Manager, MHL EQAS  
Unit No. 409-416.  
Commercial Building - 1A  
Kohinoor Mall, Kirol Road, Kurla (W),  
Mumbai - 400070



# Metropolis Healthcare Ltd., EQAS

KRSNAA DIAGNOSTICS,LTD,MOGA (1054)

## Outlier And Analyte Summary Report

Outlier Details For Cycle No 230310 and Sample No 01

Report Date : 19/12/2023

Analyte	Instrument	Result Value	Standard Unit
No Outlier			
Legend @ : Acceptable X : Unacceptable # : Not Evaluated ⌚ Delayed Result Entry			

**Problem Classification:** \_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_


**Corrective Action:** \_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

**Reviewed by:** \_\_\_\_\_

**Dated:** \_\_\_\_\_

Instrument : -

Analyte	Standard Unit	Result Value	Accepted Value
@ Crystal	-	Uric acid crystal	Uric acid crystal
Legend @ : Acceptable		Total Parameters	1
@ : Acceptable		Not Evaluated Parameters	0
X : Unacceptable		Evaluated Parameters	1
# : Not Evaluated		Outlier Parameters (X)	0
⊙ : Delayed Result Entry		EQAS Score Clinical Path - Urine Sediment Analysis Image	100.00 %



**Dr Puneet Kumar Nigam**  
PT coordinator & Technical Manager, MHL EQAS  
Unit No. 409-416.  
Commercial Building - 1A  
Kohinoor Mall, Kiroil Road, Kurla (W),  
Mumbai - 400070



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023


Clinical Path - Urine Routine Chemistry, Bilirubin (urine), -

	<b>N</b>
■ All Methods	351
■ Diazonium salt - (Your Method)	248
■ Manual - (Your Analyzer)	153

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	Negative
<b>Result Expected</b>	Neg

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

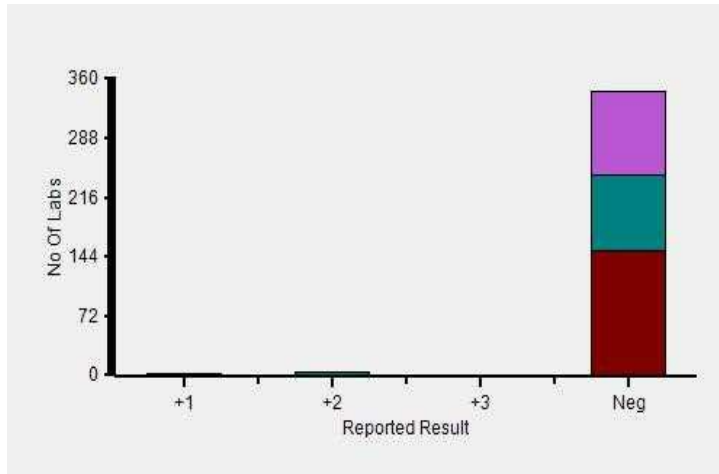

Lab : 1054

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

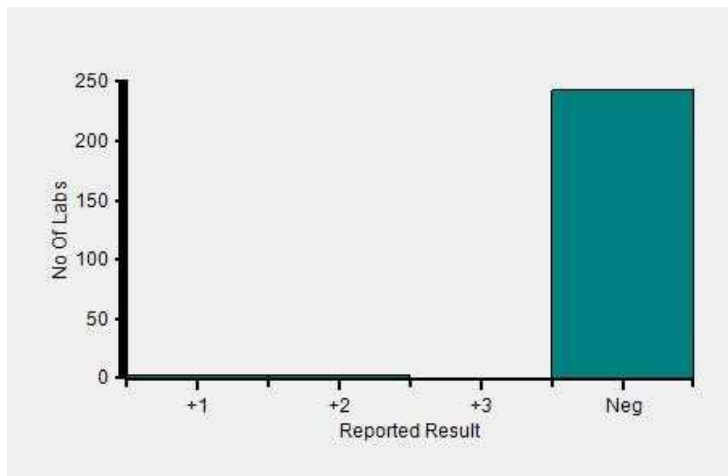

Frequency Histogram Your Analyzer

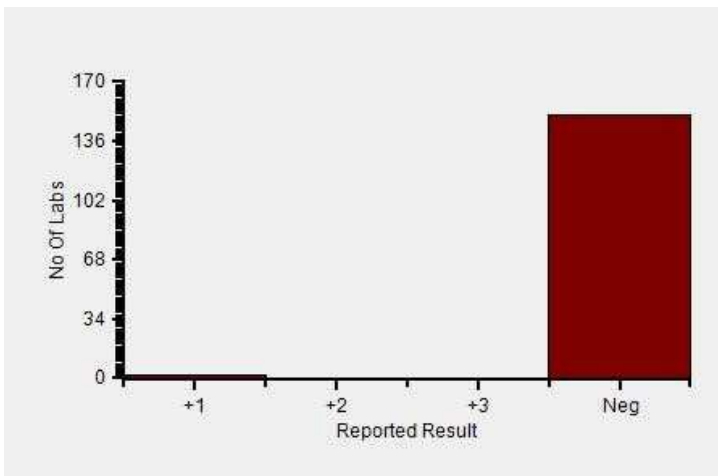

**Reported Results Legends :-**

<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>Neg</b>	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- |                       |   |
|-----------------------|---|
| • Two out of two pass | - Acceptable performance                                |
| • One out of two pass | - Review for random error & take action if appropriate  |
| • Both failed         | - Unacceptable performance, Review for systematic error |

b) Reported on 3 samples:

- |                         |   |
|-------------------------|---|
| • All pass              | - Acceptable performance                                |
| • Two out of three pass | - Review for random error & take action if appropriate  |
| • One out of three pass | - Unacceptable performance, Review for systematic error |
| • All failed            | - Unacceptable performance, Review for systematic error |



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023

Clinical Path - Urine Routine Chemistry, Blood (urine), -

	<b>N</b>
■ All Methods	356
■ Tetramethyl benzidine Reflectometric Analysis - (Your Method)	98
■ Manual - (Your Analyzer)	156


**Evaluation Based On - Method wise Peer Grouping**

**Your Result** 2+

**Result Expected** +1,+2,+3

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

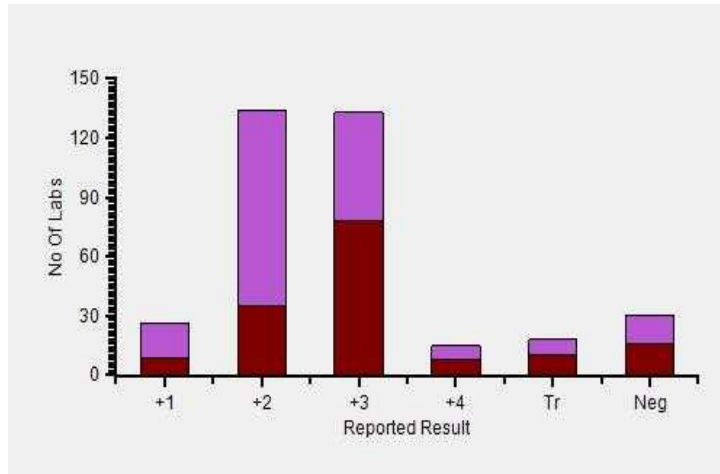

Lab : 1054

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

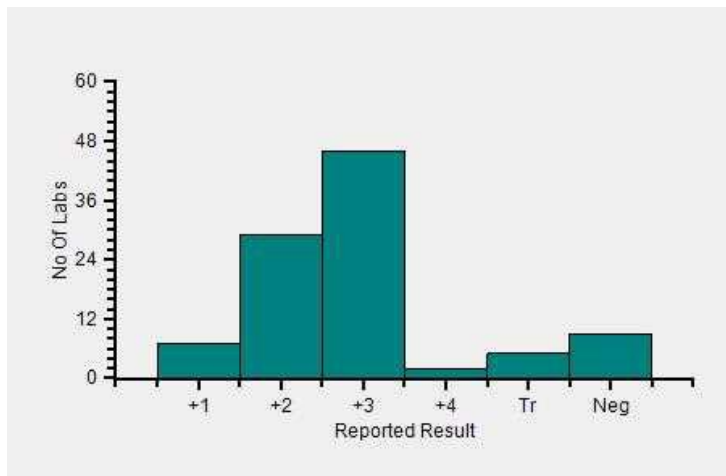

Frequency Histogram Your Analyzer

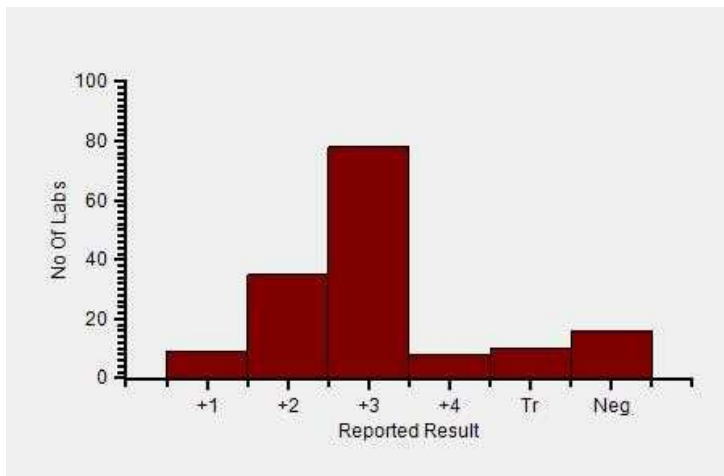

**Reported Results Legends :-**

<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>+4</b>	: 4+
<b>Tr</b>	: Trace
<b>Neg</b>	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- |                       |   |
|-----------------------|---|
| • Two out of two pass | - Acceptable performance                                |
| • One out of two pass | - Review for random error & take action if appropriate  |
| • Both failed         | - Unacceptable performance, Review for systematic error |

b) Reported on 3 samples:

- |                         |   |
|-------------------------|---|
| • All pass              | - Acceptable performance                                |
| • Two out of three pass | - Review for random error & take action if appropriate  |
| • One out of three pass | - Unacceptable performance, Review for systematic error |
| • All failed            | - Unacceptable performance, Review for systematic error |



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023

Clinical Path - Urine Routine Chemistry, Glucose (urine), -

	<b>N</b>
■ All Methods	365
■ Glucose oxidase peroxidase - (Your Method)	244
■ Manual - (Your Analyzer)	164


**Evaluation Based On - Method wise Peer Grouping**

**Your Result** 4+

**Result Expected** +2,+3,+4

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

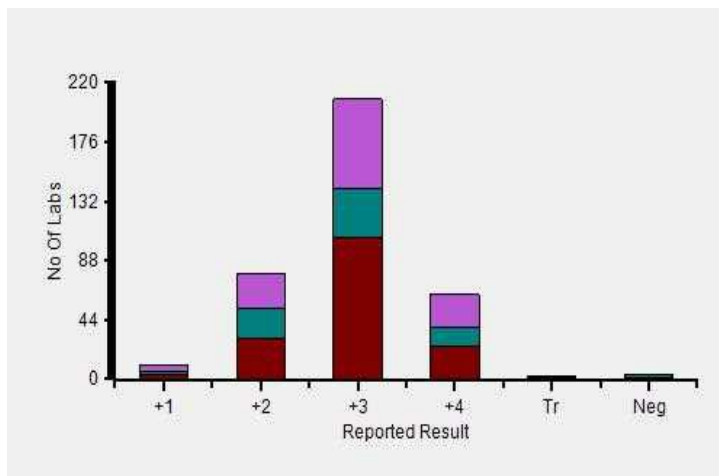

Lab : 1054

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

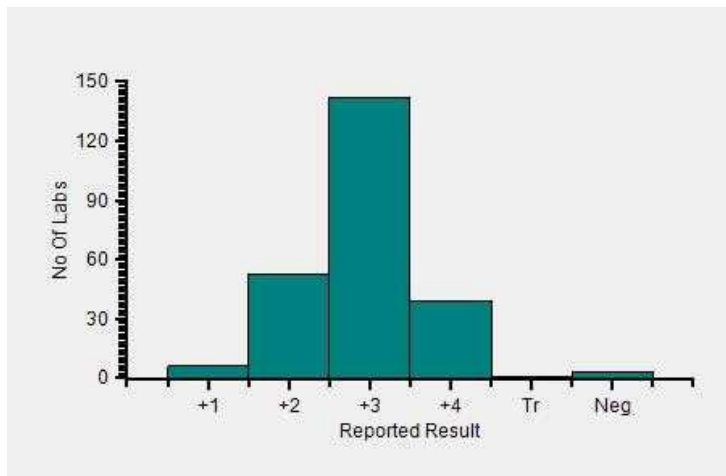

Frequency Histogram Your Analyzer

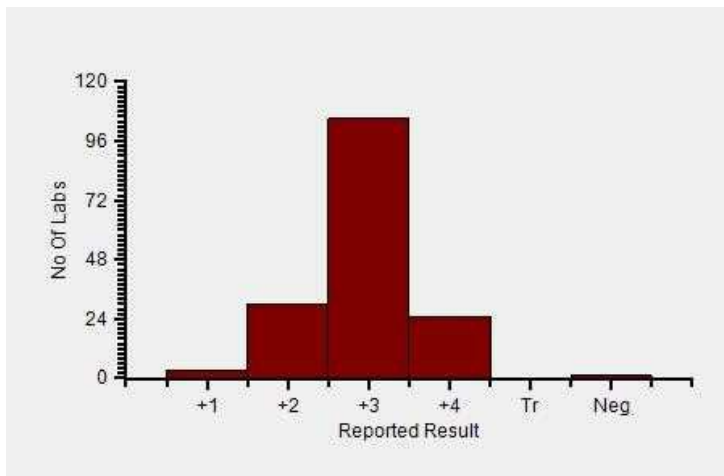

**Reported Results Legends :-**

<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>+4</b>	: 4+
<b>Tr</b>	: Trace
<b>Neg</b>	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023


Clinical Path - Urine Routine Chemistry, Ketone (urine), -

	<b>N</b>
■ All Methods	359
■ Sodium nitropruside Reflectometric Analysis - (Your Method)	202
■ Manual - (Your Analyzer)	160

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	1+
<b>Result Expected</b>	Neg

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

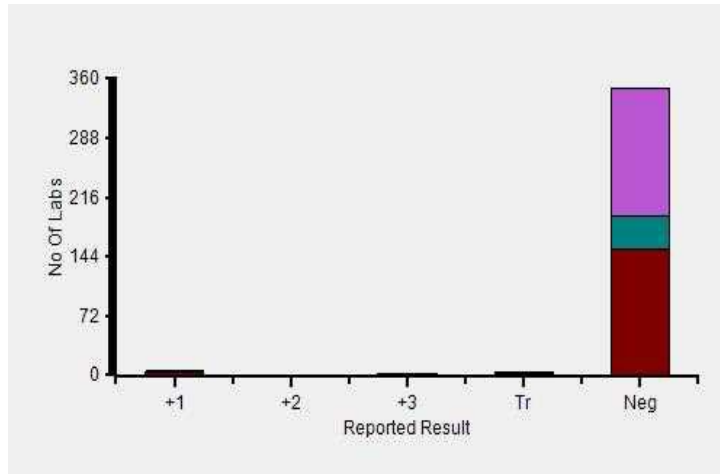

Lab : 1054

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

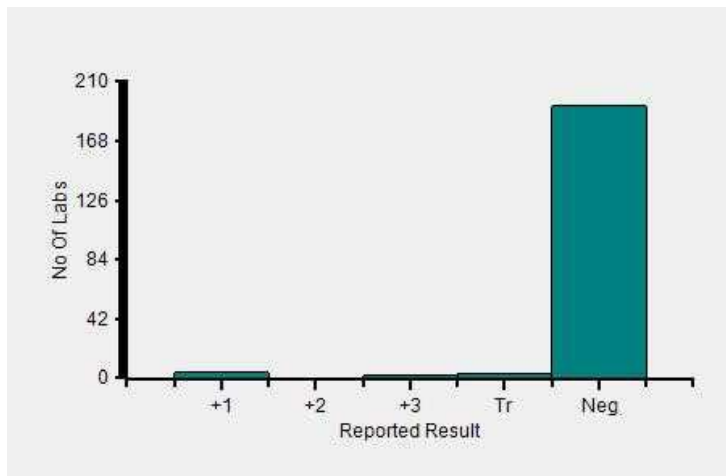

Frequency Histogram Your Analyzer

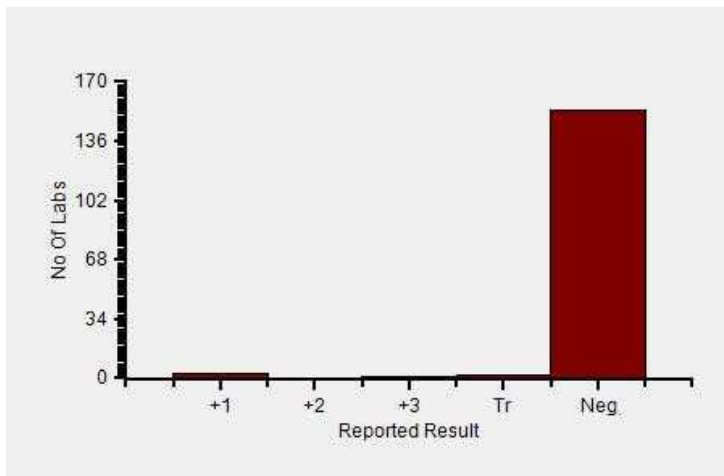

**Reported Results Legends :-**

<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>Tr</b>	: Trace
<b>Neg</b>	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error





Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023


Clinical Path - Urine Routine Chemistry, Nitrite (urine), -

	<b>N</b>
■ All Methods	347
■ Tetrahydrobenzoquinoline - (Your Method)	185
■ Manual - (Your Analyzer)	152

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	Absent
<b>Result Expected</b>	Pre

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

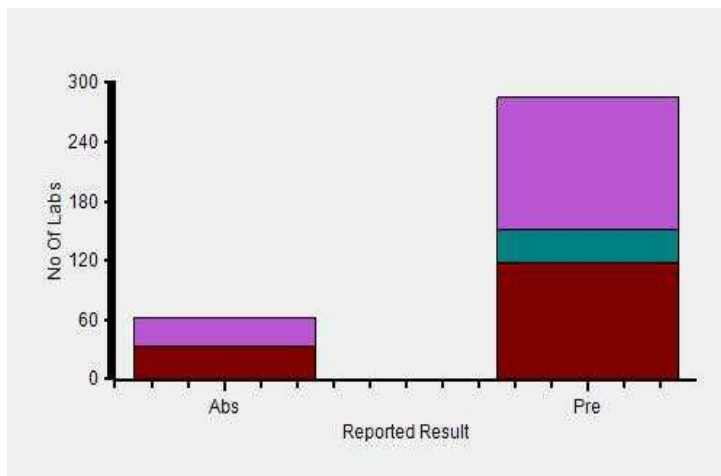

Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA


Report Date : 19/12/2023

Cycle No : 230310


Sample No : 01

Sample Date : 25/11/2023

Frequency Histogram Your Method

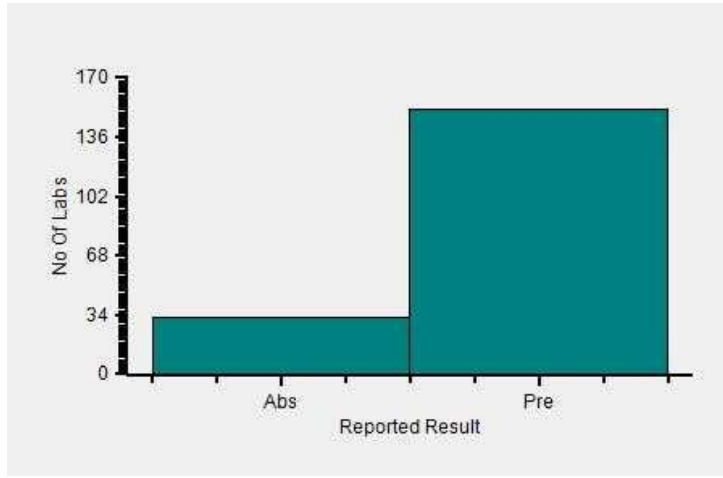

Frequency Histogram Your Analyzer

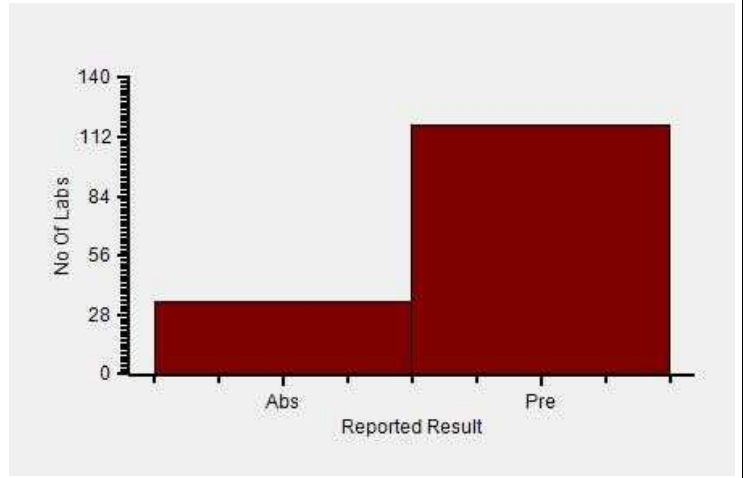

**Reported Results Legends :-**

**Abs** : Absent  
**Pre** : Present

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance
  - Two out of three pass - Review for random error & take action if appropriate
  - One out of three pass - Unacceptable performance, Review for systematic error
  - All failed - Unacceptable performance, Review for systematic error



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023


Clinical Path - Urine Routine Chemistry, pH, -

	<b>N</b>
■ All Methods	361
■ Indicator Principle - (Your Method)	278
■ Manual - (Your Analyzer)	160

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	6
<b>Result Expected</b>	6,6.5,7

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

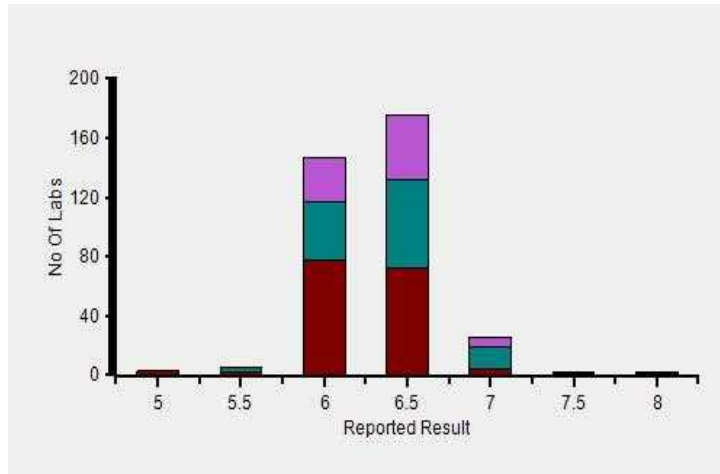

Lab : 1054

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

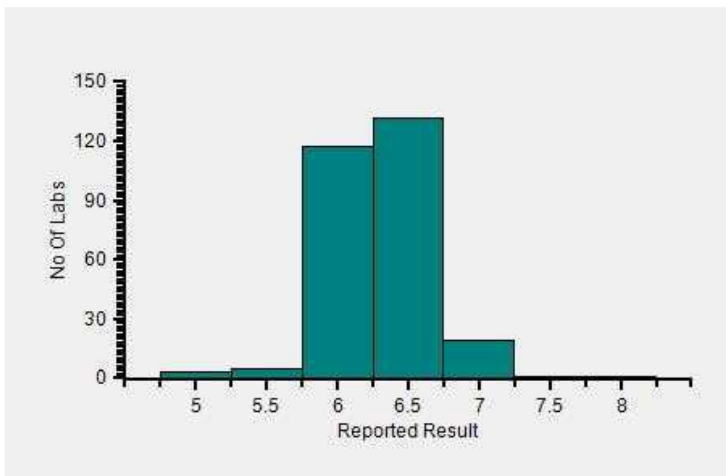

Frequency Histogram Your Analyzer

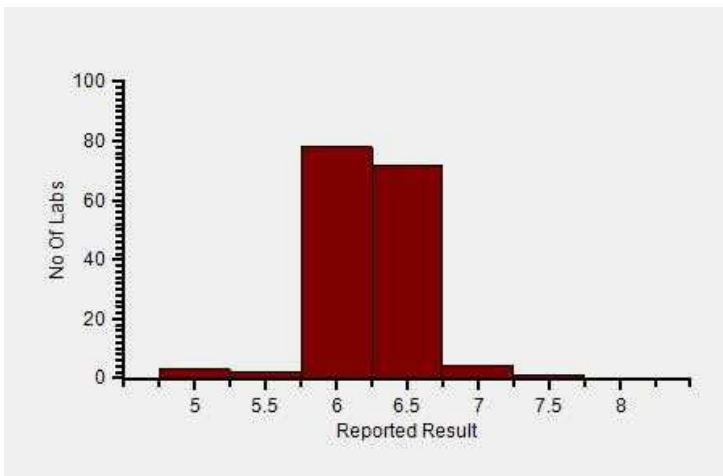

**Reported Results Legends :-**

5	: 5
5.5	: 5.5
6	: 6
6.5	: 6.5
7	: 7
7.5	: 7.5
8	: 8
8.5	: 8.5
9	: 9

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1054

Cycle No : 230310

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01

Report Date : 19/12/2023

Sample Date : 25/11/2023


Clinical Path - Urine Routine Chemistry, Protein (Urine), -

	<b>N</b>
■ All Methods	364
■ Tetra-bromophenol blue Reflectometric Analysis - (Your Method)	113
■ Manual - (Your Analyzer)	163

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	3+
<b>Result Expected</b>	+1,+2,+3

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

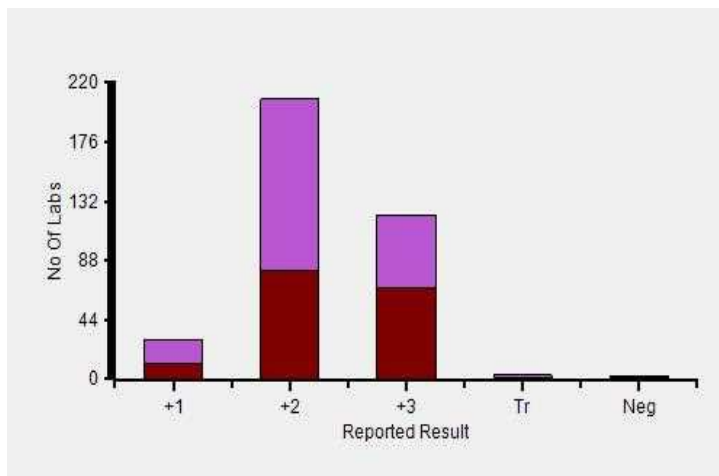

Lab : 1054

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

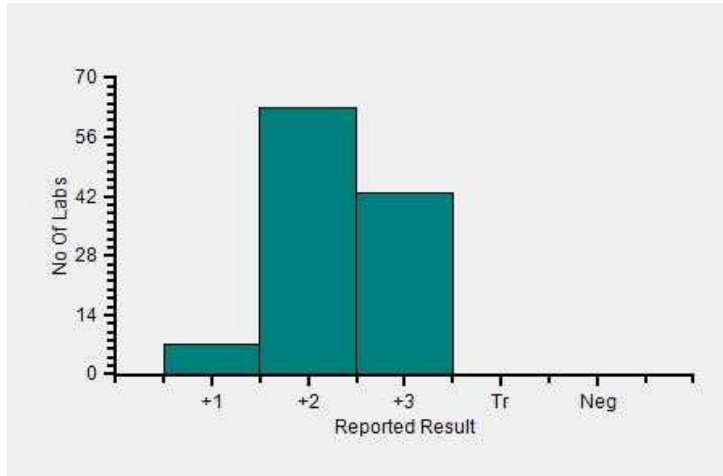

Frequency Histogram Your Analyzer

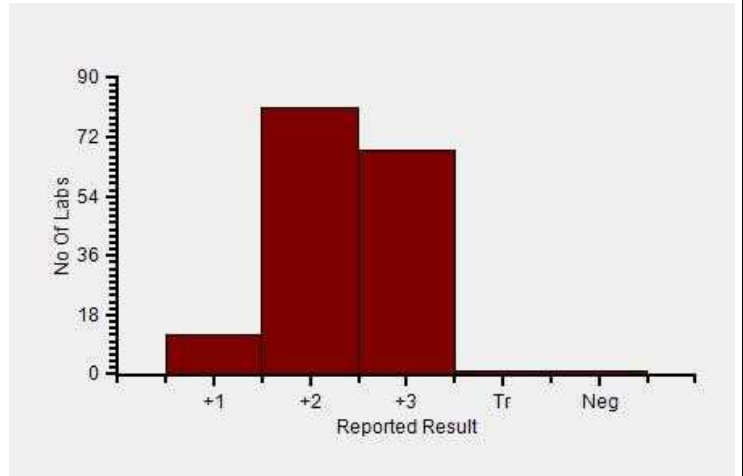

**Reported Results Legends :-**

<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>Tr</b>	: Trace
<b>Neg</b>	: Negative

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error



Lab : 1054

Cycle No : 230310

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01

Report Date : 19/12/2023

Sample Date : 25/11/2023


Clinical Path - Urine Routine Chemistry, Specific Gravity, -

	<b>N</b>
■ All Methods	357
■ pH Indicator dye - (Your Method)	78
■ Manual - (Your Analyzer)	158

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	1.020
<b>Result Expected</b>	1.015,1.020,1.025

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

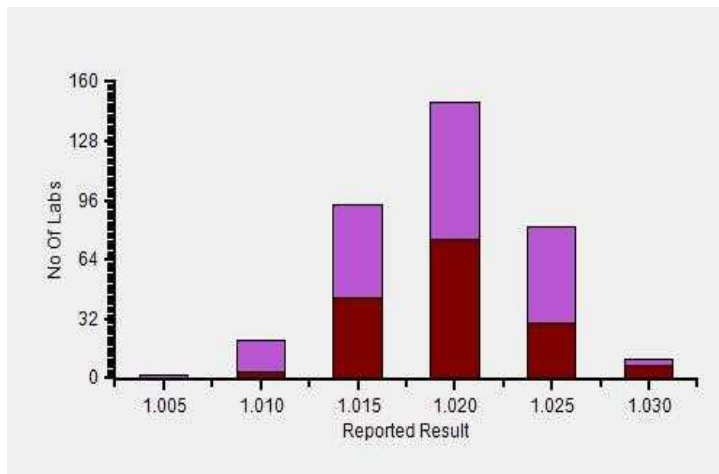

Lab : 1054

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

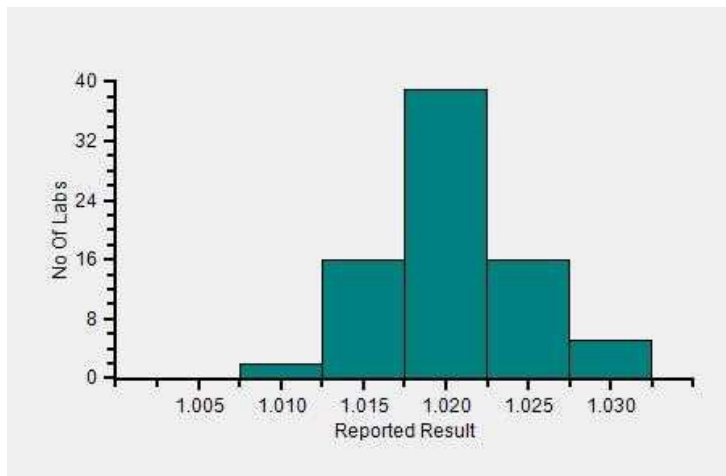

Frequency Histogram Your Analyzer

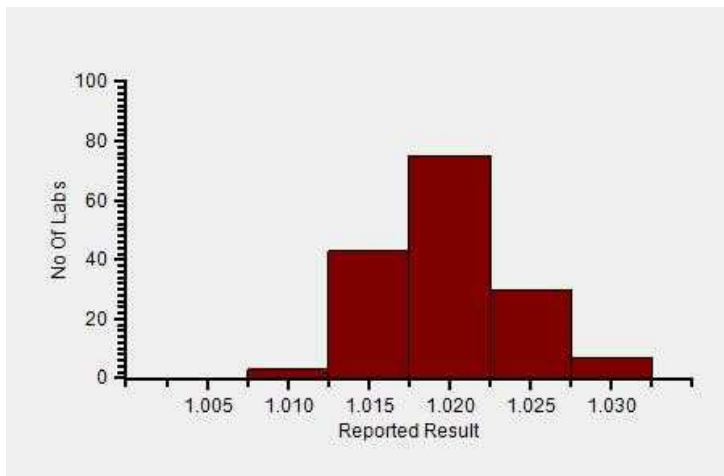

**Reported Results Legends :-**

<b>1.005</b>	: 1.005
<b>1.010</b>	: 1.010
<b>1.015</b>	: 1.015
<b>1.020</b>	: 1.020
<b>1.025</b>	: 1.025
<b>1.030</b>	: 1.030
<b>1.035</b>	: 1.035

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error





Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023


Clinical Path - Urine Routine Chemistry, Urobilinogen (urine), -

	<b>N</b>
■ All Methods	337
■ Diazonium salt - (Your Method)	139
■ Manual - (Your Analyzer)	147

<b>Evaluation Based On - Method wise Peer Grouping</b>	
<b>Your Result</b>	Normal
<b>Result Expected</b>	Nor

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

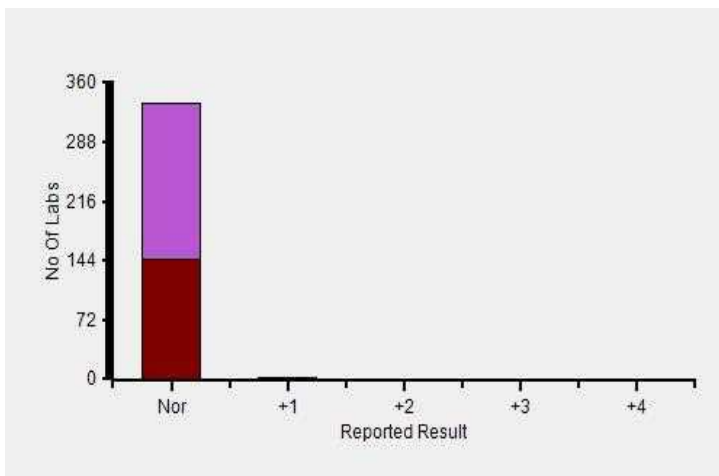

Lab : 1054

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

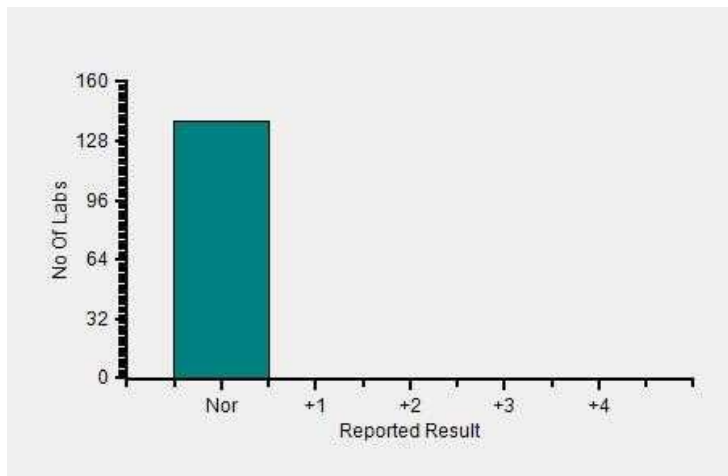

Frequency Histogram Your Analyzer

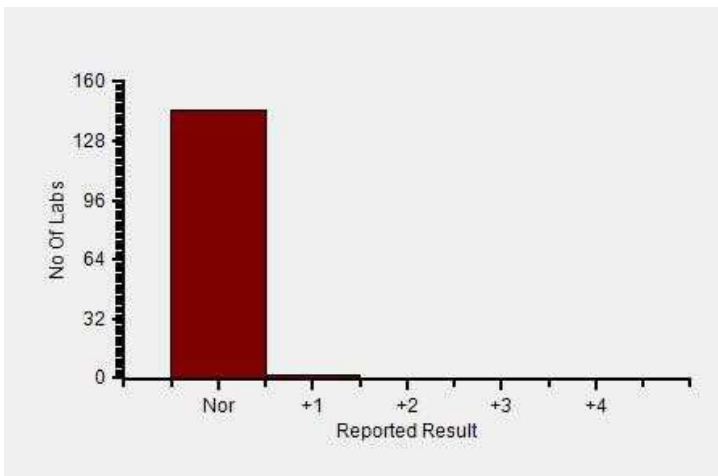

**Reported Results Legends :-**

<b>Nor</b>	: Normal
<b>+1</b>	: 1+
<b>+2</b>	: 2+
<b>+3</b>	: 3+
<b>+4</b>	: 4+

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

a) Reported on 2 samples:

- Two out of two pass - Acceptable performance
- One out of two pass - Review for random error & take action if appropriate
- Both failed - Unacceptable performance, Review for systematic error

b) Reported on 3 samples:

- All pass - Acceptable performance
- Two out of three pass - Review for random error & take action if appropriate
- One out of three pass - Unacceptable performance, Review for systematic error
- All failed - Unacceptable performance, Review for systematic error

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**

Unit No. 409-416.  
Commercial Building - 1A  
Kohinoor Mall, Kirool Road, Kurla (W),  
Mumbai - 400070

This is a computer generated report hence signature is not required



PC-1022

Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023


Clinical Path - Urine Sediment Analysis Image, Crystal, -

	<b>N</b>
■ All Methods	238
■ -- (Your Method)	238
■ -- (Your Analyzer)	238

<b>Your Result</b>	Uric acid crystal
<b>Result Expected</b>	UAC

**Note :** # is an indication that this parameter has not been evaluated

Frequency Histogram

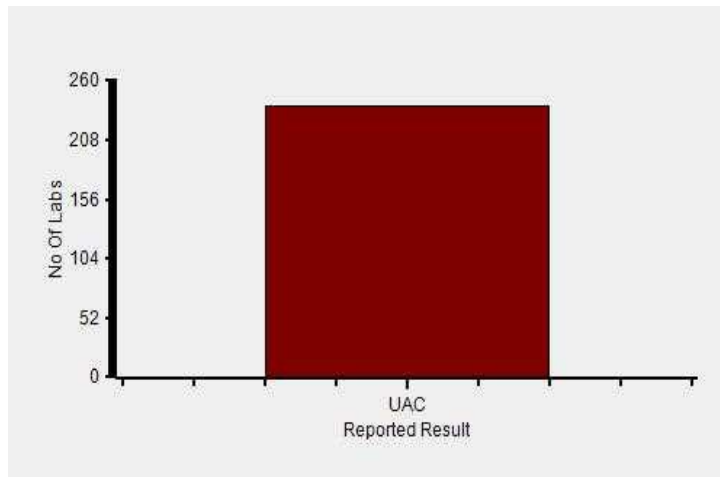

Lab : 1054

Cycle No : 230310


Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Sample No : 01


Report Date : 19/12/2023

Sample Date : 25/11/2023

Frequency Histogram Your Method

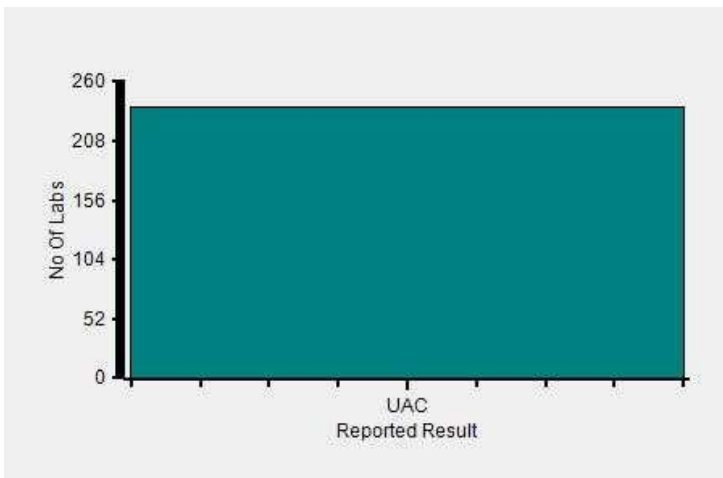

Frequency Histogram Your Analyzer

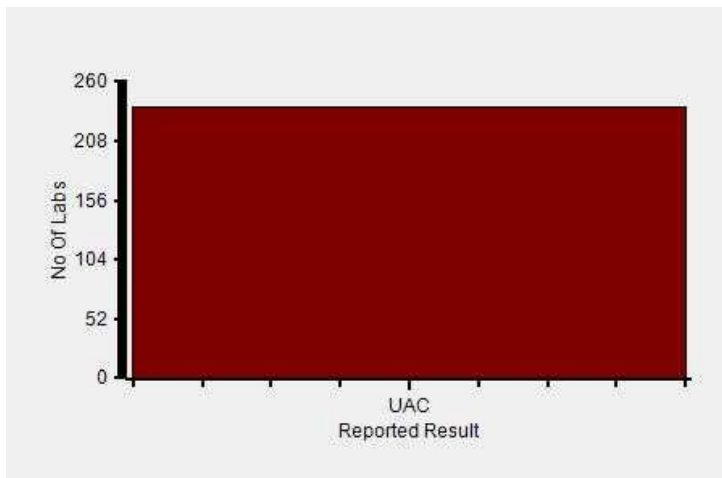

**Reported Results Legends :-**

<b>TPC</b>	: Triple phosphate crystal
<b>UAC</b>	: Uric acid crystal
<b>CC</b>	: Cystine crystal
<b>SC</b>	: Sulfonamide crystal
<b>UC</b>	: Urate crystal
<b>CaOx</b>	: Calcium oxalate crystal
<b>BC</b>	: Bilirubin crystals
<b>CHC</b>	: Cholesterol crystals
<b>ABC</b>	: Ammonium Biurate crystal
<b>NCS</b>	: No crystal seen
<b>APC</b>	: Ammonium phosphate crystal
<b>APC</b>	: Amorphous Phosphate Crystal
<b>CYSTCRYS</b>	: Cystine crystals
<b>STRUCRYS</b>	: Struvite crystals

**Comments :**

Interpretation when an analyte is reported for multiple samples in a Round:

- a) Reported on 2 samples:
  - Two out of two pass - Acceptable performance
  - One out of two pass - Review for random error & take action if appropriate
  - Both failed - Unacceptable performance, Review for systematic error
- b) Reported on 3 samples:
  - All pass - Acceptable performance



Lab : 1054

Lab Name : KRSNAA DIAGNOSTICS,LTD,MOGA

Report Date : 19/12/2023

Cycle No : 230310

Sample No : 01

Sample Date : 25/11/2023

- Two out of three pass
  - One out of three pass
  - All failed
- Review for random error & take action if appropriate
  - Unacceptable performance, Review for systematic error
  - Unacceptable performance, Review for systematic error

*Dr Puneet Kumar Nigam*

**Dr Puneet Kumar Nigam**  
**PT coordinator & Technical Manager, MHL EQAS**  
Unit No. 409-416.  
Commercial Building - 1A  
Kohinoor Mall, Kiro Road, Kurla (W),  
Mumbai - 400070

This is a computer generated report hence signature  
is not required



PC-1022